

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
 Data File : VU063618.D
 Acq On : 22 Sep 2025 14:44
 Operator : MD/SY
 Sample : VU0922MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M

Title : VOC Analysis

Signal : TIC: VU063618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	105	rBV	121730	132276	15.04%	1.973%
2	1.901	183	190	203	rVB	99476	128809	14.64%	1.921%
3	2.554	382	393	412	rBV	172309	283572	32.24%	4.230%
4	2.756	453	456	457	rBV2	627	332	0.04%	0.005%
5	2.924	505	508	511	rBV	191	118	0.01%	0.002%
6	2.956	516	518	519	rBV	261	106	0.01%	0.002%
7	3.033	534	542	553	rVB5	4183	7608	0.86%	0.113%
8	3.100	558	563	573	rBV3	363	546	0.06%	0.008%
9	3.165	575	583	585	rBV2	1630	1936	0.22%	0.029%
10	3.245	605	608	612	rBV	167	140	0.02%	0.002%
11	3.284	617	620	624	rVB	362	320	0.04%	0.005%
12	3.332	632	635	637	rBV2	540	365	0.04%	0.005%
13	3.457	668	674	676	rBV2	351	274	0.03%	0.004%
14	3.541	697	700	701	rBV	185	115	0.01%	0.002%
15	3.631	725	728	730	rBV2	127	93	0.01%	0.001%
16	3.653	733	735	738	rVV	242	143	0.02%	0.002%
17	3.669	738	740	743	rVB	335	196	0.02%	0.003%
18	3.686	743	745	747	rBV	234	133	0.02%	0.002%
19	3.756	764	767	770	rBV2	278	210	0.02%	0.003%
20	3.869	799	802	804	rVB	223	93	0.01%	0.001%
21	3.885	804	807	808	rBV	94	57	0.01%	0.001%
22	3.923	815	819	828	rVB2	363	446	0.05%	0.007%
23	3.962	828	831	832	rBV	108	62	0.01%	0.001%
24	4.026	848	851	852	rBV	89	45	0.01%	0.001%
25	4.059	858	861	863	rBV	181	85	0.01%	0.001%
26	4.139	884	886	889	rVB2	240	114	0.01%	0.002%
27	4.206	904	907	908	rBV	94	50	0.01%	0.001%
28	4.232	913	915	917	rBV	233	94	0.01%	0.001%
29	4.268	923	926	928	rBV	123	58	0.01%	0.001%
30	4.284	928	931	932	rBV	169	92	0.01%	0.001%
31	4.377	956	960	961	rBV	229	148	0.02%	0.002%
32	4.412	968	971	973	rBV	153	92	0.01%	0.001%
33	4.428	973	976	978	rBV	181	122	0.01%	0.002%
34	4.457	982	985	989	rBV	109	70	0.01%	0.001%
35	4.486	992	994	996	rBV	75	36	0.00%	0.001%
36	4.502	996	999	1001	rBV2	160	79	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
 Data File : VU063618.D
 Acq On : 22 Sep 2025 14:44
 Operator : MD/SY
 Sample : VU0922MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
 Title : VOC Analysis

37	4.518	1002	1004	1007	rVB	261	125	0.01%	0.002%
38	4.544	1007	1012	1015	rBV	345	292	0.03%	0.004%
39	4.573	1018	1021	1024	rBV	253	204	0.02%	0.003%
40	4.615	1026	1034	1067	rBV	66319	180138	20.48%	2.687%
41	5.049	1155	1169	1207	rVB	149638	346205	39.36%	5.164%
42	5.284	1239	1242	1243	rBV2	291	137	0.02%	0.002%
43	5.329	1254	1256	1258	rBV2	415	146	0.02%	0.002%
44	5.374	1266	1270	1272	rBV3	577	338	0.04%	0.005%
45	5.402	1276	1279	1281	rVB2	133	69	0.01%	0.001%
46	5.448	1289	1293	1295	rBV	368	256	0.03%	0.004%
47	5.515	1312	1314	1316	rBV	154	93	0.01%	0.001%
48	5.605	1339	1342	1346	rBV	184	159	0.02%	0.002%
49	5.711	1356	1375	1416	rBV2	292138	879664	100.00%	13.120%
50	6.042	1476	1478	1479	rBV2	231	93	0.01%	0.001%
51	6.238	1527	1539	1572	rBV	270118	573746	65.22%	8.558%
52	6.528	1619	1629	1631	rBV7	4115	5493	0.62%	0.082%
53	6.679	1663	1676	1707	rBV	188992	398772	45.33%	5.948%
54	6.885	1738	1740	1743	rVB2	392	212	0.02%	0.003%
55	7.033	1777	1786	1793	rBV3	281	410	0.05%	0.006%
56	7.277	1860	1862	1864	rBV	149	93	0.01%	0.001%
57	7.319	1873	1875	1877	rBV	371	172	0.02%	0.003%
58	7.422	1904	1907	1909	rBV	218	128	0.01%	0.002%
59	7.483	1921	1926	1929	rBV2	260	232	0.03%	0.003%
60	7.505	1931	1933	1938	rVB2	281	176	0.02%	0.003%
61	7.557	1938	1949	1971	rBV	79785	151566	17.23%	2.261%
62	7.682	1986	1988	1993	rVB3	434	293	0.03%	0.004%
63	7.721	1998	2000	2004	rBV2	414	307	0.03%	0.005%
64	7.846	2036	2039	2040	rBV2	393	205	0.02%	0.003%
65	7.888	2040	2052	2081	rBV	351853	678569	77.14%	10.121%
66	8.171	2130	2140	2161	rBV	50542	92161	10.48%	1.375%
67	8.345	2192	2194	2197	rVB2	395	212	0.02%	0.003%
68	8.441	2220	2224	2227	rBV2	228	204	0.02%	0.003%
69	8.480	2233	2236	2238	rBV2	148	93	0.01%	0.001%
70	8.544	2251	2256	2260	rBV4	734	752	0.09%	0.011%
71	8.627	2271	2282	2317	rBV2	175098	387524	44.05%	5.780%
72	8.962	2384	2386	2387	rBV2	285	125	0.01%	0.002%
73	9.107	2426	2431	2434	rBV2	503	478	0.05%	0.007%
74	9.190	2455	2457	2461	rVB	272	126	0.01%	0.002%
75	9.216	2461	2465	2470	rBV2	529	599	0.07%	0.009%
76	9.348	2504	2506	2510	rVB2	238	159	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
 Data File : VU063618.D
 Acq On : 22 Sep 2025 14:44
 Operator : MD/SY
 Sample : VU0922MBL01
 Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK121

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M

Title : VOC Analysis

77	9.409	2510	2525	2570	rBV	391734	724578	82.37%	10.807%
78	9.814	2647	2651	2655	rVB2	340	272	0.03%	0.004%
79	9.836	2655	2658	2661	rBV2	225	151	0.02%	0.002%
80	9.881	2671	2672	2675	rBV	183	82	0.01%	0.001%
81	9.959	2694	2696	2701	rBV	359	347	0.04%	0.005%
82	10.023	2712	2716	2719	rBV3	316	270	0.03%	0.004%
83	10.608	2895	2898	2901	rBV	269	172	0.02%	0.003%
84	10.746	2929	2941	2971	rBV	268664	448266	50.96%	6.686%
85	10.965	3006	3009	3012	rBV	236	135	0.02%	0.002%
86	11.396	3139	3143	3145	rBV3	308	274	0.03%	0.004%
87	11.473	3161	3167	3177	rBV5	1433	2349	0.27%	0.035%
88	11.531	3183	3185	3190	rVB	346	215	0.02%	0.003%
89	11.804	3259	3270	3289	rBV	370749	643631	73.17%	9.600%
90	12.187	3377	3389	3411	rBV	337522	586136	66.63%	8.742%
91	13.849	3898	3906	3916	rBV6	5344	9250	1.05%	0.138%
92	14.100	3976	3984	3994	rBV2	9944	19795	2.25%	0.295%
93	14.331	4049	4056	4067	rBV5	5333	8901	1.01%	0.133%




Sum of corrected areas: 6704585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
Data File : VU063618.D
Acq On : 22 Sep 2025 14:44
Operator : MD/SY
Sample : VU0922MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

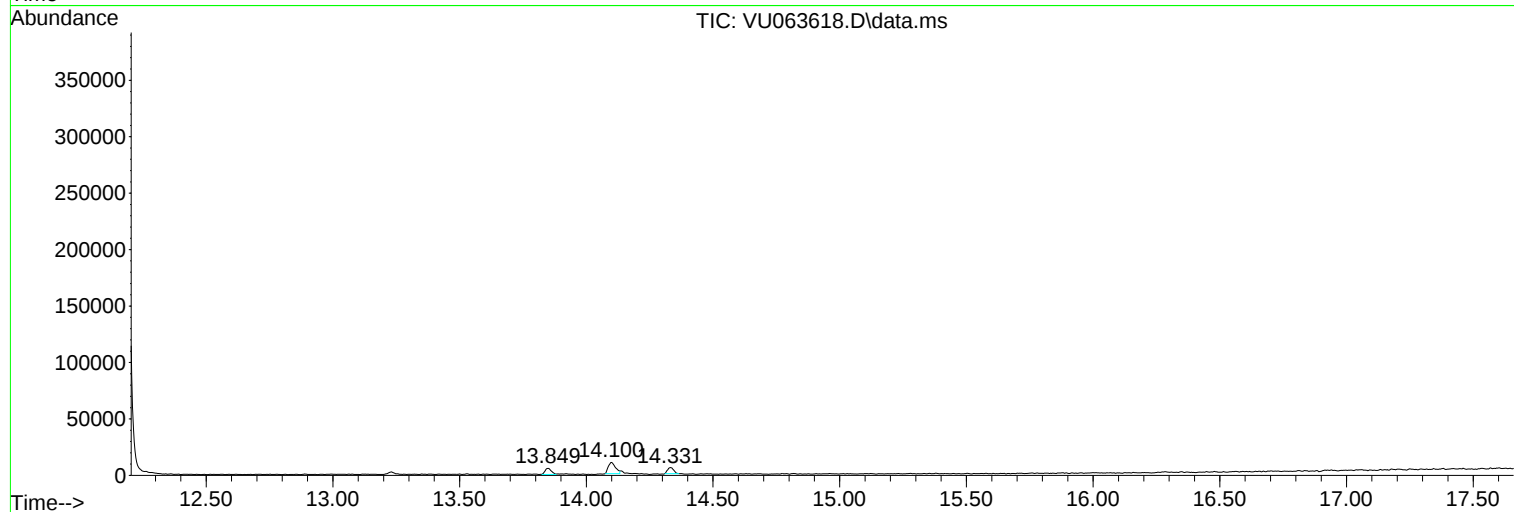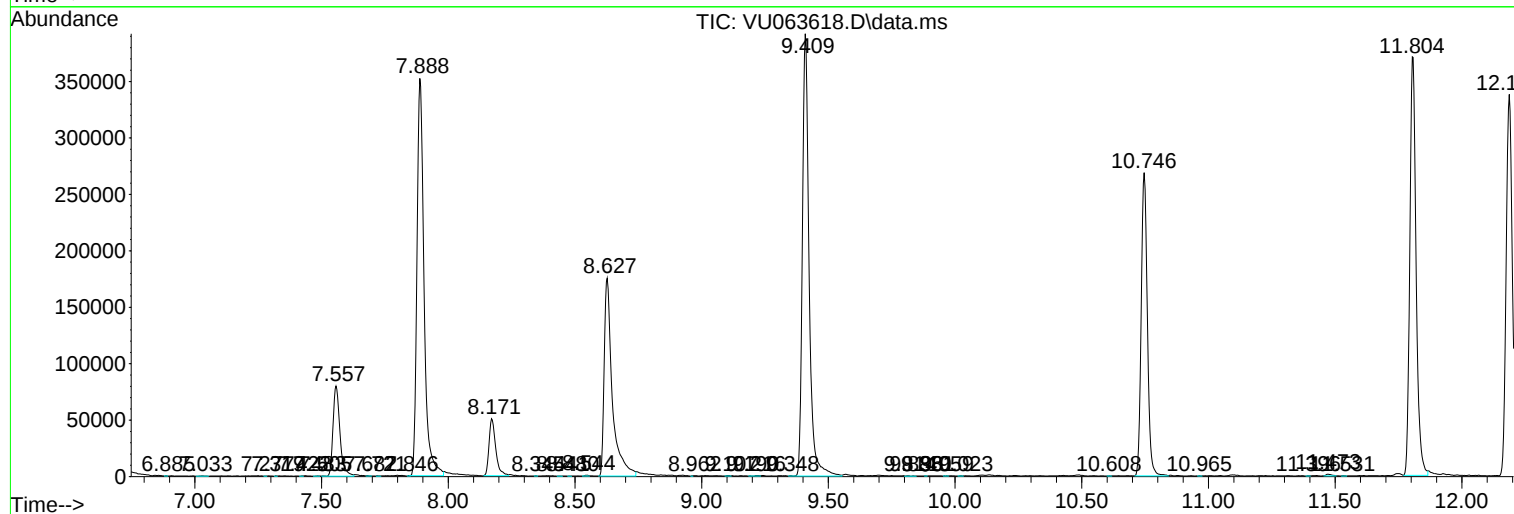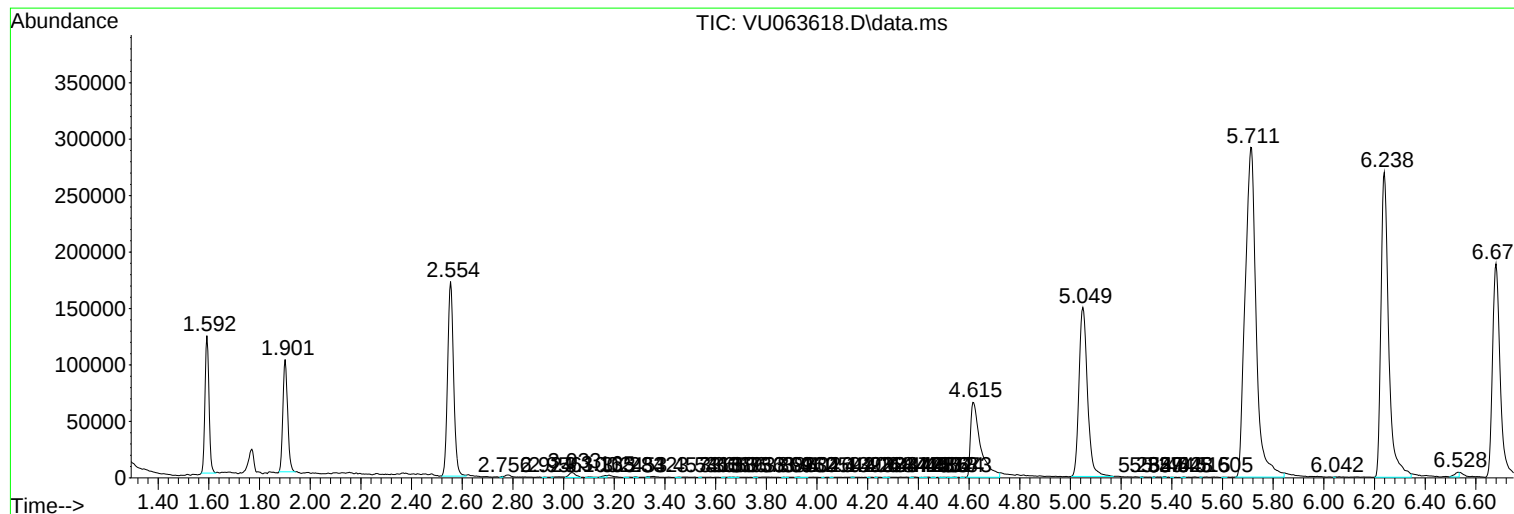

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
Data File : VU063618.D
Acq On : 22 Sep 2025 14:44
Operator : MD/SY
Sample : VU0922MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
Data File : VU063618.D
Acq On : 22 Sep 2025 14:44
Operator : MD/SY
Sample : VU0922MBL01
Misc : 5.00g/5.0mL/100uL/5mL/MSVOA_U/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK121

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc