


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092225\
Data File : VU063611.D
Acq On : 22 Sep 2025 09:09
Operator : MD/SY
Sample : BFB088
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB088

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Title : VOC Analysis
Last Update : Wed Sep 24 01:10:58 2025

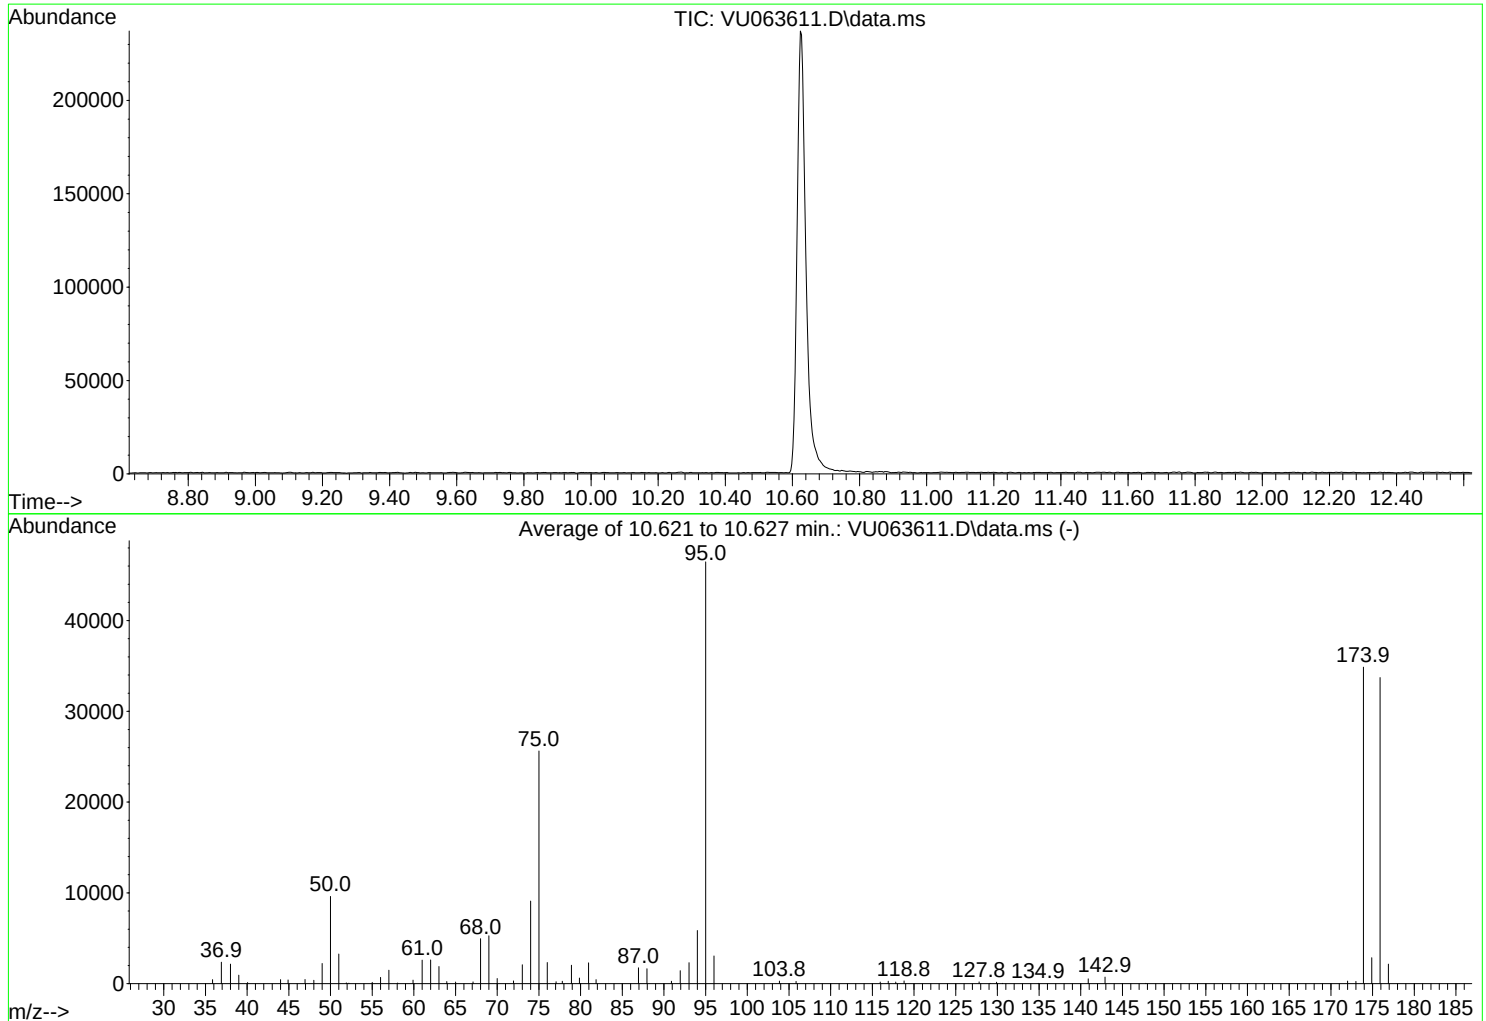

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	9611	PASS
75	95	30	80	55.1	25624	PASS
95	95	100	100	100.0	46467	PASS
96	95	5	9	6.6	3051	PASS
173	174	0.00	2	0.7	256	PASS
174	95	50	120	75.0	34861	PASS
175	174	5	9	8.2	2856	PASS
176	174	95	101	96.7	33712	PASS
177	176	5	9	6.4	2149	PASS

m/z	Abundance
39.90	242.0
44.00	381.0

Instrument :
MSVOA_U
ClientSampleId :
BFB088

m/z	Abundance
35.80	416.0
36.90	2300.0
38.00	2047.0
39.00	842.0
40.10	196.0
44.00	787.0
44.90	399.0
46.90	418.0
48.00	323.0
49.00	1987.0
50.00	9353.0
51.00	3340.0
52.20	139.0
55.00	139.0
56.00	691.0
57.00	1395.0
59.90	350.0
61.00	2520.0
62.00	2586.0
63.00	1860.0
64.00	221.0
65.00	184.0
67.10	221.0
68.00	4752.0
69.00	5010.0
70.00	557.0
71.90	210.0
73.00	1934.0
74.00	8515.0
75.00	24312.0
76.00	2285.0
77.00	171.0
77.80	283.0
78.90	1962.0
79.90	555.0
81.00	2170.0
81.90	420.0
87.00	1578.0
87.90	1570.0
90.90	225.0
92.00	1300.0
93.00	2245.0
94.00	5672.0
95.00	44616.0
96.00	3040.0
103.80	259.0
105.90	196.0
116.00	155.0
117.00	202.0
117.70	169.0
118.80	307.0
127.80	207.0
129.90	151.0
140.90	517.0
142.90	761.0
172.00	235.0
173.00	363.0
173.90	31984.0
174.90	2790.0
175.90	31472.0
176.90	1990.0

Instrument :
MSVOA_U
ClientSampleId :
BFB088

m/z	Abundance
35.90	453.0
36.90	2422.0
38.00	2235.0
39.00	956.0
40.00	173.0
44.00	838.0
44.90	421.0
46.90	444.0
48.00	398.0
49.00	2309.0
50.00	10057.0
51.00	3374.0
51.90	148.0
55.00	143.0
56.00	693.0
57.00	1511.0
58.10	112.0
59.90	399.0
61.00	2663.0
62.00	2677.0
63.00	1962.0
63.90	226.0
65.00	181.0
67.10	204.0
68.00	5064.0
69.00	5418.0
70.00	596.0
72.00	276.0
73.00	2132.0
74.00	9361.0
75.00	26432.0
76.00	2422.0
77.00	184.0
77.80	281.0
78.90	2088.0
79.90	639.0
81.00	2361.0
81.80	457.0
86.90	1834.0
88.00	1630.0
90.90	294.0
92.00	1485.0
93.00	2471.0
94.00	6002.0
95.00	47848.0
96.00	3111.0
103.90	295.0
105.90	266.0
116.00	197.0
116.90	246.0
117.80	170.0
118.80	316.0
127.80	195.0
129.90	182.0
130.60	100.0
140.90	539.0
142.90	747.0
172.00	302.0
173.00	405.0
173.90	35848.0
174.90	2970.0
175.90	34744.0
176.90	2225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB088

m/z	Abundance
35.90	455.0
36.90	2392.0
38.00	2176.0
39.00	998.0
39.80	190.0
44.00	853.0
44.90	414.0
47.00	516.0
48.00	403.0
49.00	2370.0
50.00	9422.0
51.00	3087.0
51.90	127.0
55.00	133.0
56.00	692.0
57.00	1560.0
58.00	108.0
59.90	429.0
61.00	2602.0
62.00	2563.0
63.00	1842.0
63.90	223.0
65.00	159.0
67.10	156.0
68.00	5058.0
69.00	5400.0
70.00	530.0
72.00	395.0
73.00	2170.0
74.00	9419.0
75.00	26128.0
76.00	2284.0
77.10	256.0
77.80	212.0
78.90	2027.0
79.80	646.0
80.90	2330.0
81.80	477.0
86.90	1819.0
88.00	1704.0
90.90	285.0
91.90	1490.0
93.00	2235.0
94.00	5910.0
95.00	46936.0
96.00	3003.0
103.90	289.0
105.80	284.0
115.90	197.0
116.80	341.0
117.90	193.0
118.80	275.0
127.80	169.0
129.10	103.0
129.90	169.0
134.90	118.0
140.90	549.0
142.90	658.0
147.80	128.0
172.00	315.0
173.90	36752.0
174.90	2809.0
175.90	34920.0
176.90	2233.0

Instrument :
MSVOA_U
ClientSampleId :
BFB088