

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092318\
 Data File : VU027084.D
 Acq On : 23 Sep 2018 19:56
 Operator : MD/SY
 Sample : J4954-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 128 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 SA-SW125-20180914

Quant Time: Sep 24 08:59:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 22 01:31:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	104366	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	179566	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	170676	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	77470	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	109414	52.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.18%	
35) Dibromofluoromethane	4.89	113	75765	48.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.36%	
50) Toluene-d8	7.57	98	287607	48.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.98%	
62) 4-Bromofluorobenzene	10.31	95	91944	45.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.34%	
Target Compounds						
68) m/p-Xylenes	9.38	106	477	1.657	ug/l	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092318\
Data File : VU027084.D
Acq On : 23 Sep 2018 19:56
Operator : MD/SY
Sample : J4954-03
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 128 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
SA-SW125-20180914

Quant Time: Sep 24 08:59:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 22 01:31:57 2018
Response via : Initial Calibration

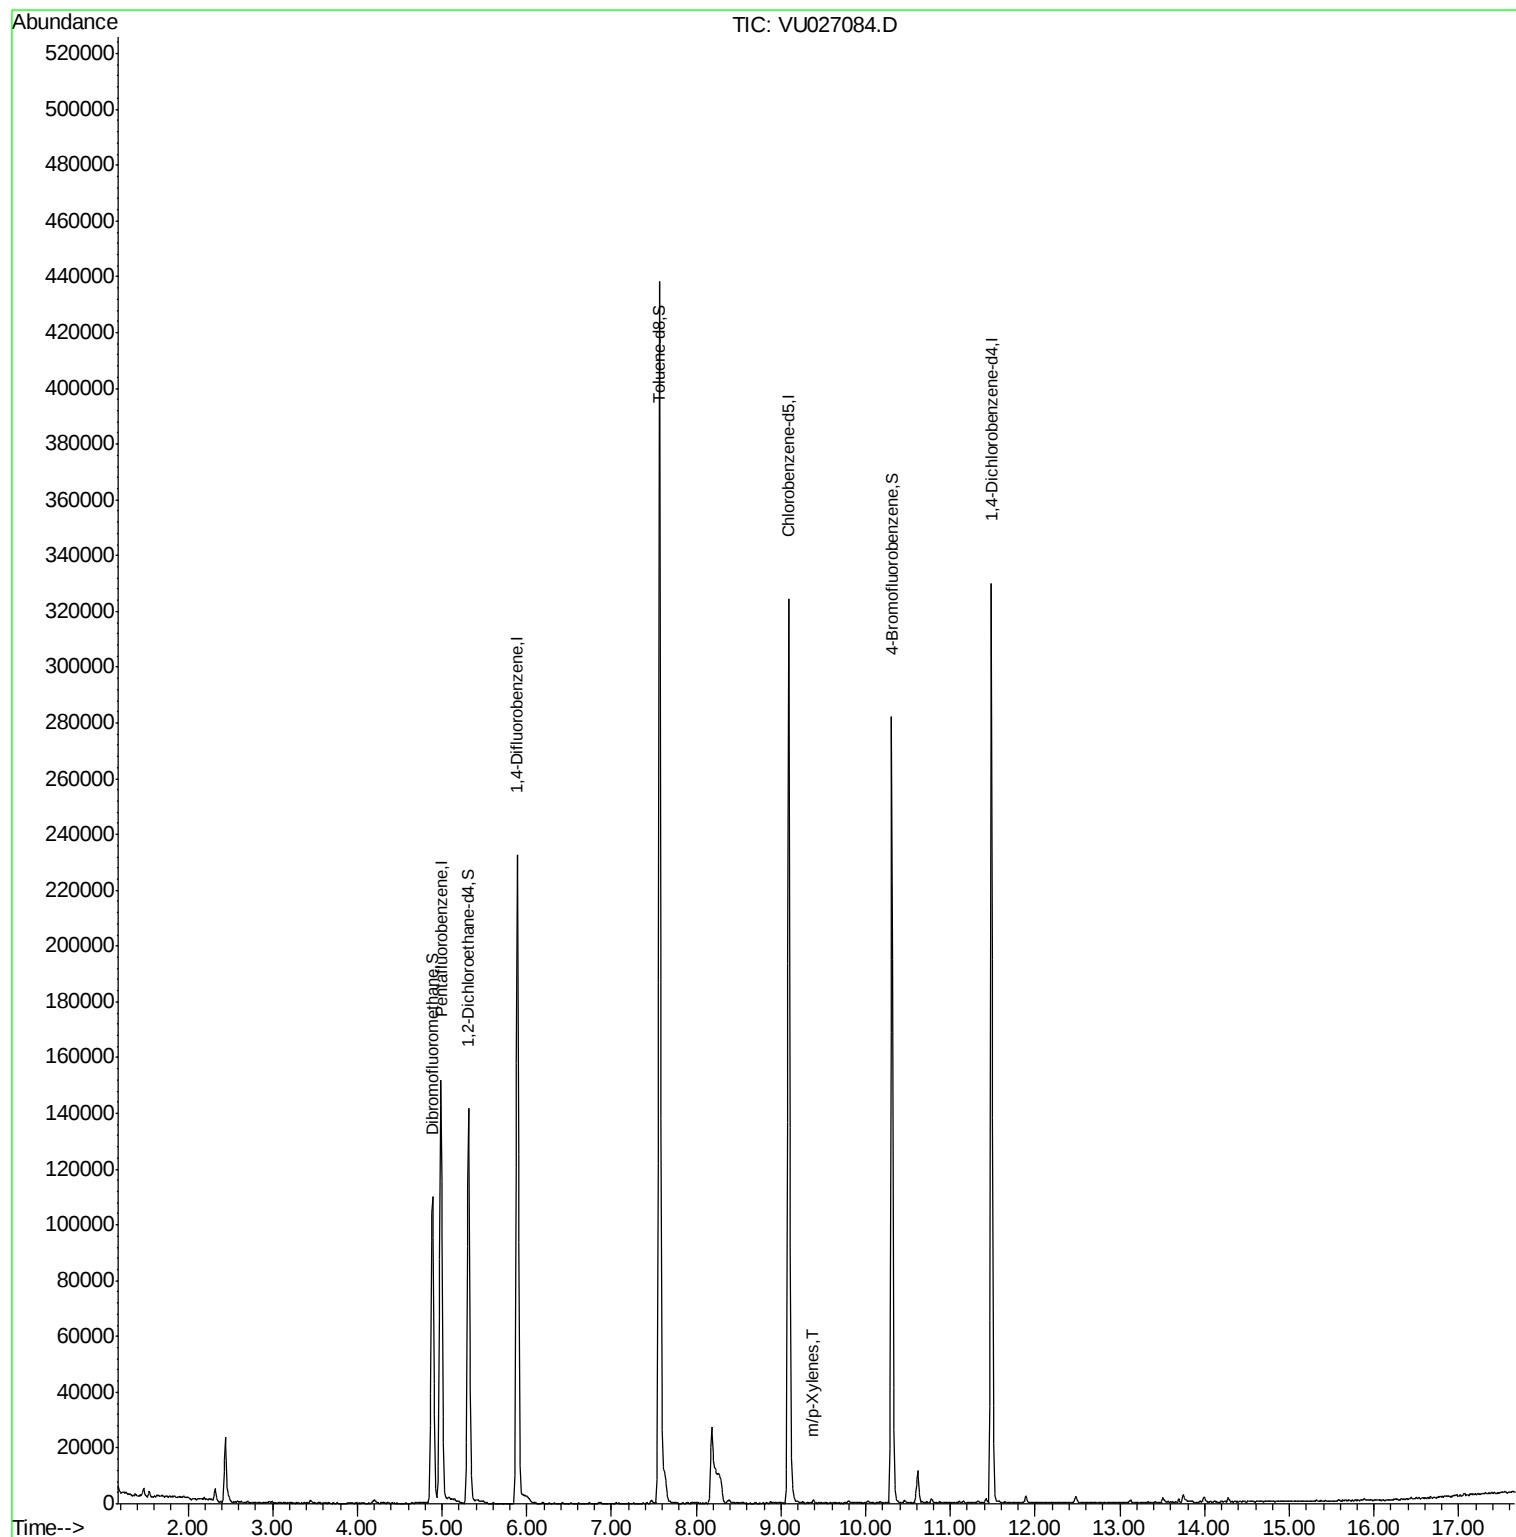

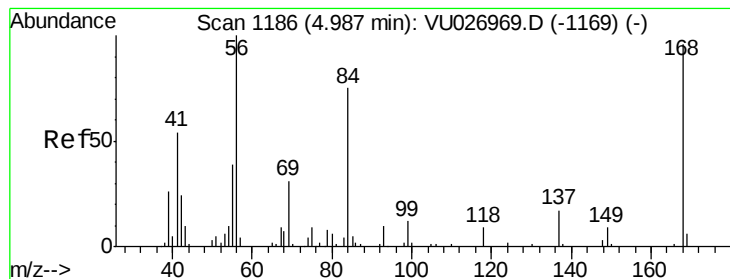

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU027084.D

Acq: 23 Sep 2018 19:56

Instrument :

MSVOA_U

ClientSampleId :


SA-SW125-20180914

Tot Ion:168 Resp: 104366

Ion Ratio Lower Upper

168 100

99 63.3 48.1 72.1

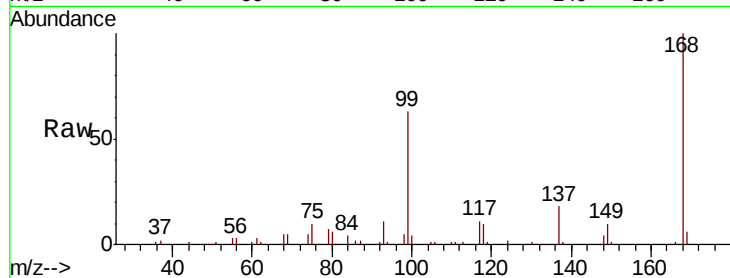

Abundance Ion 167.90 (167.60 to 168.60): VU026969.D (-1169) (-)

Ion 98.90 (98.60 to 99.60): VU026969.D (-1169) (-)

4.99

50000

40000

30000



20000

10000

0

Time-->

4.90 4.95 5.00 5.05

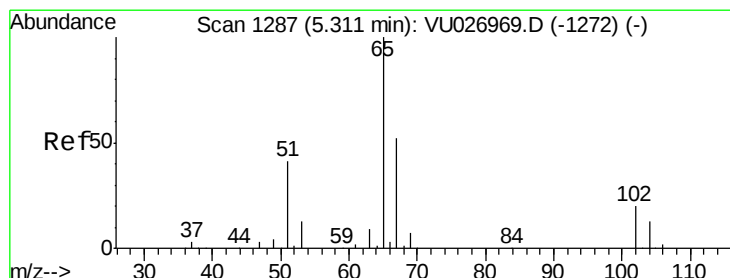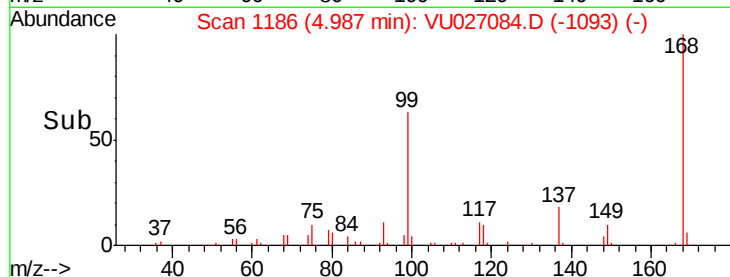

#33

1,2-Dichloroethane-d4

Concen: 52.089 ug/l

RT: 5.31 min Scan# 1287

Delta R.T. 0.00 min

Lab File: VU027084.D


Acq: 23 Sep 2018 19:56

Tgt Ion: 65 Resp: 109414

Ion Ratio Lower Upper

65 100

67 52.7 0.0 105.6

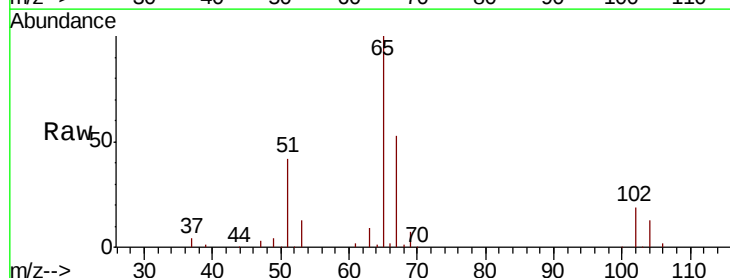

Abundance Ion 64.90 (64.60 to 65.60): VU026969.D (-1272) (-)

Ion 66.90 (66.60 to 67.60): VU026969.D (-1272) (-)

5.31

60000

50000

40000

30000


20000


10000

0

Time-->

5.20 5.25 5.30 5.35 5.40

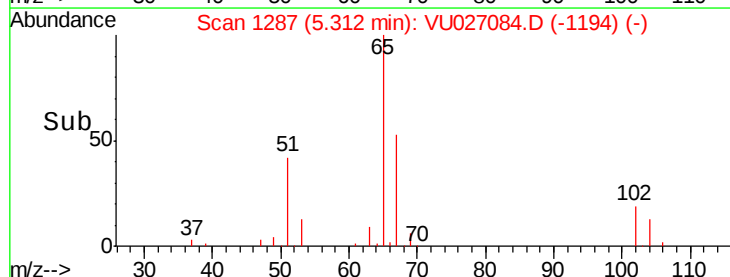


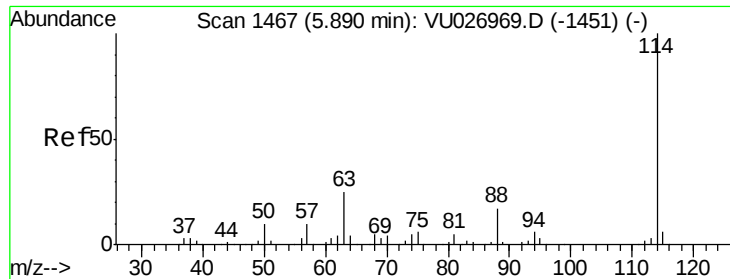




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1467
 Delta R.T. 0.00 min
 Lab File: VU027084.D
 Acq: 23 Sep 2018 19:56

Instrument :
 MSVOA_U
 ClientSampleId :
 SA-SW125-20180914

Tot Ion:114 Resp: 179566
 Ion Ratio Lower Upper
 114 100
 63 25.1 0.0 49.2
 88 17.0 0.0 33.8

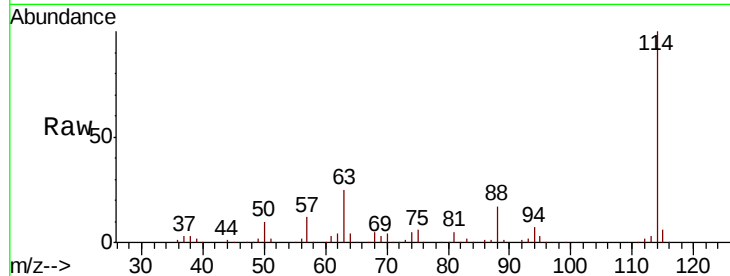


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

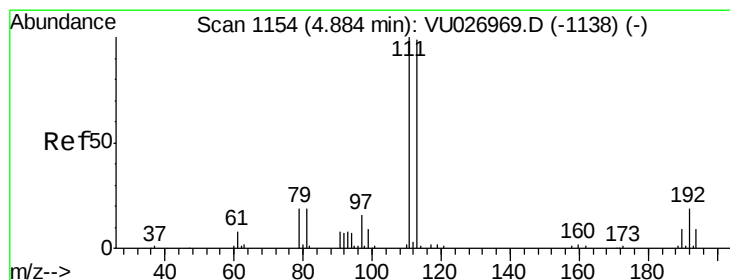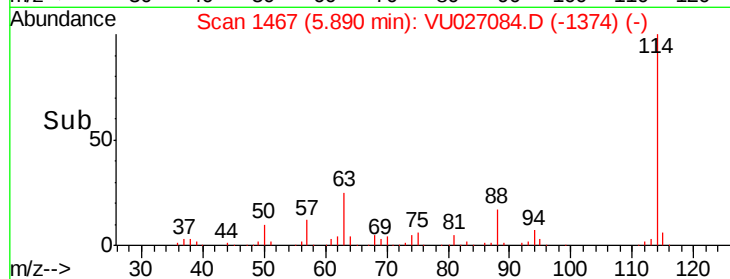
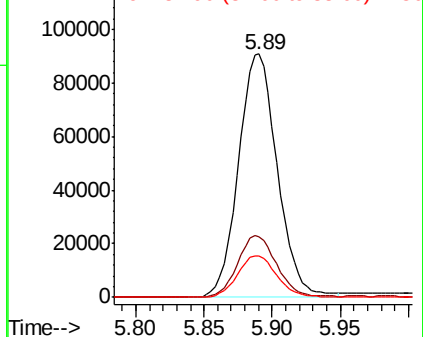


#35
 Dibromofluoromethane
 Concen: 48.677 ug/l
 RT: 4.89 min Scan# 1155
 Delta R.T. 0.00 min
 Lab File: VU027084.D
 Acq: 23 Sep 2018 19:56

Tgt Ion:113 Resp: 75765
 Ion Ratio Lower Upper
 113 100
 111 101.7 82.2 123.4
 192 18.9 15.2 22.8

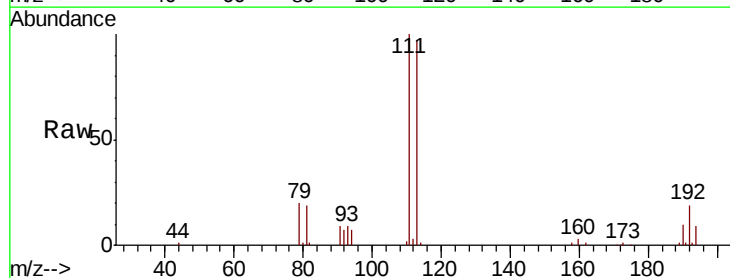

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



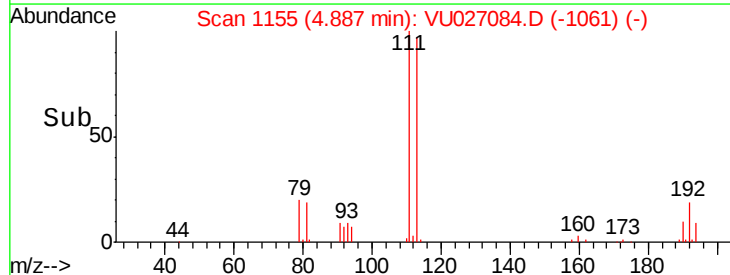
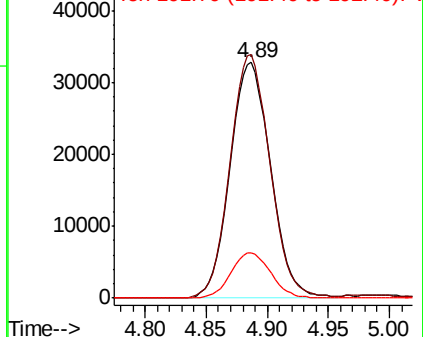




#50
Toluene-d8
Concen: 48.486 ug/l
RT: 7.57 min Scan# 1988
Delta R.T. -0.00 min
Lab File: VU027084.D
Acq: 23 Sep 2018 19:56




Instrument :
MSVOA_U
ClientSampleId :
SA-SW125-20180914


Tot Ion: 98 Resp: 287607
Ion Ratio Lower Upper
98 100
100 64.3 52.1 78.1

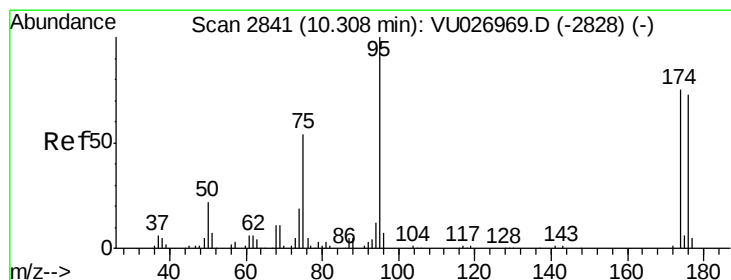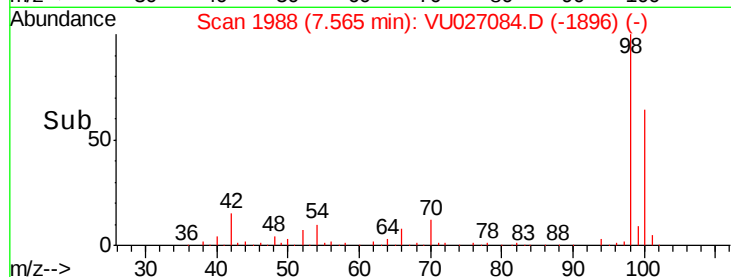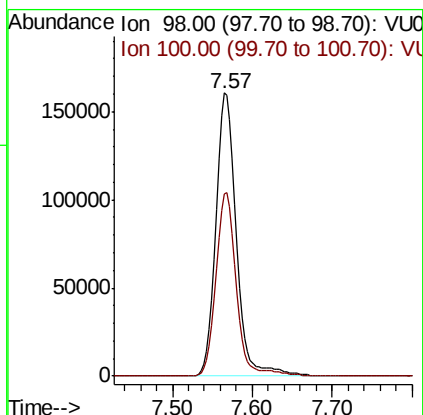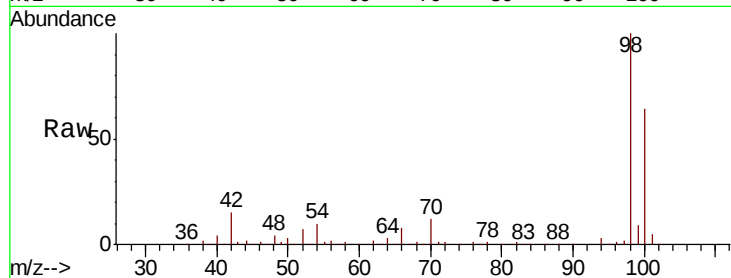

#62
4-Bromofluorobenzene
Concen: 45.173 ug/l
RT: 10.31 min Scan# 2841
Delta R.T. 0.00 min
Lab File: VU027084.D
Acq: 23 Sep 2018 19:56

Tgt Ion: 95 Resp: 91944
Ion Ratio Lower Upper
95 100
174 73.6 0.0 150.2
176 70.9 0.0 145.2

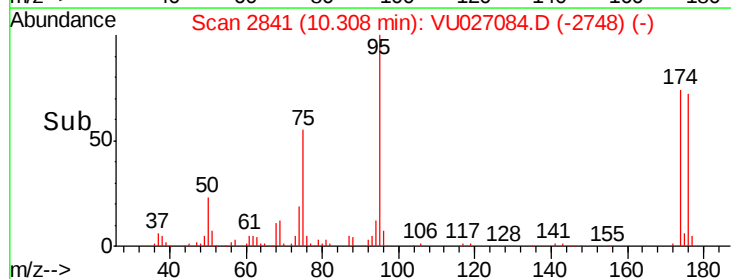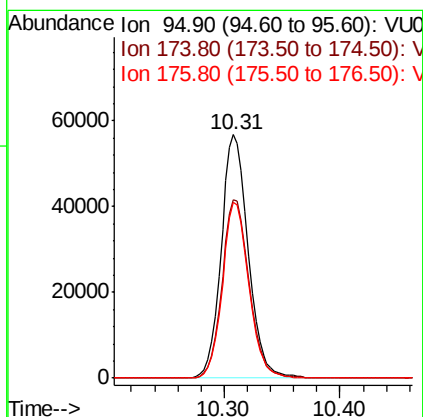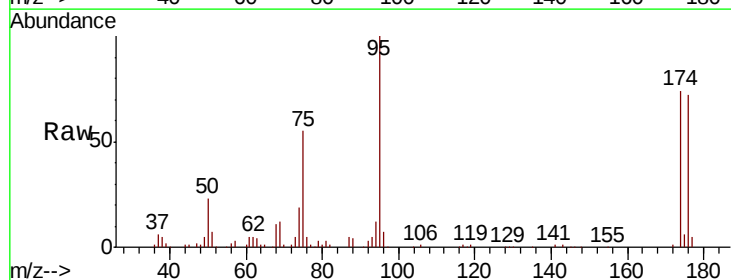


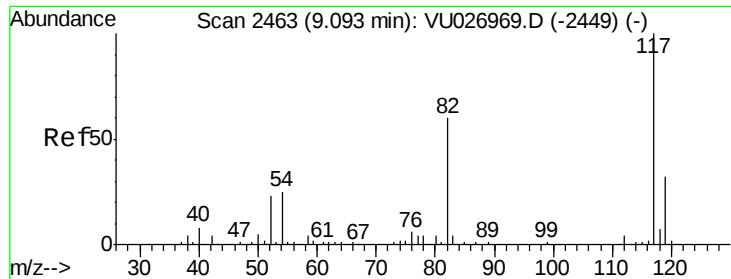




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. -0.00 min
Lab File: VU027084.D
Acq: 23 Sep 2018 19:56

Instrument :
MSVOA_U
ClientSampleId :
SA-SW125-20180914

Tot Ion:117 Resp: 170676
Ion Ratio Lower Upper
117 100
82 61.1 48.0 72.0
119 32.4 25.8 38.8

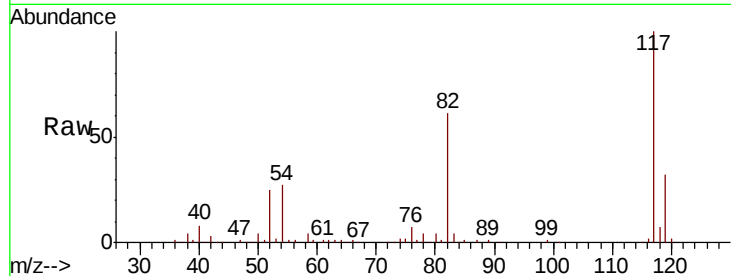


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VU0
Ion 118.90 (118.60 to 119.60): V

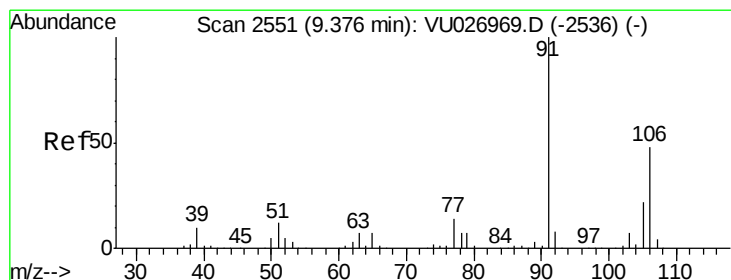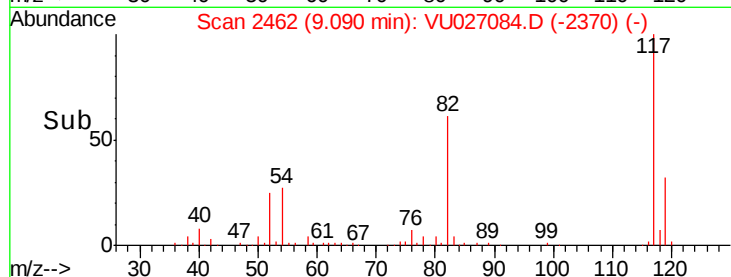
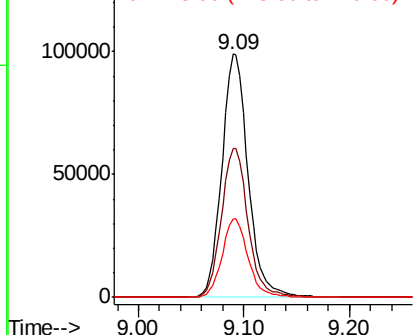



#68
m/p-Xylenes
Concen: 1.657 ug/l
RT: 9.38 min Scan# 2552
Delta R.T. 0.00 min
Lab File: VU027084.D
Acq: 23 Sep 2018 19:56

Tgt Ion:106 Resp: 477
Ion Ratio Lower Upper
106 100
91 234.4 166.5 249.7

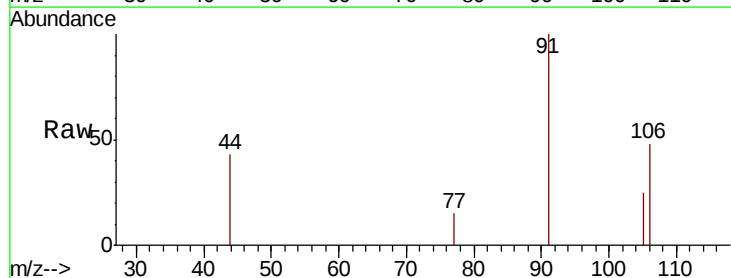

Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VU0

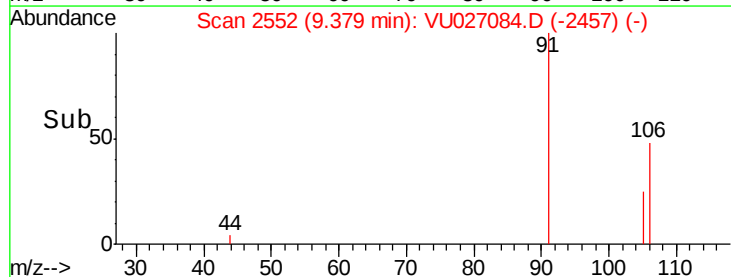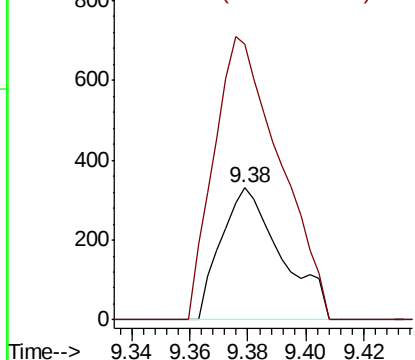

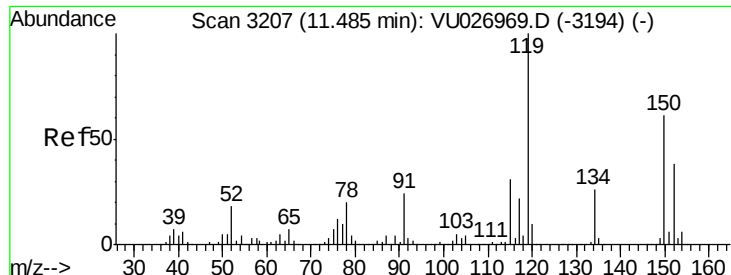

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.48 min Scan# 3207
 Delta R.T. 0.00 min
 Lab File: VU027084.D
 Acq: 23 Sep 2018 19:56

Instrument :
 MSVOA_U
 ClientSampleId :
 SA-SW125-20180914

Tot Ion:152 Resp: 77470
 Ion Ratio Lower Upper
 152 100
 115 61.8 44.9 134.5
 150 157.4 0.0 355.8

