


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092318\
 Data File : VU027040.D
 Acq On : 23 Sep 2018 00:42
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
 Title : SW846 8260
 Last Update : Sat Sep 22 01:31:57 2018

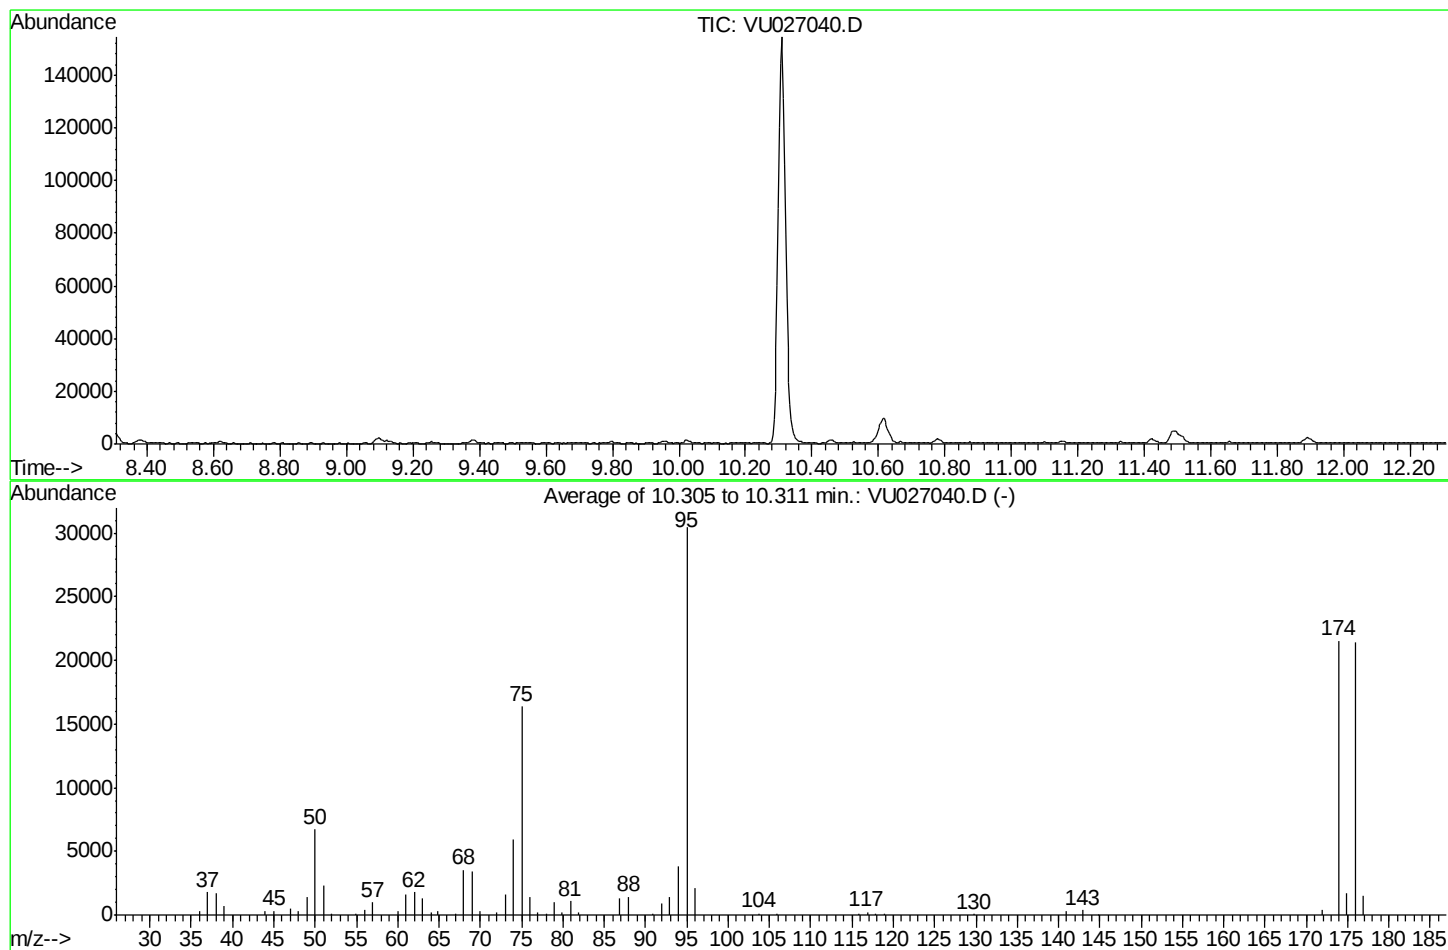

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	6722	PASS
75	95	30	60	53.7	16349	PASS
95	95	100	100	100.0	30456	PASS
96	95	5	9	6.9	2108	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.8	21570	PASS
175	174	5	9	7.9	1699	PASS
176	174	95	101	99.1	21378	PASS
177	176	5	9	6.9	1469	PASS