


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092318\
Data File : VU027064.D
Acq On : 23 Sep 2018 11:09
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 106 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

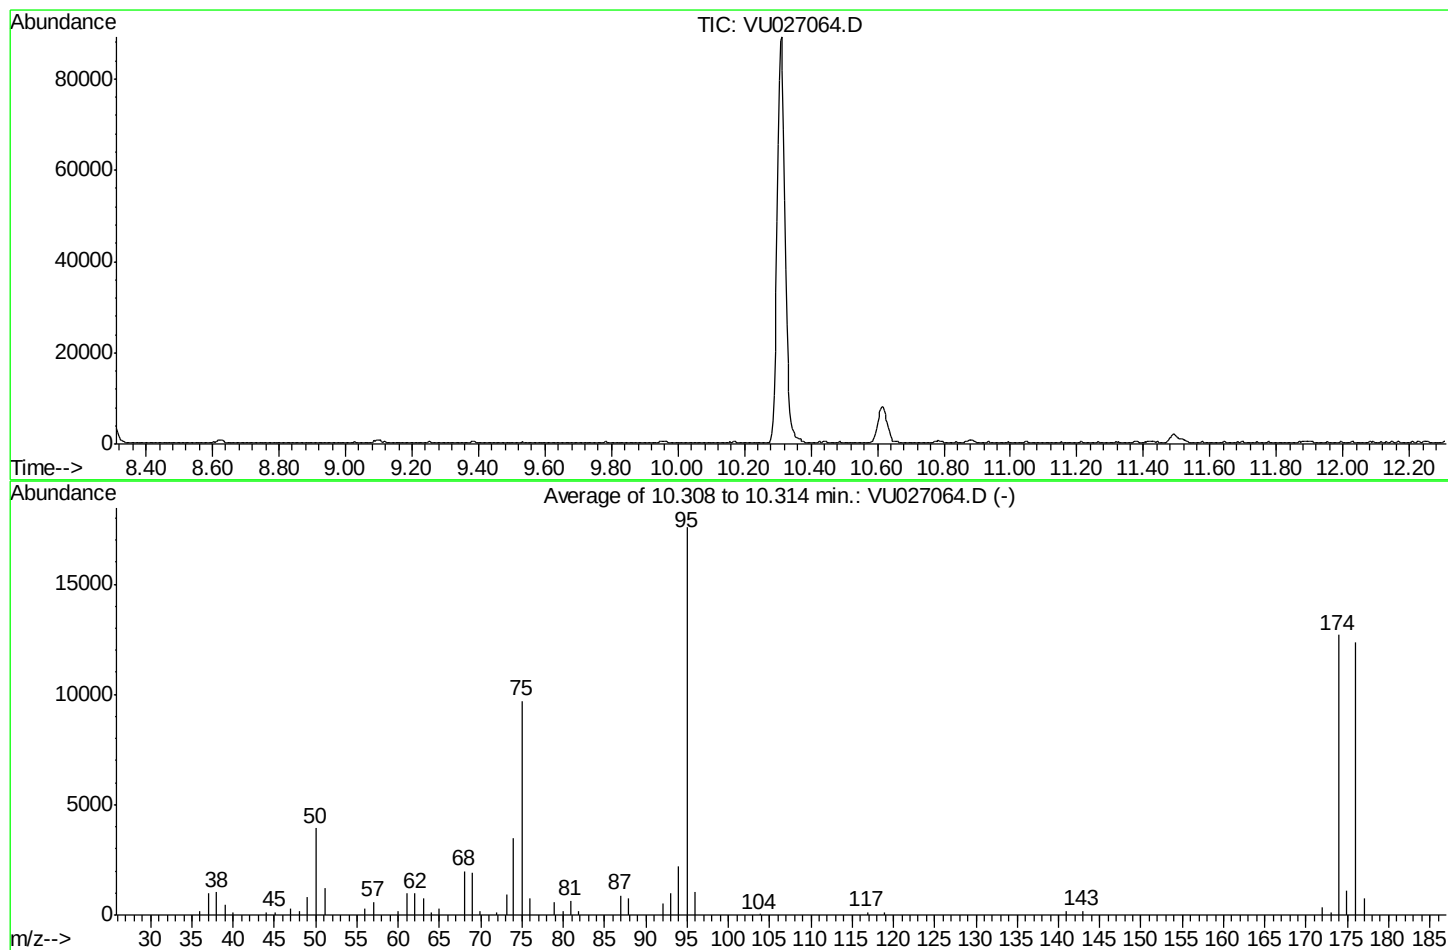

AutoFind: Scans 2841, 2842, 2843; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	3920	PASS
75	95	30	60	55.2	9701	PASS
95	95	100	100	100.0	17573	PASS
96	95	5	9	5.9	1042	PASS
173	174	0.00	2	0.7	93	PASS
174	95	50	100	72.3	12703	PASS
175	174	5	9	8.6	1096	PASS
176	174	95	101	97.4	12379	PASS
177	176	5	9	6.1	761	PASS