

Data File : VU034757.D
Acq On : 24 Sep 2019 00:50
Operator : JC/SP
Sample : K4932-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDM5

Quant Time: Sep 24 03:43:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	519352	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	487458	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	232529	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	208767	39.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.54%
7) Chloroethane-d5	1.67	69	175944	42.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.64%
11) 1,1-Dichloroethene-d2	2.26	63	292827	32.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.04%
21) 2-Butanone-d5	4.15	46	466434	114.47	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.47%
24) Chloroform-d	4.62	84	367373	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
26) 1,2-Dichloroethane-d4	5.29	65	269079	47.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.72%
32) Benzene-d6	5.32	84	736369	48.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.48%
36) 1,2-Dichloropropane-d6	6.31	67	263423	49.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.76%
41) Toluene-d8	7.54	98	712117	49.54	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.08%
43) trans-1,3-Dichloropropene-	7.83	79	116839	46.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.40%
47) 2-Hexanone-d5	8.29	63	310599	117.10	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	117.10%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	361299	49.31	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.62%
64) 1,2-Dichlorobenzene-d4	11.84	152	250878	51.45	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.90%

Target Compounds


					Qvalue
13) Acetone	2.31	43	64198	13.544	ug/L 98
16) Methylene chloride	2.68	84	1794900	417.010	ug/L 97
33) Benzene	5.37	78	33278	1.968	ug/L 100
39) cis-1,3-Dichloropropene	7.21	75	8386	1.109	ug/L 83
40) 4-Methyl-2-pentanone	7.40	43	101048	10.514	ug/L # 59
42) Toluene	7.61	91	349198	19.112	ug/L 99
52) Ethylbenzene	9.23	91	102762	4.995	ug/L 100
53) m,p-Xylene	9.35	106	252281	34.619	ug/L 96
54) o-xylene	9.76	106	170867	23.706	ug/L 96
56) Isopropylbenzene	10.14	105	27318	1.406	ug/L 97
65) 1,2-Dichlorobenzene	11.85	146	68546	8.425	ug/L 99
69) Naphthalene	13.72	128	406366	27.666	ug/L 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU034757.D
Acq On : 24 Sep 2019 00:50
Operator : JC/SP
Sample : K4932-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDM5

Quant Time: Sep 24 03:43:52 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

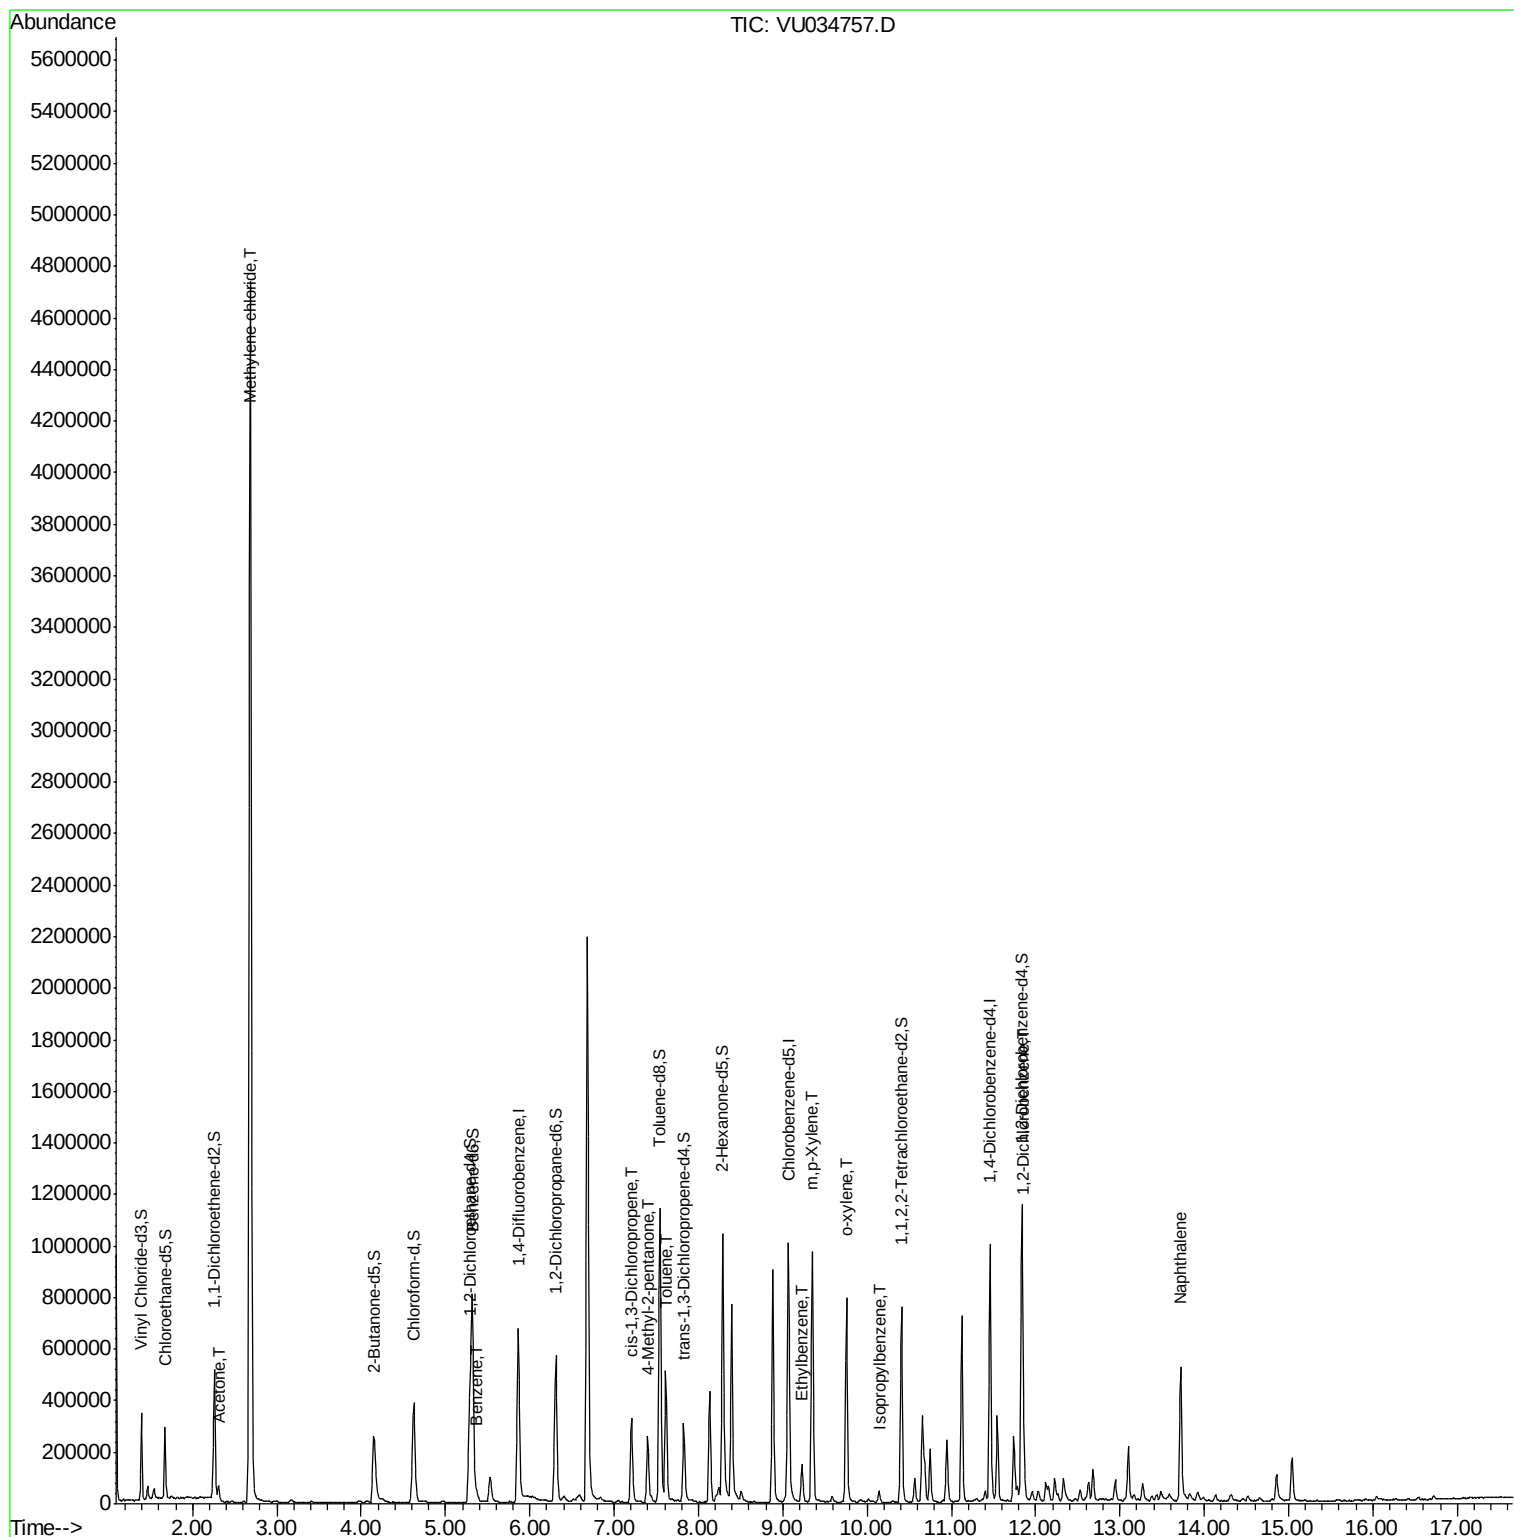

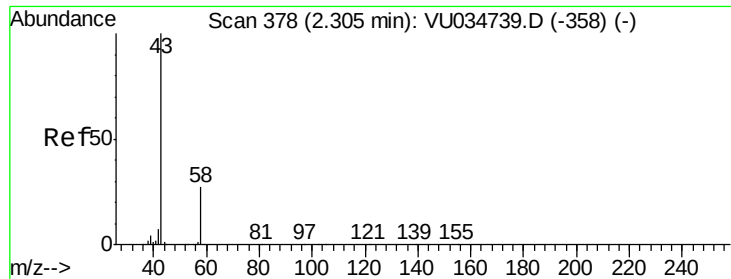

#13

Acetone

Concen: 13.544 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VU034757.D

Acq: 24 Sep 2019 00:50

Instrument :

MSVOA_U

ClientSampleId :





BFDMS

Tgt Ion: 43 Resp: 64198

Ion Ratio Lower Upper

43 100

58 27.8 0.0 53.4

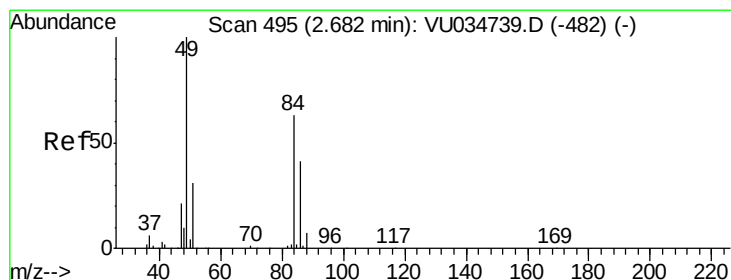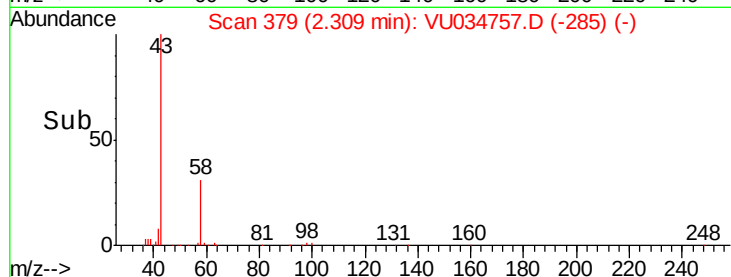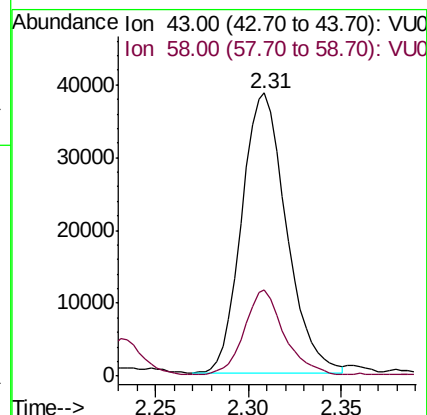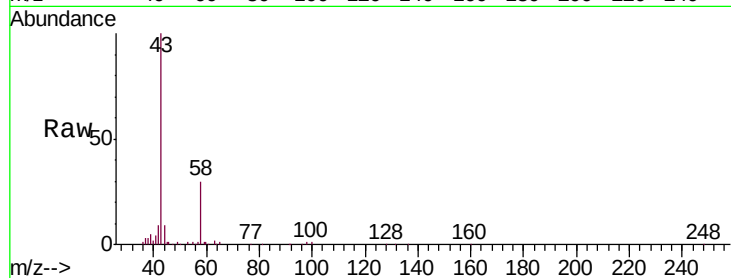

#16

Methylene chloride

Concen: 417.010 ug/L

RT: 2.68 min Scan# 496

Delta R.T. 0.00 min

Lab File: VU034757.D

Acq: 24 Sep 2019 00:50




Tgt Ion: 84 Resp: 1794900


Ion Ratio Lower Upper

84 100

86 64.9 43.0 80.0

49 159.5 109.7 203.7

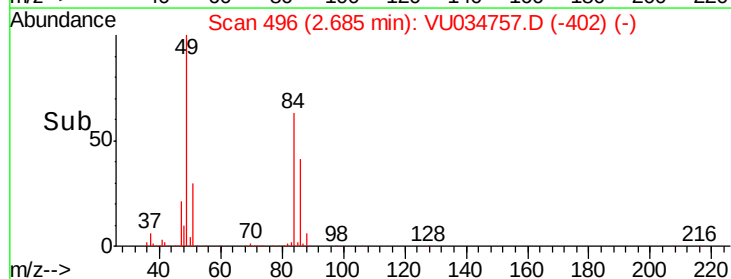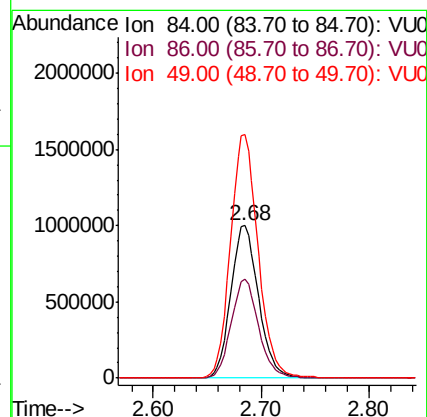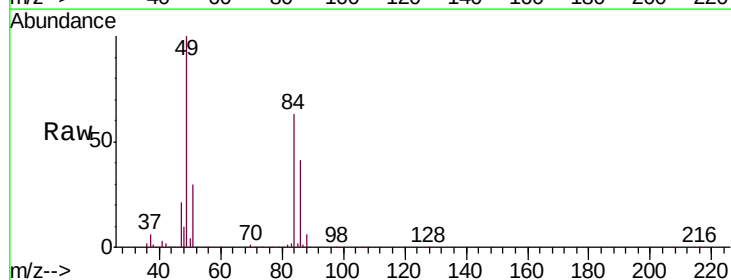

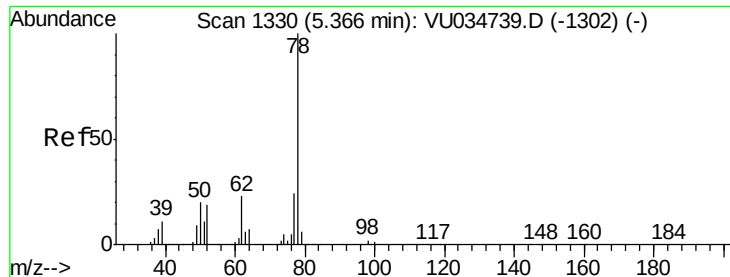

#33

Benzene

Concen: 1.968 ug/L

RT: 5.37 min Scan# 1331

Delta R.T. 0.00 min

Lab File: VU034757.D

Acq: 24 Sep 2019 00:50


Instrument :

MSVOA_U




ClientSampleId :

BFDM5

Tgt Ion: 78 Resp: 33278

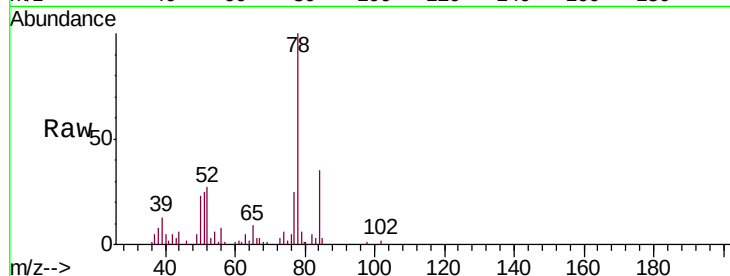

Abundance Ion 78.00 (77.70 to 78.70): VU0

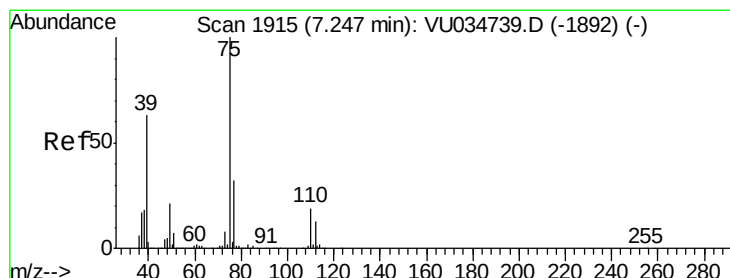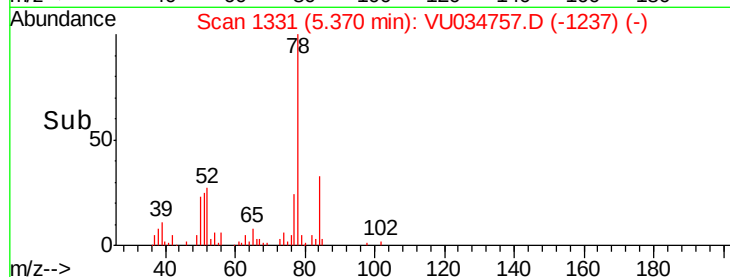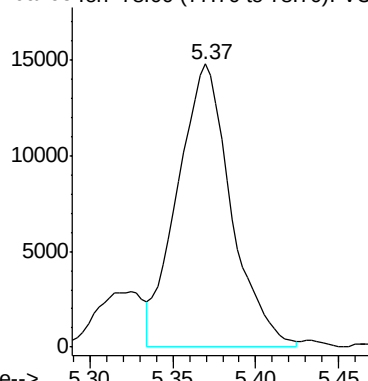

#39

cis-1,3-Dichloropropene

Concen: 1.109 ug/L

RT: 7.21 min Scan# 1903

Delta R.T. -0.04 min

Lab File: VU034757.D


Acq: 24 Sep 2019 00:50

Tgt Ion: 75 Resp: 8386



Ion Ratio Lower Upper


75 100

77 39.8 21.4 39.8

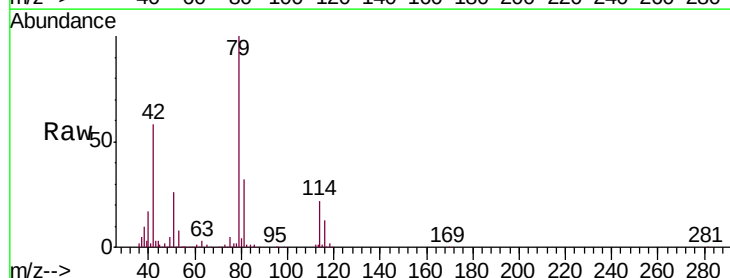

Abundance Ion 75.00 (74.70 to 75.70): VU0



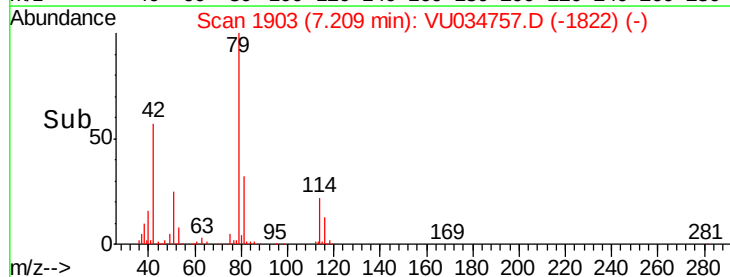
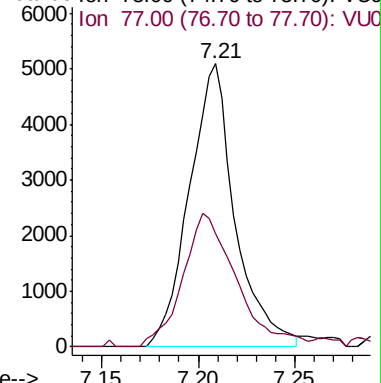


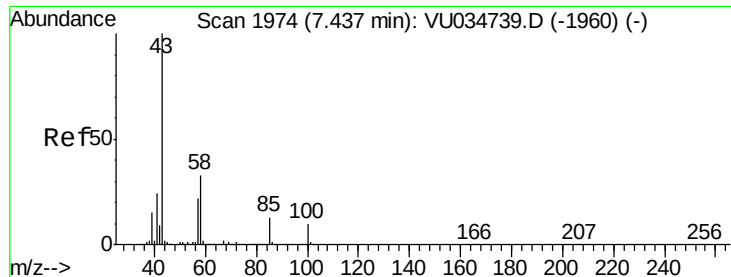

#40
 4-Methyl-2-pentanone
 Concen: 10.514 ug/L
 RT: 7.40 min Scan# 1962
 Delta R.T. -0.04 min
 Lab File: VU034757.D
 Acq: 24 Sep 2019 00:50




Instrument :
 MSVOA_U
 ClientSampleId :
 BFDM5


Tgt Ion: 43 Resp: 101048
 Ion Ratio Lower Upper
 43 100
 58 6.0 25.2 37.8#
 100 0.0 7.7 11.5#

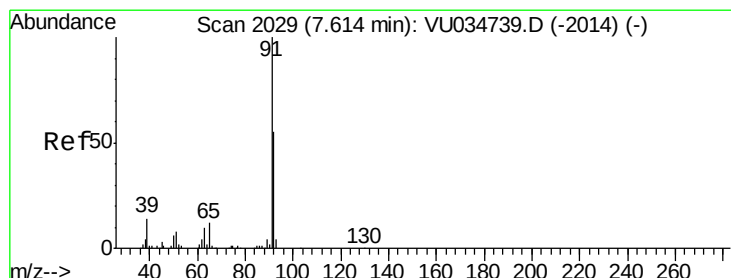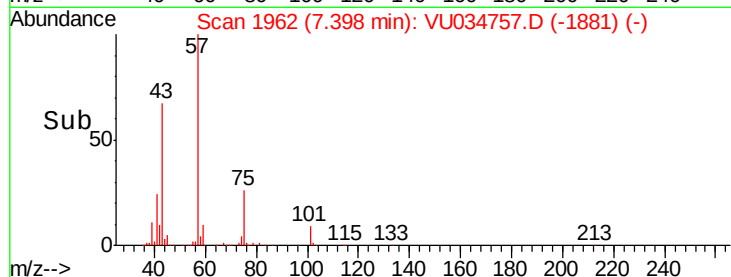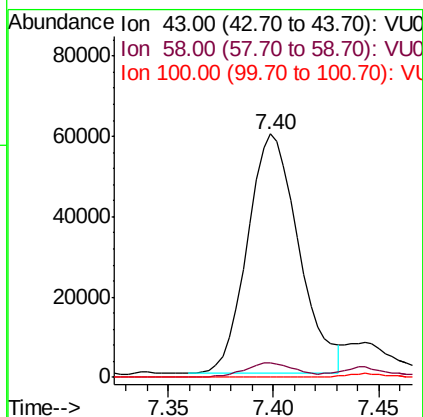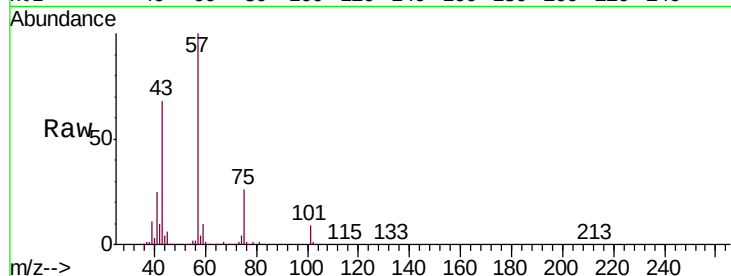

#42
 Toluene
 Concen: 19.112 ug/L
 RT: 7.61 min Scan# 2029
 Delta R.T. -0.00 min
 Lab File: VU034757.D
 Acq: 24 Sep 2019 00:50

Tgt Ion: 91 Resp: 349198
 Ion Ratio Lower Upper
 91 100
 92 55.5 38.2 71.0

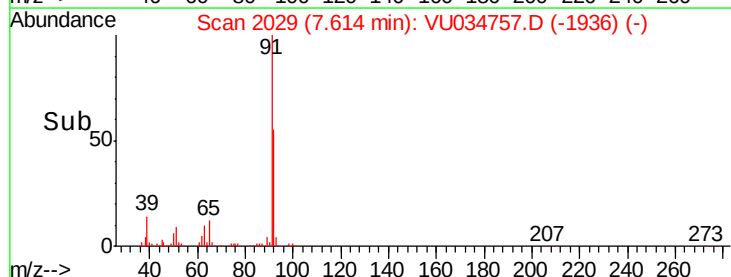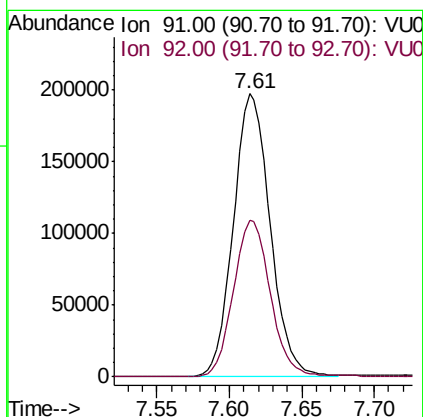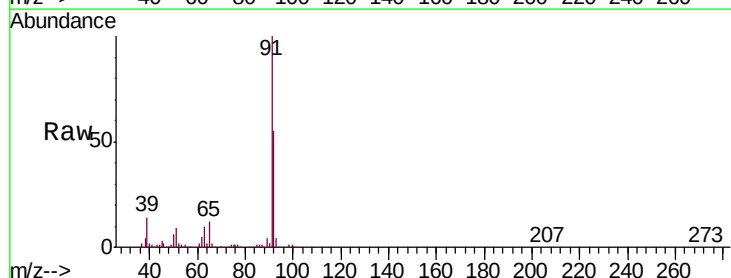

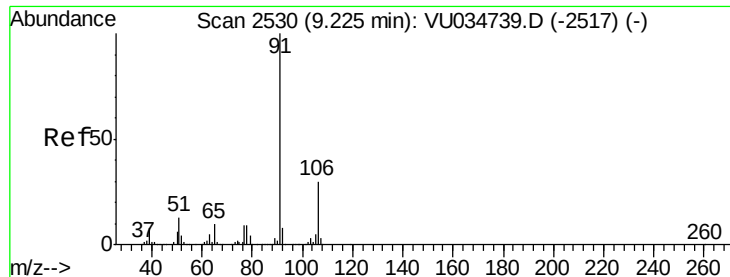

#52

Ethylbenzene

Concen: 4.995 ug/L

RT: 9.23 min Scan# 2531

Delta R.T. 0.00 min

Lab File: VU034757.D

Acq: 24 Sep 2019 00:50

Instrument :

MSVOA_U

ClientSampleId :


BFDM5

Tgt Ion: 91 Resp: 102762




Ion Ratio Lower Upper

91 100

106 29.5 20.6 38.4

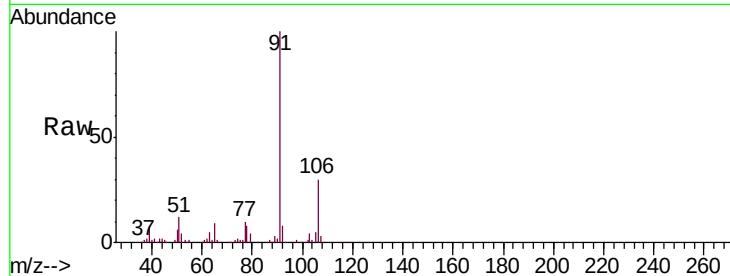

Abundance Ion 91.00 (90.70 to 91.70): VU034739.D (-2517) (-)

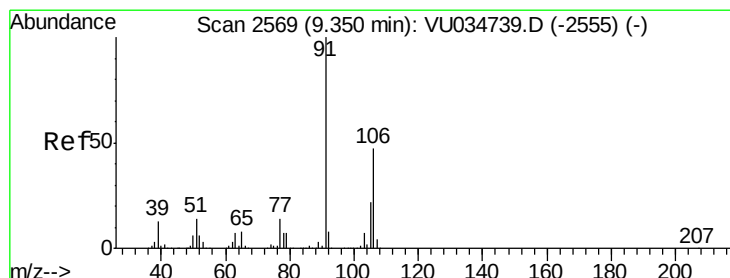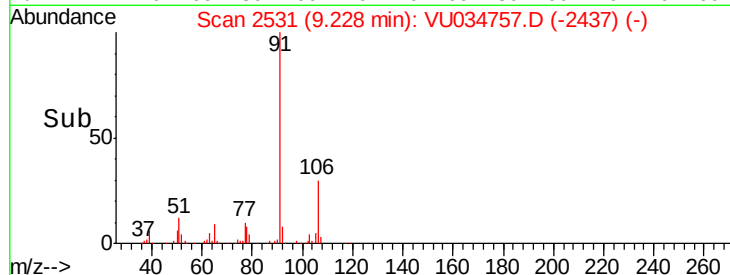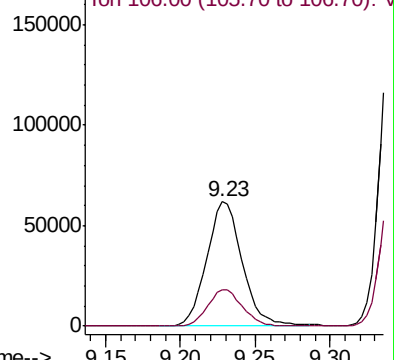

#53

m,p-Xylene

Concen: 34.619 ug/L

RT: 9.35 min Scan# 2569

Delta R.T. -0.00 min

Lab File: VU034757.D


Acq: 24 Sep 2019 00:50

Tgt Ion: 106 Resp: 252281



Ion Ratio Lower Upper


106 100

91 216.6 146.9 272.7

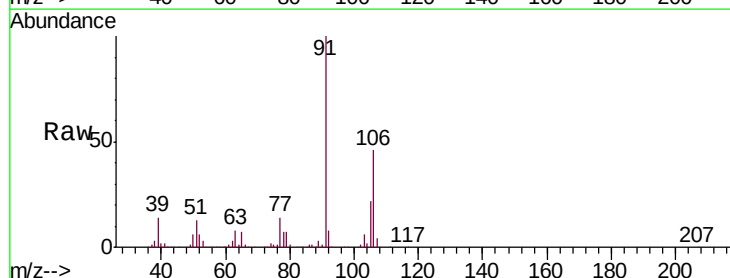

Abundance Ion 106.00 (105.70 to 106.70): VU034739.D (-2555) (-)



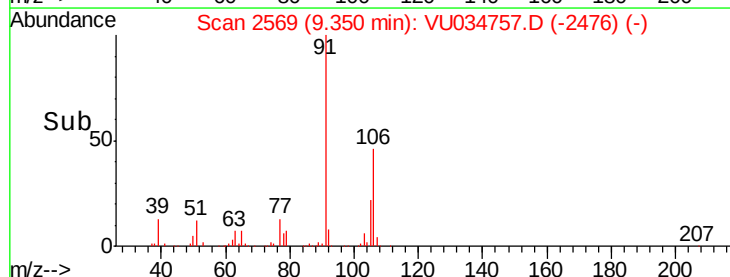
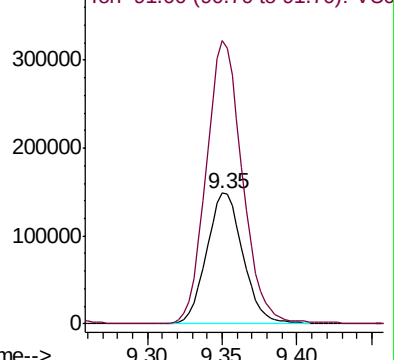


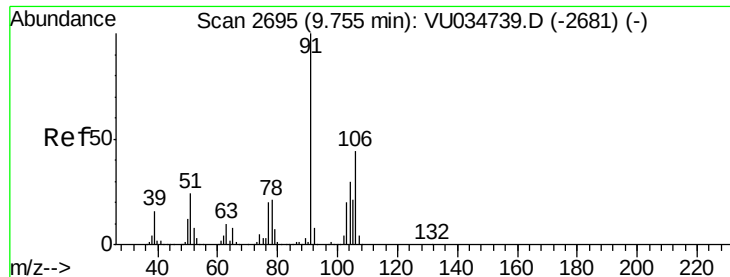

#54
o-xylene
Concen: 23.706 ug/L
RT: 9.76 min Scan# 2695
Delta R.T. -0.00 min
Lab File: VU034757.D
Acq: 24 Sep 2019 00:50




Instrument :
MSVOA_U
ClientSampleId :
BFDM5


Tgt Ion:106 Resp: 170867
Ion Ratio Lower Upper
106 100
91 229.5 155.6 289.0

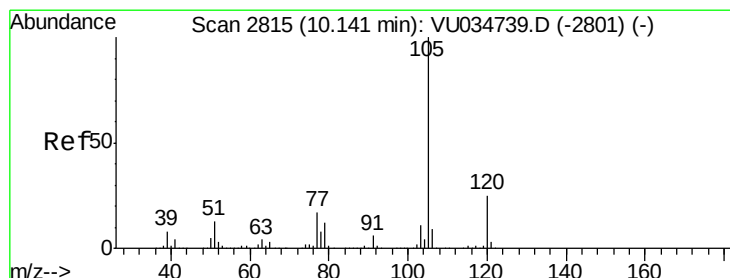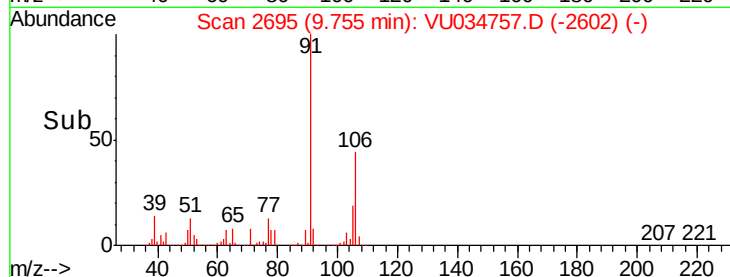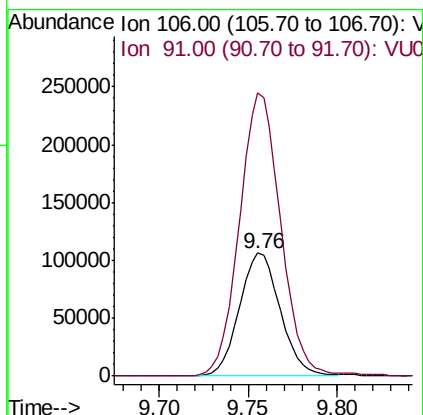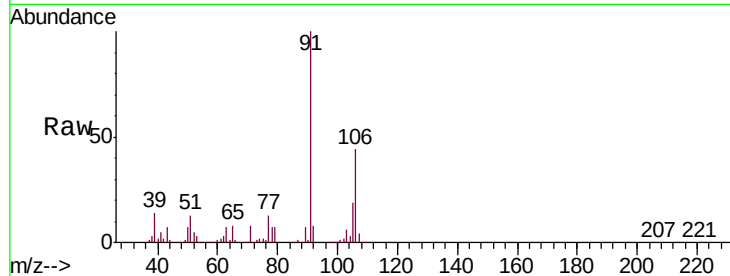

#56
Isopropylbenzene
Concen: 1.406 ug/L
RT: 10.14 min Scan# 2816
Delta R.T. 0.00 min
Lab File: VU034757.D
Acq: 24 Sep 2019 00:50

Tgt Ion:105 Resp: 27318
Ion Ratio Lower Upper
105 100
120 27.0 20.4 30.6
77 18.9 14.2 21.4


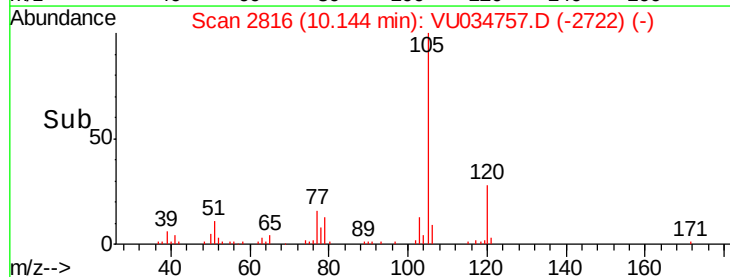
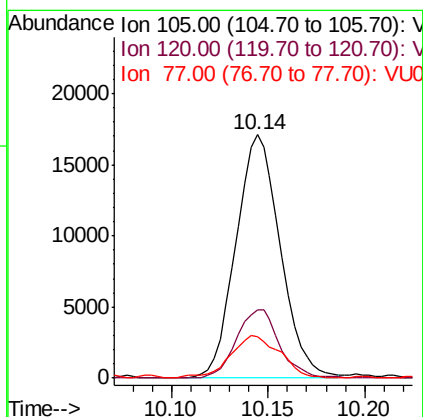
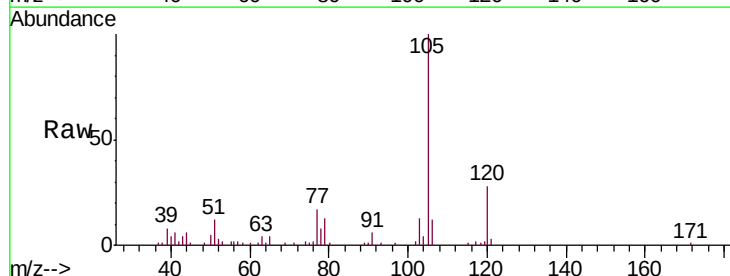


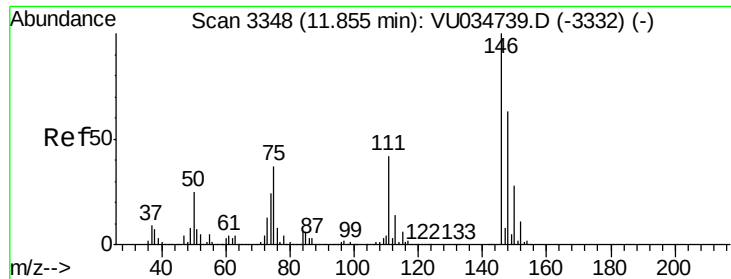

#65
 1,2-Dichlorobenzene
 Concen: 8.425 ug/L
 RT: 11.85 min Scan# 3348
 Delta R.T. -0.00 min
 Lab File: VU034757.D
 Acq: 24 Sep 2019 00:50

Instrument :
 MSVOA_U
 ClientSampled :
 BFDM5

Tgt Ion:146 Resp: 68546
 Ion Ratio Lower Upper
 146 100
 111 44.0 35.2 52.8
 148 64.4 53.0 79.6

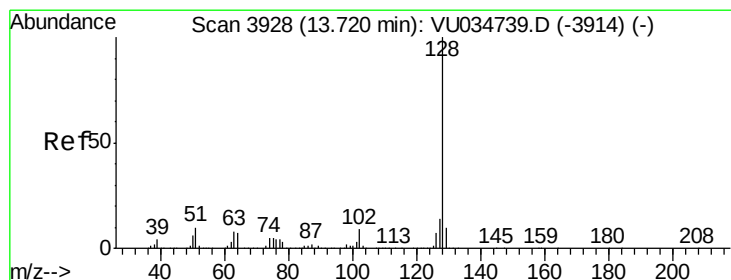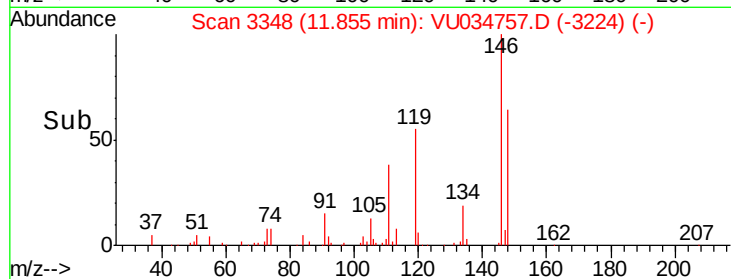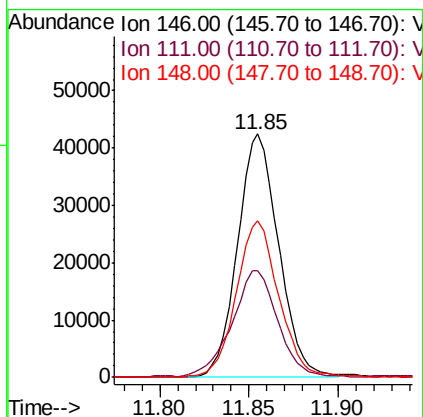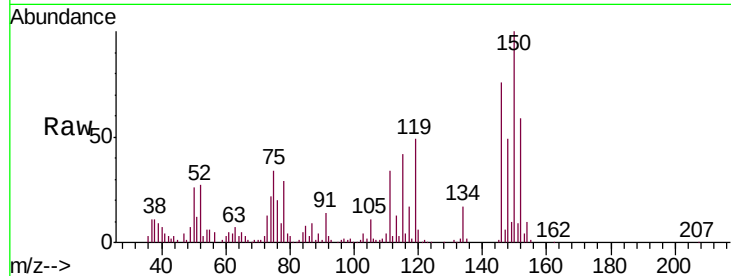

#69
 Naphthalene
 Concen: 27.666 ug/L
 RT: 13.72 min Scan# 3928
 Delta R.T. -0.00 min
 Lab File: VU034757.D
 Acq: 24 Sep 2019 00:50

Tgt Ion:128 Resp: 406366
 Ion Ratio Lower Upper
 128 100
 127 13.0 10.8 16.2
 129 10.7 8.6 12.8

