

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Quantitation Report (QT Reviewed)


Data File : VU034756.D
Acq On : 24 Sep 2019 00:27
Operator : JC/SP
Sample : K4932-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDK1

Manual Integrations
APPROVED

MMDadoda
9/24/2019 10:36:30 AM

Quant Time: Sep 24 05:47:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

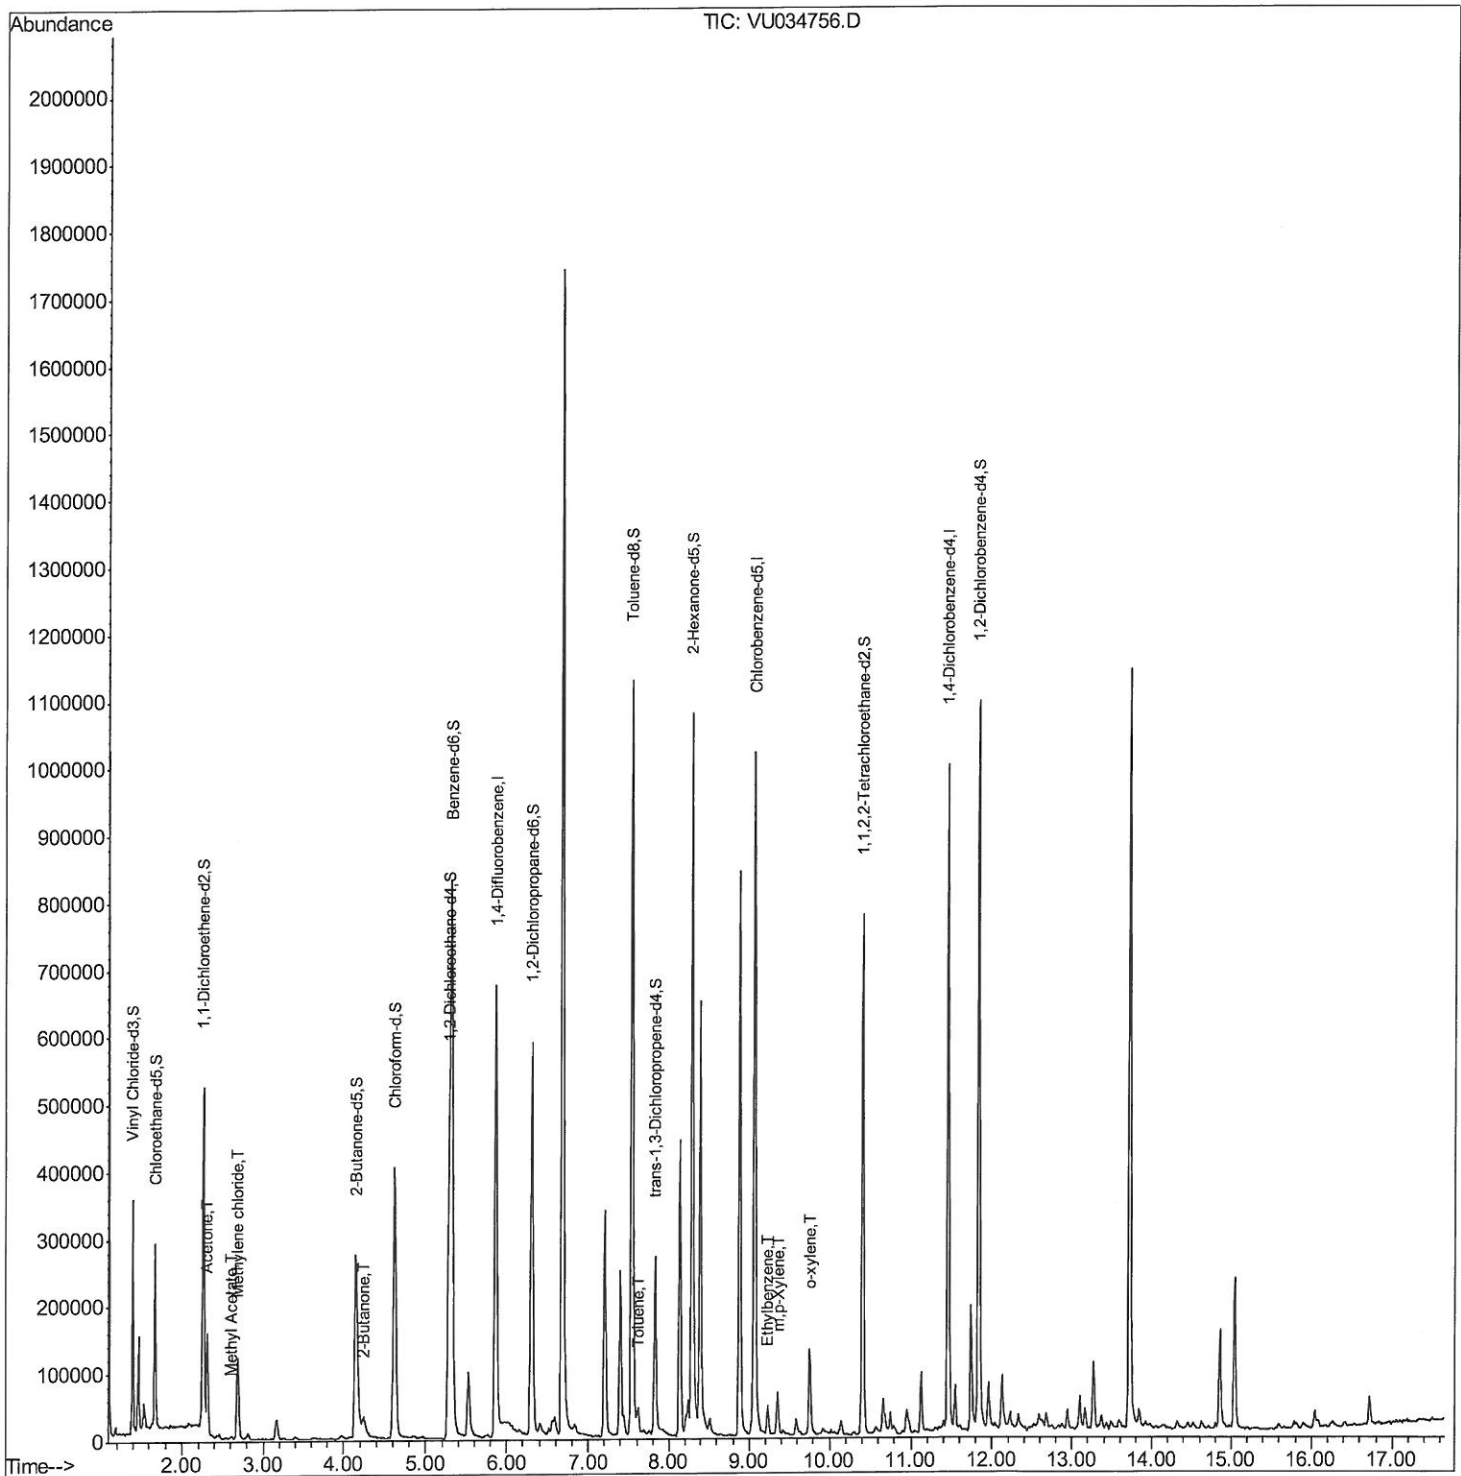

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Quantitation Report (Qedit)




Data File : VU034756.D
Acq On : 24 Sep 2019 00:27
Operator : JC/SP
Sample : K4932-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDK1

Manual Integrations
APPROVED

MMDadoda
9/24/2019 10:36:30 AM

Quant Time: Sep 24 03:43:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

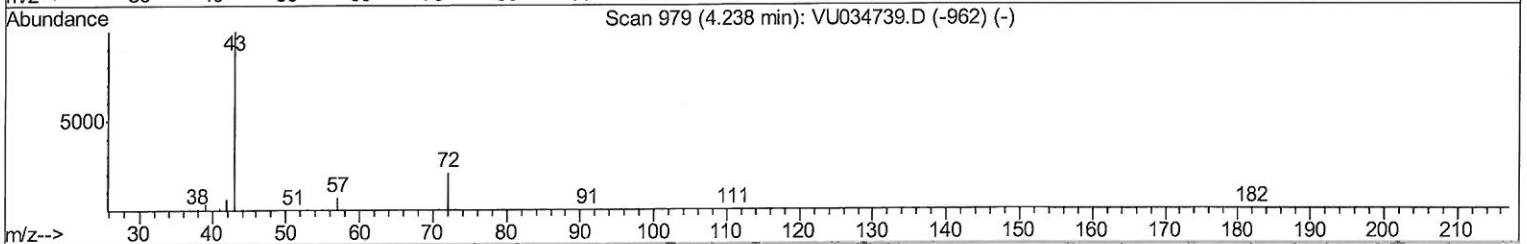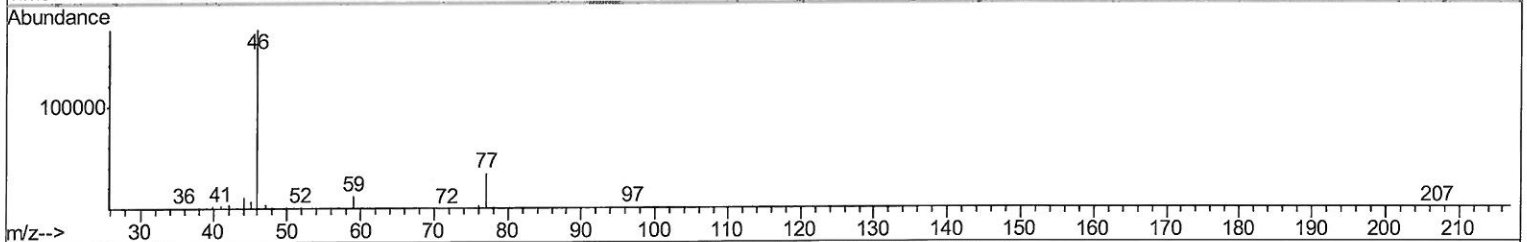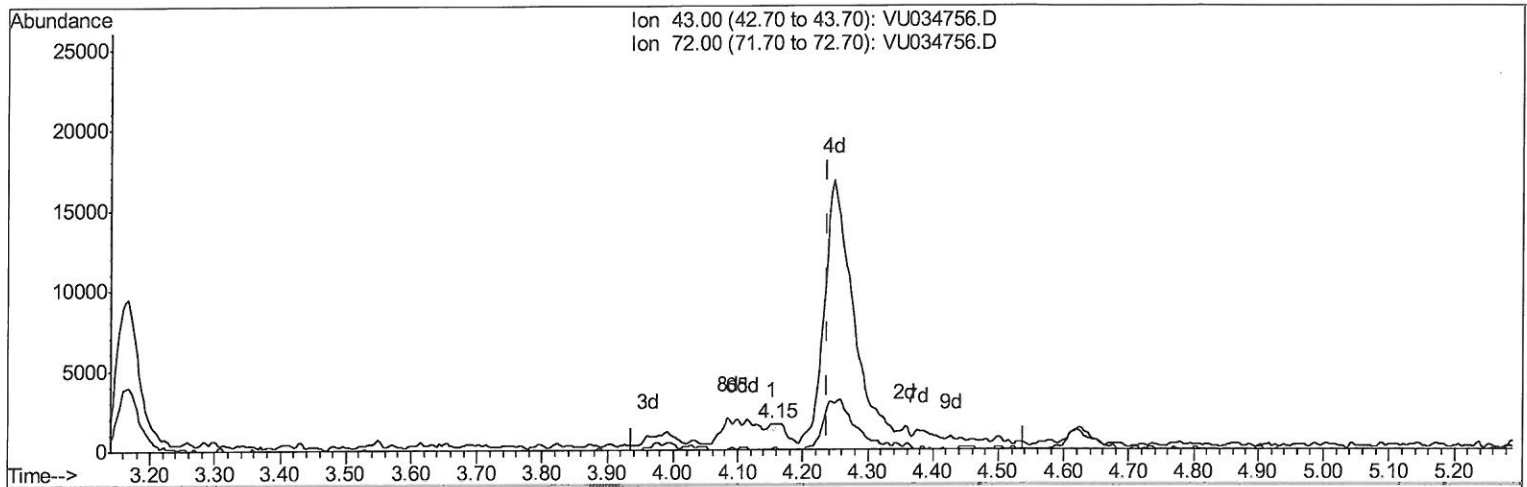

TIC: VU034756.D

(22) 2-Butanone (T)

4.154min (-0.084) 0.05ug/L

response 261

Ion	Exp%	Act%
43.00	100	100
72.00	20.40	26.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Quantitation Report (Qedit)




Data File : VU034756.D
Acq On : 24 Sep 2019 00:27
Operator : JC/SP
Sample : K4932-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDK1

Manual Integrations
APPROVED

MMDadoda
9/24/2019 10:36:30 AM

Quant Time: Sep 24 03:43:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

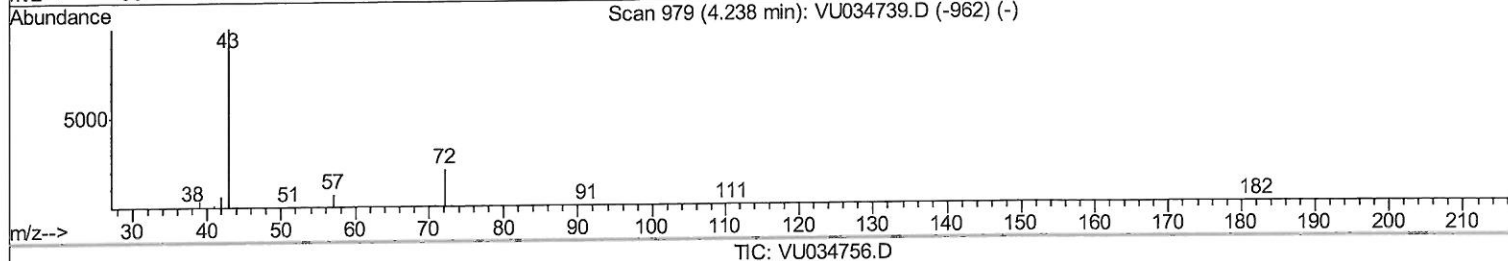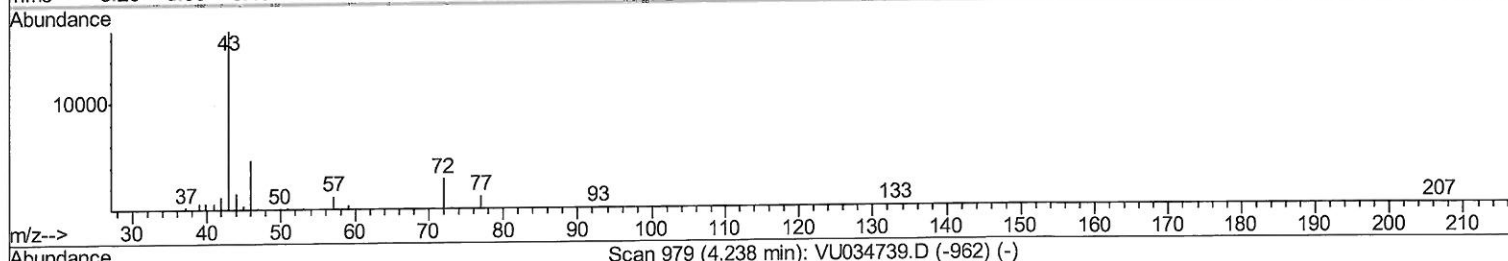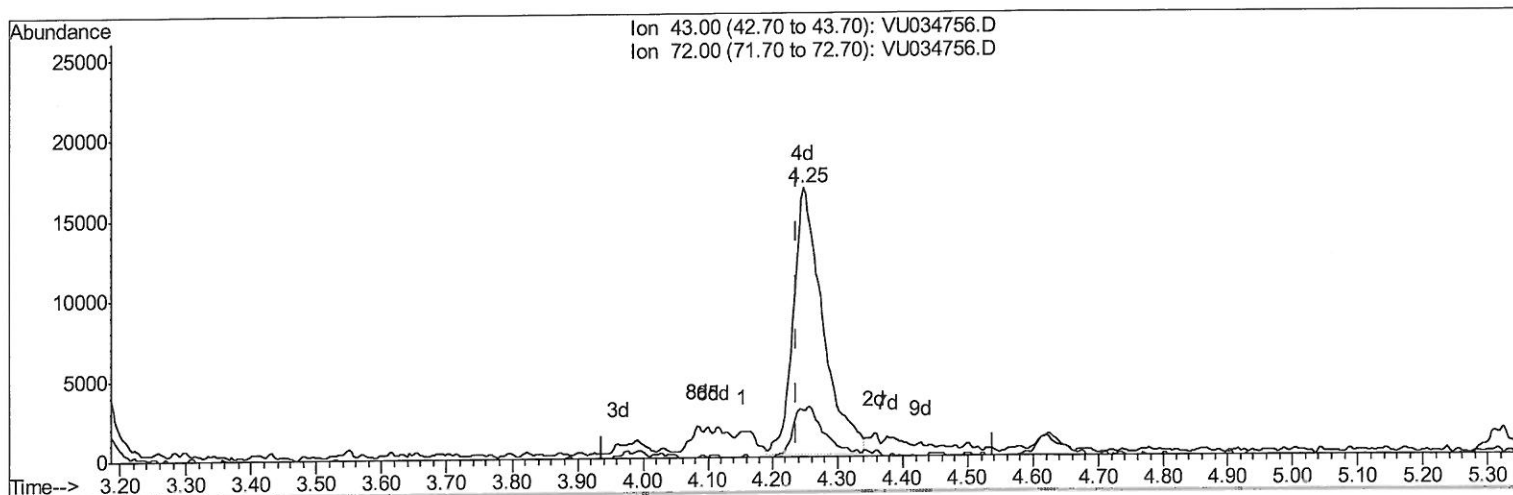

(22) 2-Butanone (T)

4.247min (+0.010) 9.28ug/L m

response 52992

Ion	Exp%	Act%
43.00	100	100
72.00	20.40	0.13#
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
10104119

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Quantitation Report (QT Reviewed)

Data File : VU034756.D
Acq On : 24 Sep 2019 00:27
Operator : JC/SP
Sample : K4932-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFDK1

Manual Integrations
APPROVED

MMDadoda
9/24/2019 10:36:30 AM

Quant Time: Sep 24 05:47:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:36:55 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.86	114	525954	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.07	117	490381	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.46	152	228412	50.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	1.39	65	213766	39.70	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.40%
7) Chloroethane-d5	1.67	69	171740	41.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	82.54%
11) 1,1-Dichloroethene-d2	2.26	63	295092	32.36	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.72%
21) 2-Butanone-d5	4.15	46	468514	113.53	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.53%
24) Chloroform-d	4.62	84	369218	47.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.34%
26) 1,2-Dichloroethane-d4	5.29	65	276022	47.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.94%
32) Benzene-d6	5.32	84	756646	49.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.56%
36) 1,2-Dichloropropane-d6	6.31	67	269120	50.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.32%
41) Toluene-d8	7.54	98	713861	49.37	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.74%
43) trans-1,3-Dichloropropene-	7.83	79	124794	49.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.10%
47) 2-Hexanone-d5	8.29	63	324435	121.59	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	121.59%
57) 1,1,2,2-Tetrachloroethane-	10.41	84	365504	49.58	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.16%
64) 1,2-Dichlorobenzene-d4	11.84	152	248178	51.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.64%

Target Compounds					Qvalue
13) Acetone	2.31	43	166436	34.672	ug/L 100
15) Methyl Acetate	2.61	43	7021	1.095	ug/L 95
16) Methylene chloride	2.68	84	47364	10.866	ug/L 95
22) 2-Butanone	4.25	43	52992m	9.279	ug/L 95
42) Toluene	7.62	91	25325	1.378	ug/L 94
52) Ethylbenzene	9.23	91	29516	1.426	ug/L 97
53) m,p-Xylene	9.35	106	16525	2.254	ug/L 98
54) o-xylene	9.76	106	18977	2.617	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed