

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034728.D
 Acq On : 23 Sep 2019 12:28
 Operator : JC/SP
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.177	23	27	31	rBV2	7245	6507	0.27%	0.036%
2	1.395	87	95	109	rBV	339412	362977	15.15%	2.017%
3	1.540	133	140	154	rVB2	38016	51123	2.13%	0.284%
4	1.672	174	181	200	rVB	271055	345848	14.43%	1.922%
5	2.257	354	363	386	rVB	507698	795465	33.19%	4.421%
6	2.688	489	497	506	rVB4	8135	14642	0.61%	0.081%
7	2.804	530	533	535	rBV3	2427	1286	0.05%	0.007%
8	3.048	606	609	612	rBV5	1457	1006	0.04%	0.006%
9	3.067	612	615	617	rBV3	1501	1013	0.04%	0.006%
10	3.254	670	673	676	rBV4	1325	856	0.04%	0.005%
11	3.472	736	741	745	rBV5	2002	1721	0.07%	0.010%
12	3.537	756	761	763	rBV3	1665	1266	0.05%	0.007%
13	3.572	769	772	775	rVV4	1226	1086	0.05%	0.006%
14	3.588	775	777	779	rVV3	1482	863	0.04%	0.005%
15	3.601	779	781	784	rVV4	1515	990	0.04%	0.006%
16	3.746	824	826	833	rVB6	1975	2026	0.08%	0.011%
17	3.894	865	872	874	rBV5	1130	1282	0.05%	0.007%
18	3.984	893	900	906	rVB9	1846	2373	0.10%	0.013%
19	4.022	906	912	915	rBV6	1853	1657	0.07%	0.009%
20	4.151	940	952	978	rBV	222212	586505	24.47%	3.259%
21	4.489	1055	1057	1061	rVB3	1510	736	0.03%	0.004%
22	4.624	1082	1099	1123	rBV2	364951	910531	37.99%	5.060%
23	5.077	1239	1240	1247	rVB6	1155	755	0.03%	0.004%
24	5.315	1290	1314	1345	rBV2	791032	2396518	100.00%	13.318%
25	5.733	1441	1444	1447	rBV3	2045	1192	0.05%	0.007%
26	5.749	1447	1449	1452	rVB3	1296	690	0.03%	0.004%
27	5.865	1472	1485	1513	rBV	631316	1270961	53.03%	7.063%
28	6.138	1567	1570	1571	rBV2	2265	1328	0.06%	0.007%
29	6.308	1605	1623	1645	rBV	538856	1123782	46.89%	6.245%
30	6.556	1698	1700	1705	rVB5	2013	1209	0.05%	0.007%
31	6.604	1713	1715	1719	rVB4	2158	1278	0.05%	0.007%
32	6.736	1752	1756	1757	rBV2	1750	1144	0.05%	0.006%
33	6.784	1769	1771	1777	rVB6	1721	1438	0.06%	0.008%
34	6.871	1793	1798	1801	rBV6	1086	869	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034728.D
 Acq On : 23 Sep 2019 12:28
 Operator : JC/SP
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	6.906	1805	1809	1813	rVV6	1061	914	0.04%	0.005%
36	6.929	1813	1816	1820	rVV4	1074	891	0.04%	0.005%
37	6.955	1820	1824	1829	rVB5	1942	1912	0.08%	0.011%
38	6.977	1829	1831	1834	rVB3	1781	848	0.04%	0.005%
39	6.996	1834	1837	1838	rBV3	1711	874	0.04%	0.005%
40	7.205	1890	1902	1928	rBV	322533	610499	25.47%	3.393%
41	7.440	1972	1975	1977	rBV4	2593	1732	0.07%	0.010%
42	7.543	1992	2007	2027	rBV	1082484	1921402	80.17%	10.678%
43	7.746	2066	2070	2073	rVB3	1706	1284	0.05%	0.007%
44	7.829	2086	2096	2121	rBV2	215933	402875	16.81%	2.239%
45	7.977	2138	2142	2148	rBV8	1781	1874	0.08%	0.010%
46	8.051	2162	2165	2170	rBV6	1550	1361	0.06%	0.008%
47	8.093	2174	2178	2180	rBV4	1448	958	0.04%	0.005%
48	8.212	2210	2215	2216	rBV3	3001	2176	0.09%	0.012%
49	8.289	2228	2239	2276	rBV	674097	1357004	56.62%	7.541%
50	8.521	2309	2311	2320	rVB9	2296	2570	0.11%	0.014%
51	8.562	2320	2324	2334	rBV9	2049	2399	0.10%	0.013%
52	8.684	2358	2362	2365	rBV5	1949	1149	0.05%	0.006%
53	8.733	2375	2377	2380	rBV3	1126	797	0.03%	0.004%
54	8.797	2393	2397	2398	rBV4	985	736	0.03%	0.004%
55	8.916	2428	2434	2438	rBV7	1526	1888	0.08%	0.010%
56	9.067	2469	2481	2508	rBV	929901	1606784	67.05%	8.929%
57	9.276	2543	2546	2551	rBV6	1274	1009	0.04%	0.006%
58	9.363	2567	2573	2581	rBV6	2850	4212	0.18%	0.023%
59	9.508	2616	2618	2624	rVB5	1271	766	0.03%	0.004%
60	9.578	2635	2640	2644	rVB7	1086	1080	0.05%	0.006%
61	9.758	2693	2696	2698	rBV4	1877	1456	0.06%	0.008%
62	9.781	2700	2703	2704	rBV3	1101	697	0.03%	0.004%
63	9.861	2725	2728	2731	rBV4	1288	967	0.04%	0.005%
64	9.977	2760	2764	2769	rVB4	1992	1626	0.07%	0.009%
65	10.016	2772	2776	2779	rBV3	1397	1002	0.04%	0.006%
66	10.035	2779	2782	2783	rBV	1200	703	0.03%	0.004%
67	10.080	2792	2796	2800	rVB6	916	816	0.03%	0.005%
68	10.138	2811	2814	2824	rBV6	2311	2872	0.12%	0.016%
69	10.218	2835	2839	2843	rVB5	1011	1025	0.04%	0.006%
70	10.247	2843	2848	2852	rBV6	1272	1301	0.05%	0.007%
71	10.334	2873	2875	2878	rBV3	1614	1298	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034728.D
 Acq On : 23 Sep 2019 12:28
 Operator : JC/SP
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.408	2886	2898	2925	rBV	691821	1142841	47.69%	6.351%
73	10.582	2948	2952	2957	rBV6	1833	1797	0.07%	0.010%
74	10.646	2968	2972	2975	rBV6	1285	956	0.04%	0.005%
75	10.700	2985	2989	2991	rBV4	1326	733	0.03%	0.004%
76	10.717	2991	2994	2997	rVB3	1631	973	0.04%	0.005%
77	10.752	3000	3005	3010	rBV8	3890	4347	0.18%	0.024%
78	10.987	3076	3078	3082	rVB5	1607	866	0.04%	0.005%
79	11.012	3082	3086	3090	rBV7	944	817	0.03%	0.005%
80	11.064	3097	3102	3107	rVB7	2716	2854	0.12%	0.016%
81	11.128	3116	3122	3132	rBV8	3964	5659	0.24%	0.031%
82	11.289	3168	3172	3173	rBV3	1107	898	0.04%	0.005%
83	11.382	3196	3201	3203	rBV3	2016	1884	0.08%	0.010%
84	11.463	3214	3226	3247	rBV	838670	1409416	58.81%	7.833%
85	11.839	3330	3343	3366	rBV	911399	1567400	65.40%	8.711%
86	12.253	3469	3472	3477	rBV6	1755	1783	0.07%	0.010%
87	12.524	3554	3556	3558	rBV3	1590	799	0.03%	0.004%
88	12.614	3581	3584	3587	rBV3	1126	866	0.04%	0.005%
89	12.639	3590	3592	3594	rVV2	1651	669	0.03%	0.004%
90	12.694	3606	3609	3611	rBV3	1544	1006	0.04%	0.006%
91	12.707	3611	3613	3616	rVB3	1672	897	0.04%	0.005%
92	12.852	3654	3658	3659	rBV3	1435	1086	0.05%	0.006%
93	12.980	3696	3698	3701	rVB4	1703	859	0.04%	0.005%
94	12.999	3701	3704	3707	rVB4	1401	899	0.04%	0.005%
95	13.102	3732	3736	3740	rBV5	1731	1691	0.07%	0.009%
96	13.334	3805	3808	3810	rBV3	1840	1057	0.04%	0.006%
97	13.639	3900	3903	3906	rBV4	1955	1307	0.05%	0.007%
98	13.967	4003	4005	4007	rBV3	2091	1253	0.05%	0.007%
99	14.376	4129	4132	4134	rBV3	1322	882	0.04%	0.005%
100	14.806	4263	4266	4268	rBV4	1589	1013	0.04%	0.006%


Sum of corrected areas: 17994188

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092319\
Data File : VU034728.D
Acq On : 23 Sep 2019 12:28
Operator : JC/SP
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

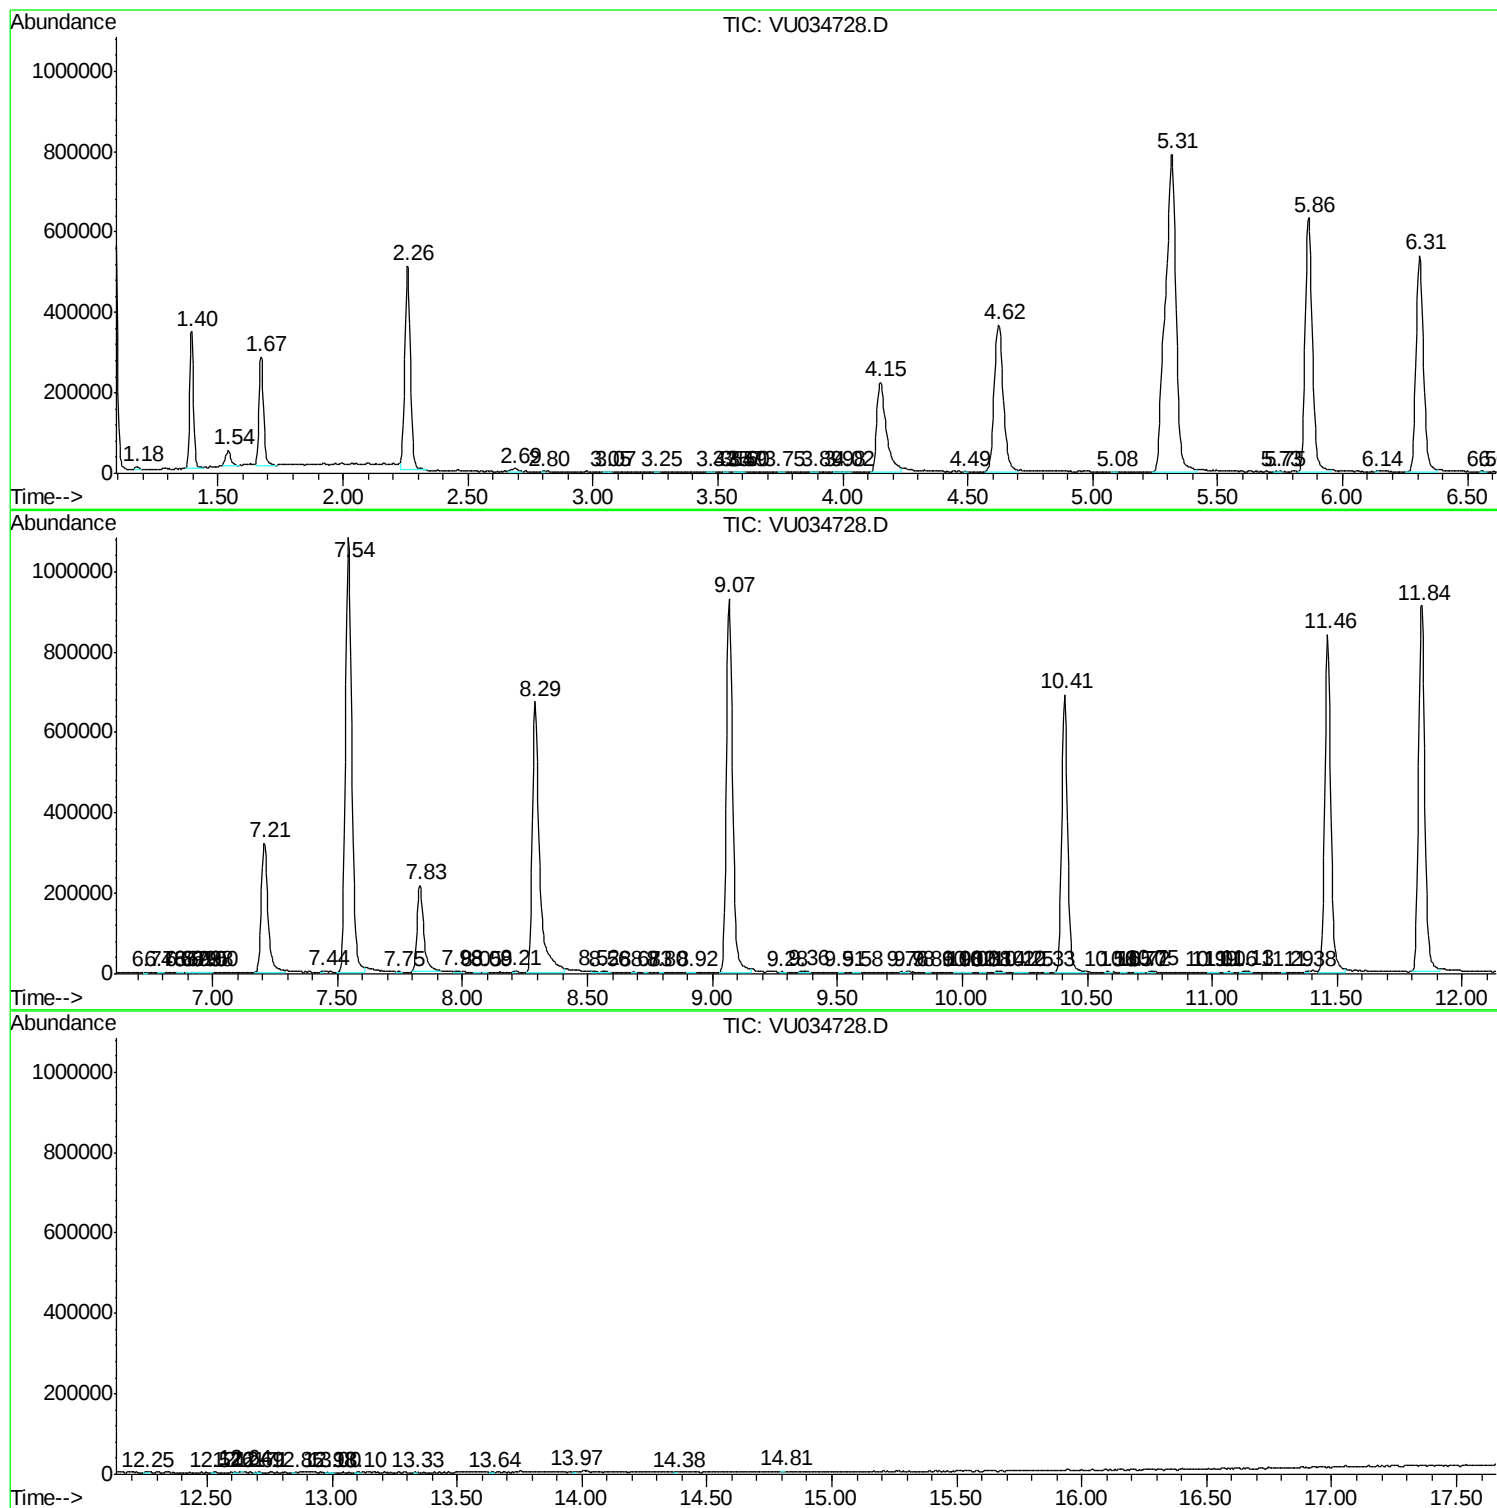

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Data File : VU034728.D
Acq On : 23 Sep 2019 12:28
Operator : JC/SP
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Data File : VU034728.D
Acq On : 23 Sep 2019 12:28
Operator : JC/SP
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK36

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc