

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034740.D
 Acq On : 23 Sep 2019 18:11
 Operator : JC/SP
 Sample : VU0923WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	87	94	105	rBV	353892	356107	15.48%	2.018%
2	1.543	135	141	148	rVB3	34513	43883	1.91%	0.249%
3	1.669	173	180	195	rVB	254837	331072	14.40%	1.876%
4	2.257	354	363	384	rVB	489613	751358	32.67%	4.258%
5	2.354	391	393	396	rBV4	2179	1278	0.06%	0.007%
6	2.485	432	434	438	rVB5	1760	1191	0.05%	0.007%
7	2.566	457	459	461	rBV3	1245	730	0.03%	0.004%
8	2.746	513	515	519	rBV4	1076	752	0.03%	0.004%
9	2.794	529	530	534	rBV4	1038	800	0.03%	0.005%
10	2.829	539	541	544	rBV2	1696	1131	0.05%	0.006%
11	2.907	562	565	569	rVB5	2073	1267	0.06%	0.007%
12	2.955	575	580	584	rBV6	2073	2545	0.11%	0.014%
13	3.022	599	601	608	rBV5	1647	1293	0.06%	0.007%
14	3.151	638	641	643	rBV4	1233	741	0.03%	0.004%
15	3.167	643	646	650	rBV4	1438	1061	0.05%	0.006%
16	3.212	658	660	665	rVB4	1940	1267	0.06%	0.007%
17	3.328	694	696	703	rBV6	1063	1095	0.05%	0.006%
18	3.357	703	705	709	rBV3	996	817	0.04%	0.005%
19	3.440	724	731	732	rBV5	1108	1026	0.04%	0.006%
20	3.579	771	774	778	rVB4	1427	1078	0.05%	0.006%
21	3.601	778	781	783	rBV3	1430	895	0.04%	0.005%
22	3.678	798	805	807	rBV5	1753	1708	0.07%	0.010%
23	3.836	849	854	857	rBV5	1539	934	0.04%	0.005%
24	3.952	887	890	894	rVB3	1267	991	0.04%	0.006%
25	3.981	898	899	905	rVB5	1536	1326	0.06%	0.008%
26	4.019	909	911	915	rVB4	1578	957	0.04%	0.005%
27	4.048	915	920	921	rBV3	1506	1413	0.06%	0.008%
28	4.106	935	938	941	rBV4	1683	1282	0.06%	0.007%
29	4.151	941	952	982	rBV	220734	615974	26.78%	3.490%
30	4.537	1067	1072	1076	rBV4	1228	1201	0.05%	0.007%
31	4.624	1084	1099	1121	rBV2	336833	859182	37.36%	4.869%
32	4.762	1138	1142	1145	rBV4	1616	1566	0.07%	0.009%
33	4.907	1185	1187	1192	rVB5	1423	1001	0.04%	0.006%
34	5.051	1228	1232	1237	rBV8	2590	1875	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034740.D
 Acq On : 23 Sep 2019 18:11
 Operator : JC/SP
 Sample : VU0923WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

35	5.083	1240	1242	1248	rVB7	1973	1388	0.06%	0.008%
36	5.106	1248	1249	1254	rBV4	1090	942	0.04%	0.005%
37	5.315	1291	1314	1339	rBV2	778297	2299747	100.00%	13.032%
38	5.701	1430	1434	1436	rBV4	1546	1158	0.05%	0.007%
39	5.862	1470	1484	1510	rBV	634688	1274459	55.42%	7.222%
40	6.064	1545	1547	1551	rVB5	1696	1128	0.05%	0.006%
41	6.308	1607	1623	1643	rBV	535079	1092316	47.50%	6.190%
42	6.460	1667	1670	1674	rVB4	2156	1535	0.07%	0.009%
43	6.669	1733	1735	1738	rVB3	1436	794	0.03%	0.004%
44	6.858	1790	1794	1796	rVB5	1433	1037	0.05%	0.006%
45	7.000	1833	1838	1840	rVB3	950	814	0.04%	0.005%
46	7.164	1886	1889	1890	rBV3	1620	766	0.03%	0.004%
47	7.206	1890	1902	1928	rVV	308334	582439	25.33%	3.300%
48	7.543	1992	2007	2025	rBV	1057173	1857266	80.76%	10.524%
49	7.829	2084	2096	2114	rBV2	207938	382521	16.63%	2.168%
50	8.157	2191	2198	2200	rBV7	1973	2292	0.10%	0.013%
51	8.183	2204	2206	2209	rVB3	1639	848	0.04%	0.005%
52	8.202	2209	2212	2214	rBV4	1675	1069	0.05%	0.006%
53	8.289	2228	2239	2279	rBV	705629	1397624	60.77%	7.920%
54	8.787	2390	2394	2395	rBV4	1230	827	0.04%	0.005%
55	8.842	2409	2411	2414	rVB4	1289	872	0.04%	0.005%
56	8.903	2423	2430	2434	rBV7	1646	1978	0.09%	0.011%
57	8.945	2437	2443	2445	rBV6	1084	1061	0.05%	0.006%
58	8.968	2447	2450	2453	rVB4	1251	819	0.04%	0.005%
59	9.067	2468	2481	2502	rBV	929057	1587787	69.04%	8.997%
60	9.228	2528	2531	2535	rBV7	2315	2356	0.10%	0.013%
61	9.289	2546	2550	2553	rBV5	1482	970	0.04%	0.005%
62	9.315	2555	2558	2564	rVB7	1612	961	0.04%	0.005%
63	9.357	2564	2571	2576	rBV7	2658	3605	0.16%	0.020%
64	9.427	2587	2593	2597	rVB8	1633	1945	0.08%	0.011%
65	9.469	2604	2606	2610	rVB4	1649	815	0.04%	0.005%
66	9.704	2677	2679	2681	rBV3	1414	828	0.04%	0.005%
67	9.755	2691	2695	2697	rVB4	1322	750	0.03%	0.004%
68	9.775	2697	2701	2706	rBV8	1716	1713	0.07%	0.010%
69	9.948	2752	2755	2759	rBV4	1052	735	0.03%	0.004%
70	10.131	2806	2812	2813	rBV5	1348	1416	0.06%	0.008%
71	10.154	2813	2819	2824	rVV9	2868	4191	0.18%	0.024%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034740.D
 Acq On : 23 Sep 2019 18:11
 Operator : JC/SP
 Sample : VU0923WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK38

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis

72	10.305	2863	2866	2870	rVB3	1472	1055	0.05%	0.006%
73	10.331	2870	2874	2876	rBV3	1405	1040	0.05%	0.006%
74	10.408	2884	2898	2922	rBV	677601	1112293	48.37%	6.303%
75	10.495	2922	2925	2929	rVB5	3392	2406	0.10%	0.014%
76	10.553	2939	2943	2944	rBV3	1598	925	0.04%	0.005%
77	10.562	2944	2946	2951	rVV5	1426	1109	0.05%	0.006%
78	10.633	2966	2968	2974	rVB5	1451	1369	0.06%	0.008%
79	10.701	2986	2989	2995	rVB6	1522	1392	0.06%	0.008%
80	10.794	3013	3018	3029	rVB8	3556	5833	0.25%	0.033%
81	10.842	3029	3033	3035	rVB3	1178	796	0.03%	0.005%
82	10.942	3062	3064	3066	rVB3	1853	801	0.03%	0.005%
83	11.077	3103	3106	3109	rBV3	1616	800	0.03%	0.005%
84	11.276	3165	3168	3172	rBV6	1568	1172	0.05%	0.007%
85	11.318	3178	3181	3185	rVB4	1622	1035	0.05%	0.006%
86	11.350	3188	3191	3194	rBV3	1628	1220	0.05%	0.007%
87	11.405	3201	3208	3214	rBV8	5259	6987	0.30%	0.040%
88	11.459	3214	3225	3247	rBV	875393	1442714	62.73%	8.175%
89	11.836	3330	3342	3366	rBV	906120	1543373	67.11%	8.746%
90	12.270	3475	3477	3483	rBV7	1218	1121	0.05%	0.006%
91	12.331	3493	3496	3498	rBV4	1492	926	0.04%	0.005%
92	12.408	3517	3520	3522	rBV3	2380	1443	0.06%	0.008%
93	12.443	3528	3531	3534	rBV3	2947	2367	0.10%	0.013%
94	12.578	3570	3573	3576	rVB5	1081	770	0.03%	0.004%
95	12.881	3663	3667	3671	rBV7	2414	2343	0.10%	0.013%
96	13.286	3790	3793	3794	rBV3	1445	769	0.03%	0.004%
97	13.389	3822	3825	3828	rBV4	1699	1039	0.05%	0.006%
98	13.659	3907	3909	3913	rVB3	2292	1406	0.06%	0.008%
99	13.684	3914	3917	3920	rVV5	1647	1053	0.05%	0.006%
100	14.218	4080	4083	4090	rBV7	2574	3163	0.14%	0.018%


Sum of corrected areas: 17647289

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092319\
Data File : VU034740.D
Acq On : 23 Sep 2019 18:11
Operator : JC/SP
Sample : VU0923WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK38

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

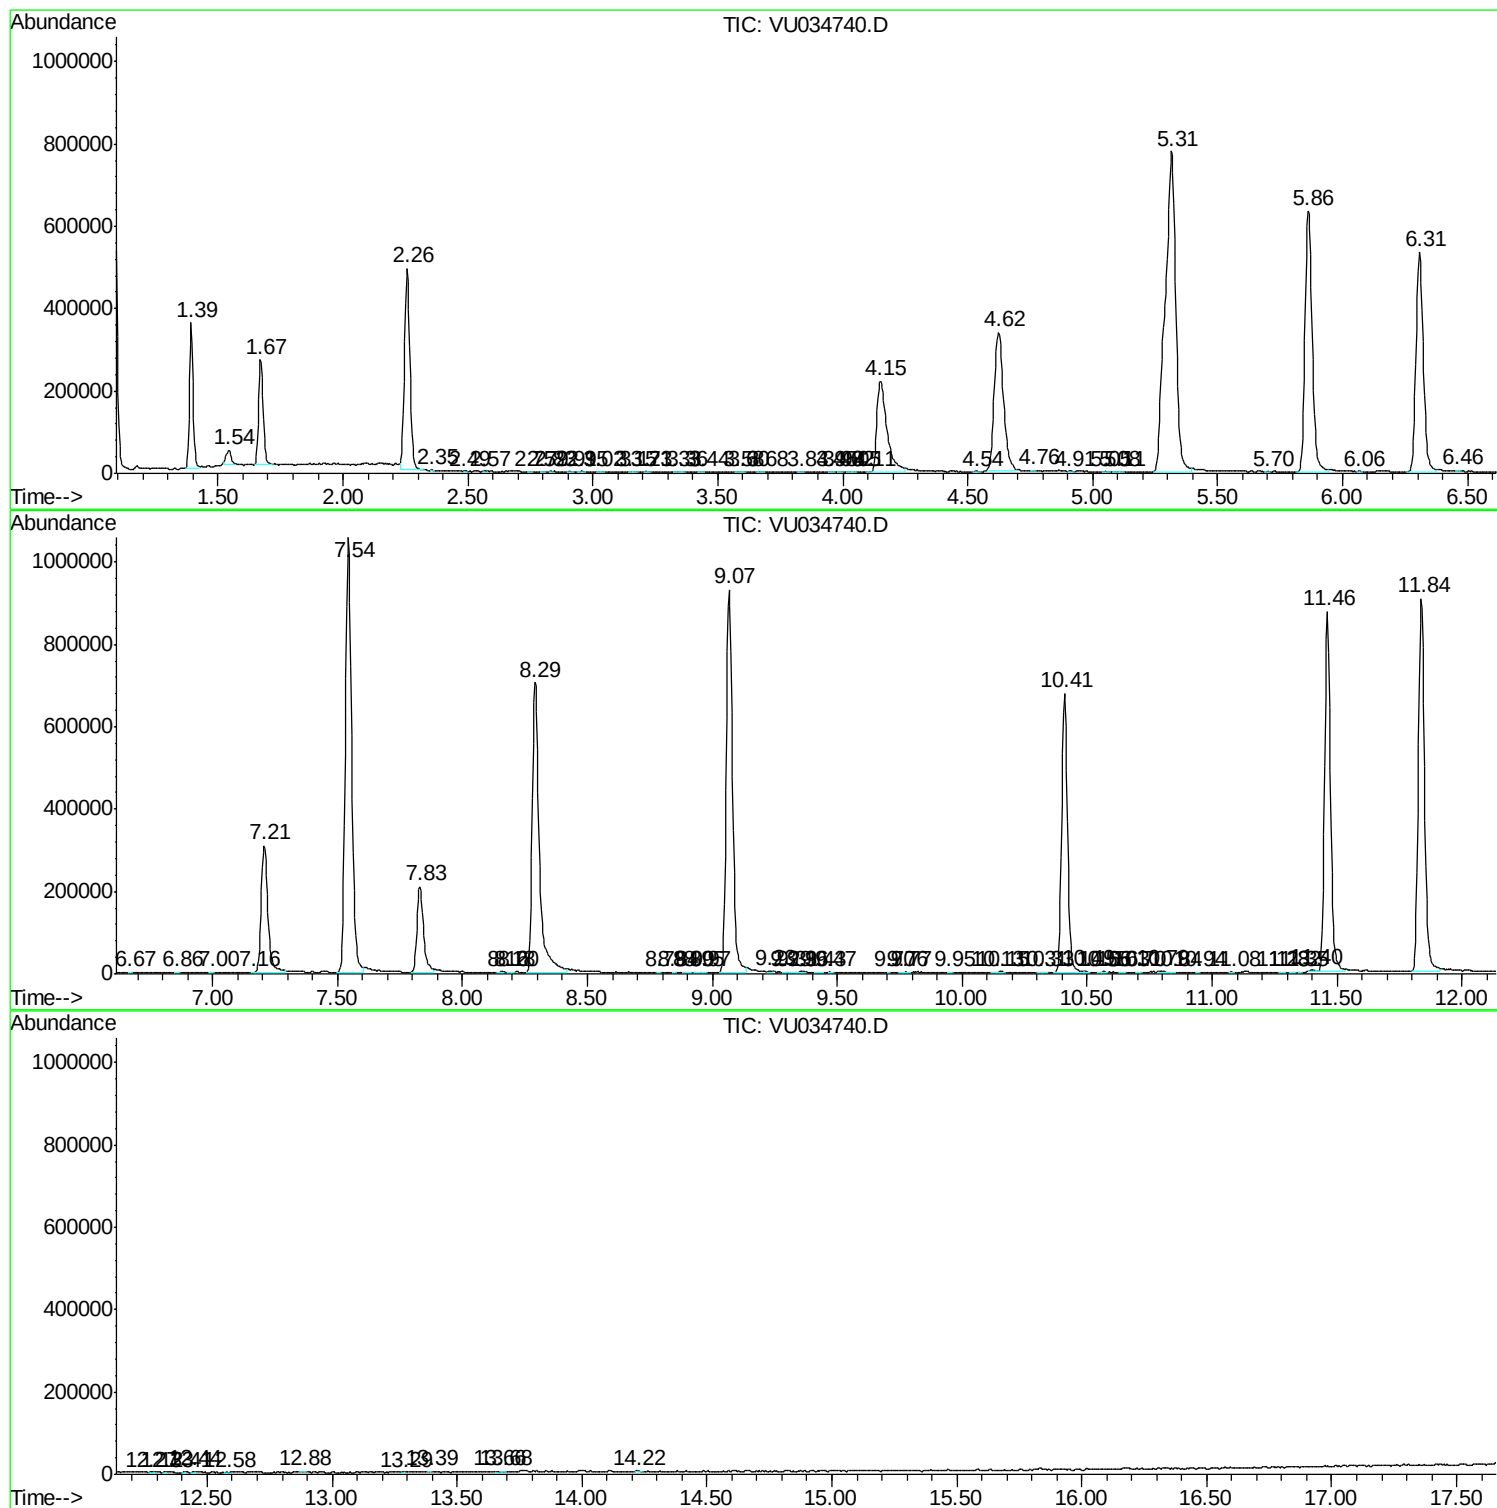

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Data File : VU034740.D
Acq On : 23 Sep 2019 18:11
Operator : JC/SP
Sample : VU0923WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK38

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092319\
Data File : VU034740.D
Acq On : 23 Sep 2019 18:11
Operator : JC/SP
Sample : VU0923WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK38

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc