


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092319\
 Data File : VU034726.D
 Acq On : 23 Sep 2019 09:25
 Operator : JC/SP
 Sample : BFB36
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 25 08:01:52 2019

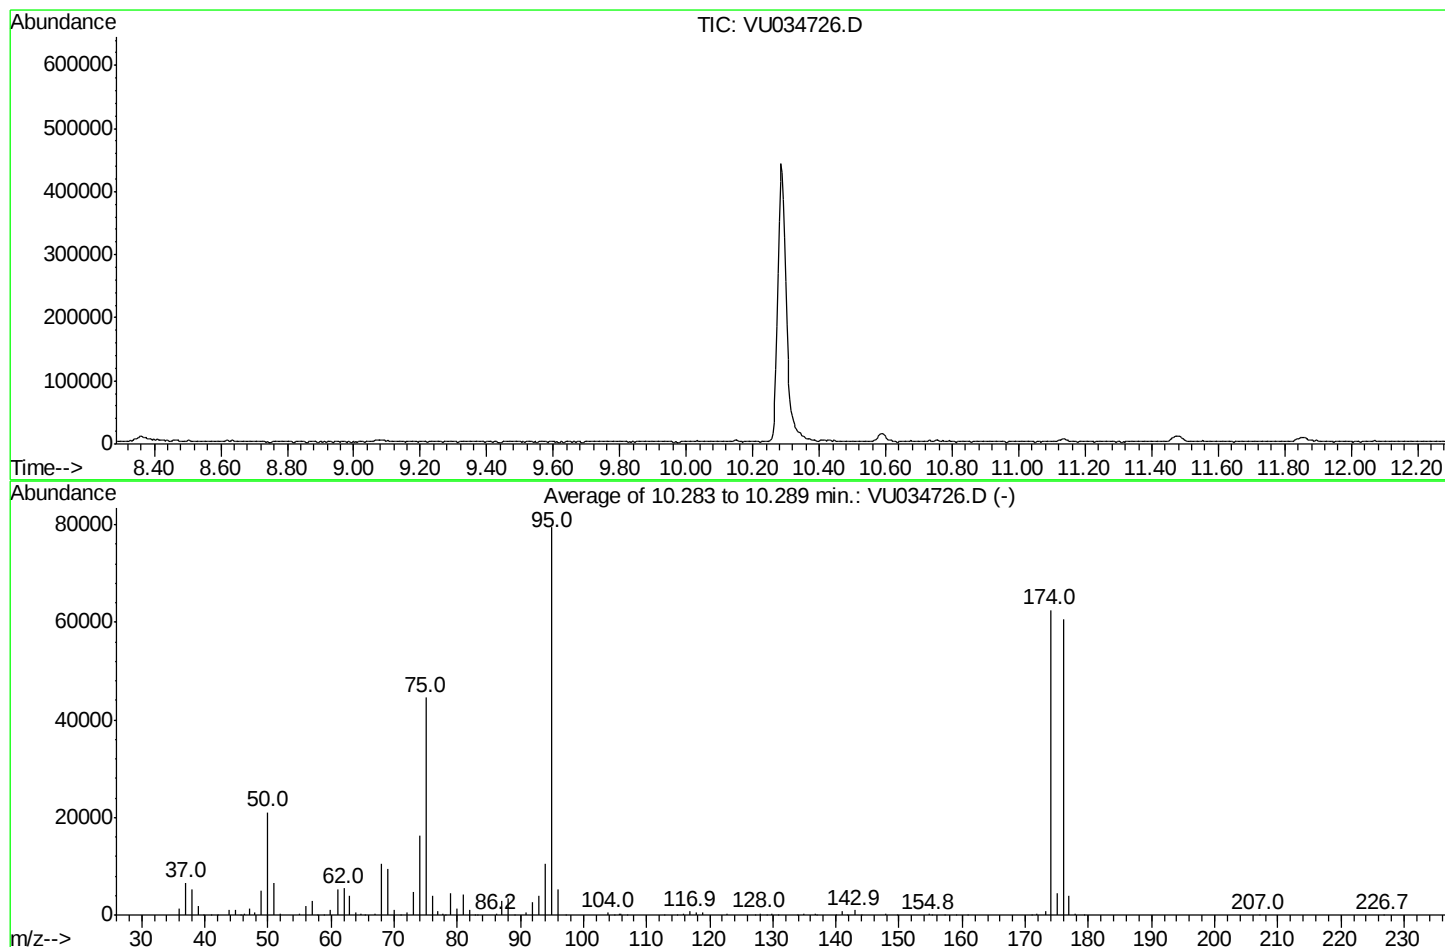

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.6	21138	PASS
75	95	30	80	56.0	44549	PASS
95	95	100	100	100.0	79498	PASS
96	95	5	9	6.6	5211	PASS
173	174	0.00	2	1.4	848	PASS
174	95	50	120	78.6	62501	PASS
175	174	5	9	7.2	4514	PASS
176	174	95	101	97.1	60666	PASS
177	176	5	9	6.5	3927	PASS

Scan 2847 (10.244 min): VU034726.D
BFB36

m/z	Abundance
38.10	123.0
39.10	269.0
39.80	392.0
41.00	324.0
42.00	100.0
42.80	238.0
43.30	260.0
43.90	789.0
44.90	115.0
47.00	101.0
53.90	133.0
54.90	217.0
55.90	183.0
69.10	147.0
70.20	119.0
82.80	106.0
101.80	103.0
207.00	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1325.0
37.00	6671.0
37.90	5262.0
39.00	2100.0
39.90	365.0
41.00	283.0
42.80	123.0
43.90	1608.0
45.00	1009.0
46.30	168.0
47.00	1163.0
48.00	585.0
49.00	5015.0
50.00	20696.0
51.00	6018.0
51.90	401.0
54.10	127.0
55.00	601.0
56.00	1833.0
57.00	2944.0
57.80	104.0
60.00	781.0
61.00	4916.0
62.00	5038.0
63.00	3889.0
64.00	448.0
64.70	279.0
67.00	409.0
68.00	10206.0
69.00	9891.0
70.00	1032.0
71.10	128.0
72.00	566.0
73.00	4534.0
74.00	15780.0
75.00	44168.0
76.00	3631.0
76.90	647.0
78.10	274.0
78.90	4344.0
79.90	1384.0
80.90	4004.0
81.90	964.0
82.80	253.0
86.10	220.0
87.00	2864.0
88.00	3015.0
90.90	470.0
91.90	3058.0
93.00	3971.0
94.00	10637.0
95.00	76440.0
96.00	5207.0
97.10	114.0
103.90	522.0
105.70	455.0
106.90	109.0
115.90	386.0
116.90	588.0
117.90	344.0
118.90	599.0
122.80	212.0
127.90	341.0
129.90	241.0
130.90	173.0
133.80	108.0
134.90	175.0
136.70	195.0
140.00	127.0
140.90	850.0
143.00	918.0
144.10	114.0
147.80	113.0
154.70	190.0
155.10	122.0
157.10	113.0
159.00	131.0
170.90	183.0
171.90	292.0
173.10	1240.0
174.00	59024.0
175.00	4701.0
176.00	57496.0
176.90	3898.0
177.90	201.0
207.00	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1315.0
37.00	6879.0
38.00	5574.0
39.00	2153.0
39.90	451.0
41.00	344.0
42.10	162.0
43.90	1794.0
45.00	1204.0
46.30	219.0
47.00	1363.0
47.90	639.0
49.00	5179.0
50.00	21880.0
51.00	6815.0
51.90	269.0
55.00	560.0
56.10	1963.0
56.90	3123.0
58.90	117.0
59.90	1025.0
61.00	5302.0
62.00	5604.0
63.00	4178.0
64.00	515.0
64.70	214.0
65.40	103.0
67.00	380.0
68.00	10921.0
69.00	9629.0
70.00	1175.0
72.00	583.0
73.00	4834.0
74.00	16872.0
75.00	45744.0
76.00	4134.0
76.90	774.0
77.80	353.0
78.90	4626.0
79.90	1431.0
80.90	4326.0
82.00	1016.0
82.80	243.0
83.20	200.0
86.20	210.0
87.00	2915.0
88.00	3515.0
89.00	100.0
90.90	551.0
91.90	2742.0
93.00	4006.0
94.00	10813.0
95.00	81752.0
96.00	5380.0
97.10	127.0
104.00	506.0
105.90	489.0
112.80	161.0
115.80	341.0
116.90	711.0
117.90	467.0
118.80	582.0
122.80	200.0
127.20	102.0
128.00	331.0
128.90	142.0
129.90	307.0
130.90	153.0
135.00	165.0
136.80	232.0
140.10	133.0
140.90	928.0
141.80	112.0
142.90	918.0
144.10	151.0
147.80	173.0
149.70	105.0
154.70	203.0
155.10	156.0
157.10	125.0
159.00	131.0
160.90	132.0
170.90	159.0
171.90	252.0
173.20	1305.0
174.00	64520.0
175.00	4579.0
176.00	62808.0
176.90	4088.0
177.90	254.0
207.00	229.0
226.70	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1103.0
37.00	6507.0
38.00	5568.0
39.00	2121.0
39.90	499.0
41.00	353.0
42.10	211.0
42.70	128.0
44.00	1913.0
45.00	1354.0
45.70	124.0
46.30	176.0
47.00	1363.0
47.90	613.0
49.00	5012.0
50.00	20840.0
51.00	6638.0
51.90	164.0
55.00	500.0
56.10	2051.0
56.90	3009.0
58.90	109.0
59.90	1138.0
61.00	5282.0
62.00	5545.0
63.00	4116.0
64.00	509.0
65.40	153.0
66.90	354.0
68.00	10503.0
69.00	8996.0
70.00	1056.0
72.00	545.0
73.00	4570.0
74.00	16400.0
75.00	43736.0
76.00	4413.0
77.00	771.0
77.80	391.0
78.90	4367.0
79.90	1275.0
81.00	4046.0
82.00	1037.0
82.80	203.0
83.10	189.0
86.20	176.0
87.00	2762.0
88.00	3373.0
89.00	132.0
90.90	542.0
92.00	2481.0
93.00	3757.0
94.00	9883.0
95.00	80304.0
96.00	5047.0
97.10	133.0
104.00	441.0
104.90	128.0
106.00	523.0
106.80	132.0
112.80	189.0
114.80	106.0
115.80	223.0
116.90	752.0
117.90	465.0
118.80	494.0
122.80	142.0
127.20	109.0
128.00	276.0
129.00	202.0
129.90	391.0
135.00	168.0
137.00	250.0
140.90	916.0
141.90	121.0
142.90	971.0
144.10	133.0
147.80	189.0
149.70	131.0
154.80	182.0
157.10	141.0
160.90	190.0
171.90	221.0
174.00	63960.0
175.00	4262.0
176.00	61696.0
176.90	3797.0
177.90	199.0
179.30	129.0
207.00	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36