

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044794.D
Acq On : 23 Sep 2021 18:57
Operator : SY/MD
Sample : M3876-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1




Instrument :
MSVOA_U
ClientSampleId :
EW7Z1

Manual Integrations
APPROVED

MMDadoda
9/24/2021 11:02:43 AM

Quant Time: Sep 24 05:39:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 24 05:26:38 2021
Response via : Initial Calibration

9/24/2021 11:02:43 AM

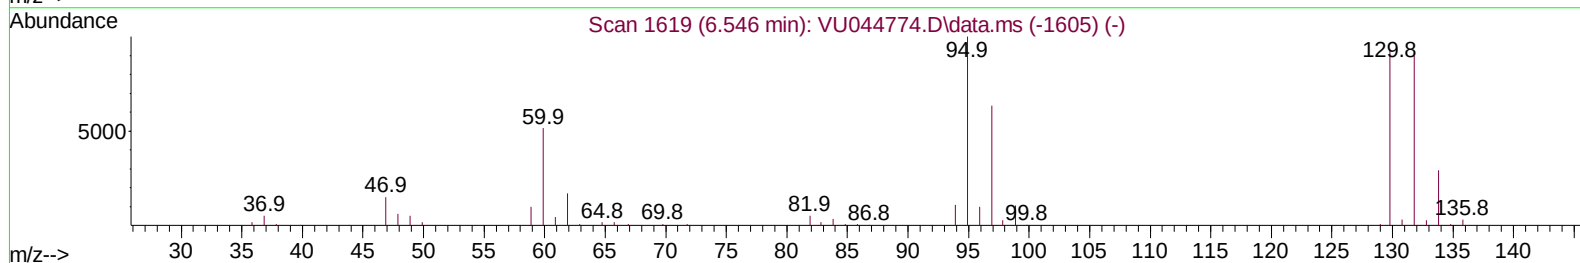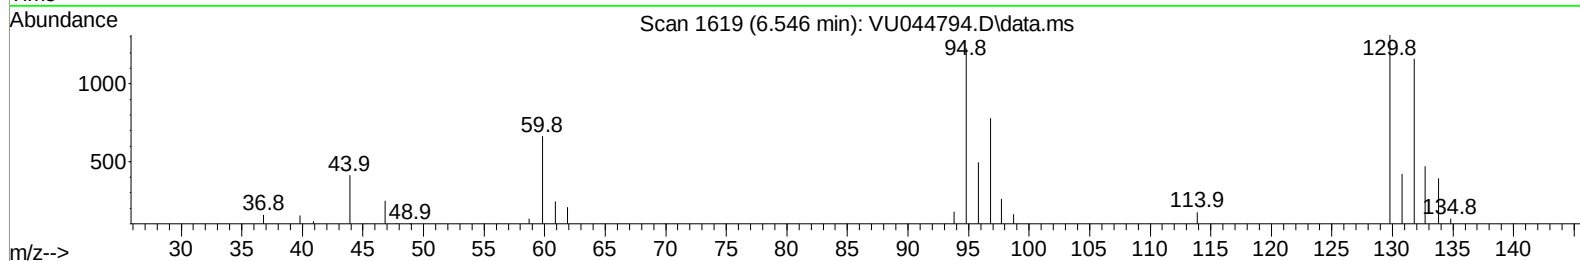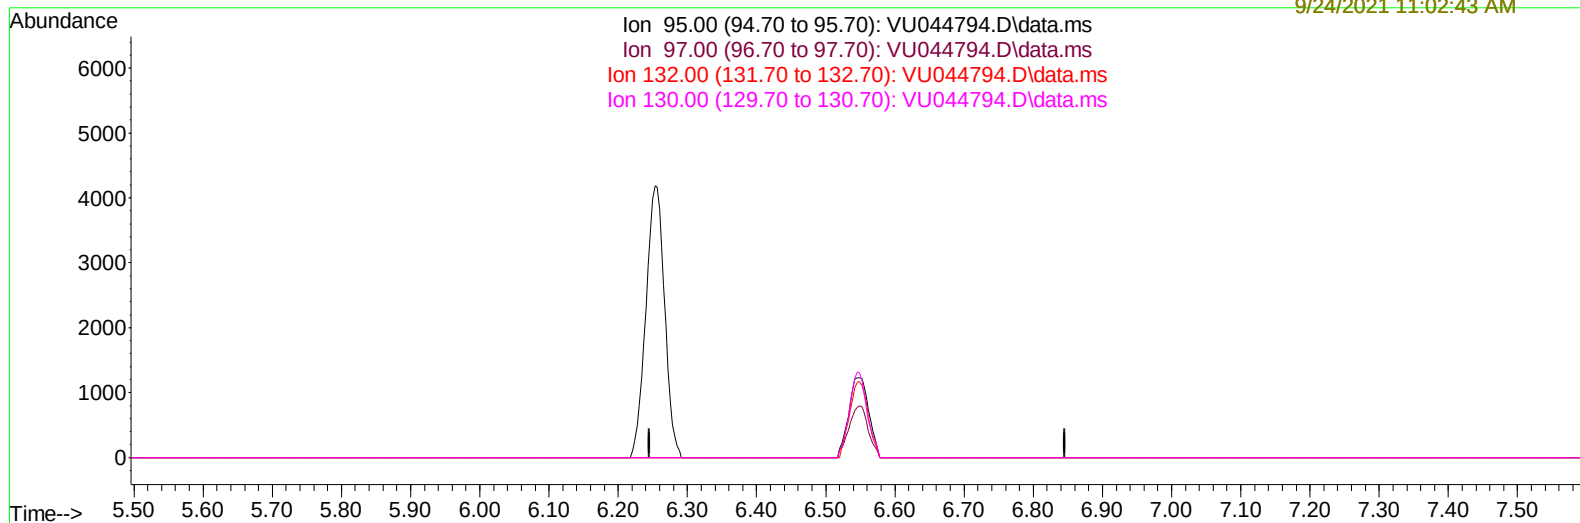

TIC: VU044794.D\data.ms

(34) Trichloroethene (T)

6.546min (-6.546) 0.00 ug/L

response 0

Ion	Exp%	Act%
95.00	100.00	0.00
97.00	63.40	0.00#
132.00	89.90	0.00#
130.00	92.90	0.00#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044794.D
Acq On : 23 Sep 2021 18:57
Operator : SY/MD
Sample : M3876-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1




Instrument :
MSVOA_U
ClientSampleId :
EW7Z1

Manual Integrations
APPROVED

MMDadoda
9/24/2021 11:02:43 AM

Quant Time: Sep 24 05:39:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 24 05:26:38 2021
Response via : Initial Calibration

9/24/2021 11:02:43 AM

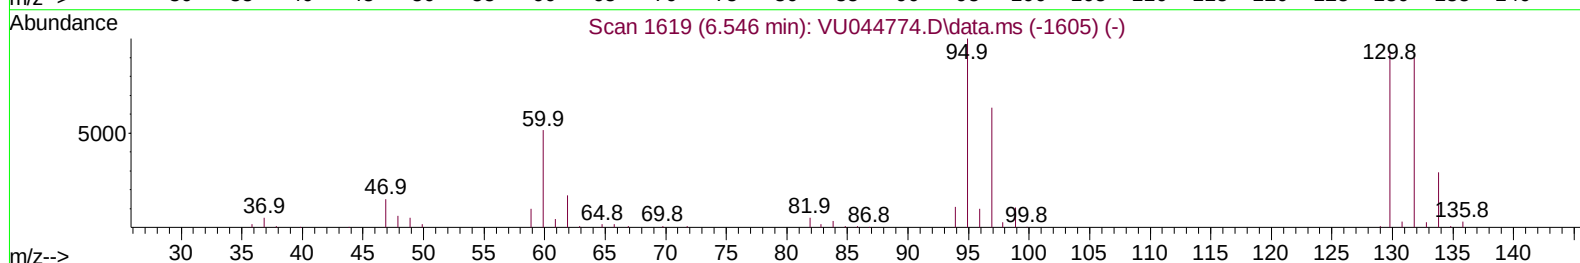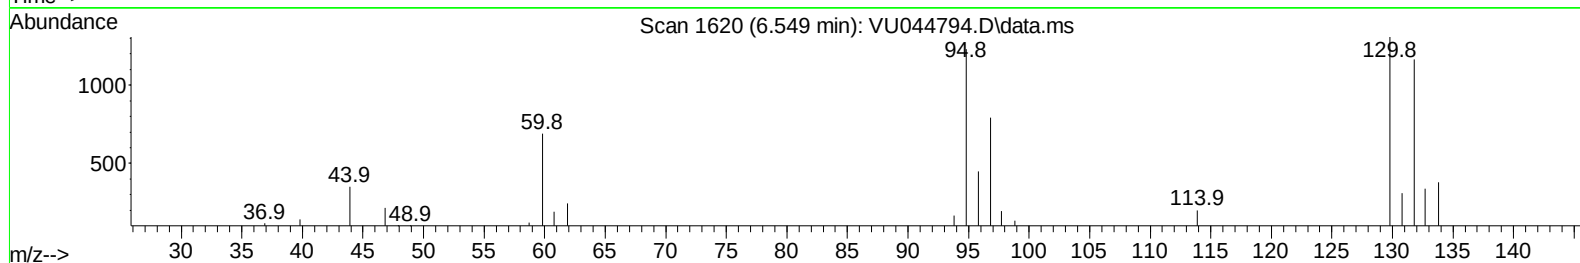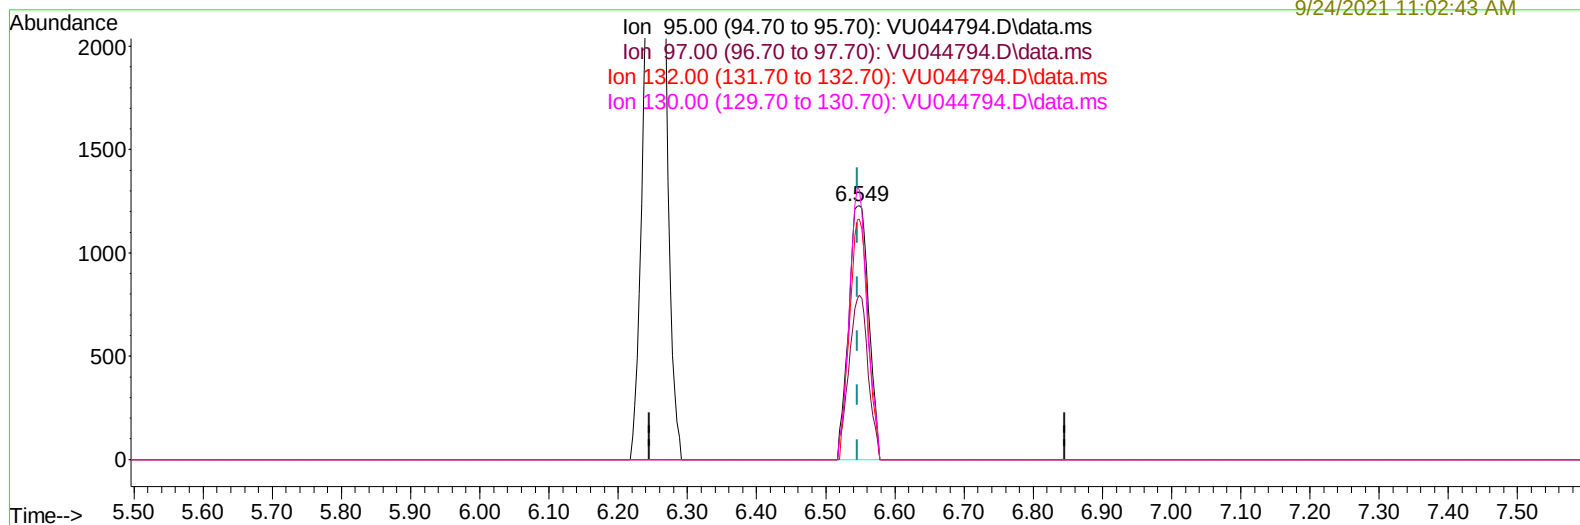

TIC: VU044794.D\data.ms

(34) Trichloroethene (T)

6.549min (+ 0.003) 1.15 ug/L m

response 2464

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	63.40	64.55
132.00	89.90	94.72
130.00	92.90	106.26

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044794.D
 Acq On : 23 Sep 2021 18:57
 Operator : SY/MD
 Sample : M3876-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 EW7Z1

Manual Integrations
 APPROVED

MMDadoda
 9/24/2021 11:02:43 AM

Quant Time: Sep 24 05:39:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 24 05:26:38 2021
 Response via : Initial Calibration

9/24/2021 11:02:43 AM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	250003	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	241336	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.815	152	105986	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	122702	44.834	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	89.660%	
7) Chloroethane-d5	1.909	69	99437	45.850	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	91.700%	
11) 1,1-Dichloroethene-d2	2.568	63	155399	33.812	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	67.620%	
21) 2-Butanone-d5	4.626	46	220889	102.091	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	102.090%	
24) Chloroform-d	5.070	84	197394	45.667	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.340%	
26) 1,2-Dichloroethane-d4	5.706	65	139938	47.795	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.580%	
32) Benzene-d6	5.732	84	397047	47.413	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.820%	
36) 1,2-Dichloropropane-d6	6.697	67	131845	48.285	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	96.560%	
41) Toluene-d8	7.902	98	325756	45.076	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	90.160%	
43) trans-1,3-Dichloroprop...	8.182	79	54196	44.619	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	89.240%	
47) 2-Hexanone-d5	8.636	63	152930	101.064	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	101.060%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	196371	46.183	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	92.360%	
66) 1,2-Dichlorobenzene-d4	12.198	152	116359	50.447	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	100.900%	
Target Compounds						
13) Acetone	2.633	43	10835	4.332	ug/L	99
20) cis-1,2-Dichloroethene	4.674	96	6111	2.719	ug/L	85
34) Trichloroethene	6.549	95	2464m	1.146	ug/L	
42) Toluene	7.973	91	5198	0.572	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044794.D
Acq On : 23 Sep 2021 18:57
Operator : SY/MD
Sample : M3876-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Z1

Manual Integrations
APPROVED

MMDadoda
9/24/2021 11:02:43 AM

Quant Time: Sep 24 05:39:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 24 05:26:38 2021
Response via : Initial Calibration

