

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044785.D
 Acq On : 23 Sep 2021 15:26
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Quant Time: Sep 24 05:38:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 24 05:26:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	269283	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	259267	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	113612	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	133297	45.218	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.440%
7) Chloroethane-d5	1.909	69	107629	46.074	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.140%
11) 1,1-Dichloroethene-d2	2.568	63	173754	35.098	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.200%
21) 2-Butanone-d5	4.623	46	240503	103.198	ug/L	-0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.200%
24) Chloroform-d	5.070	84	212412	45.623	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.240%
26) 1,2-Dichloroethane-d4	5.706	65	151697	48.102	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.200%
32) Benzene-d6	5.732	84	434122	48.255	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.500%
36) 1,2-Dichloropropane-d6	6.694	67	142734	48.657	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.320%
41) Toluene-d8	7.902	98	365902	47.129	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.260%
43) trans-1,3-Dichloroprop...	8.182	79	61229	46.923	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.840%
47) 2-Hexanone-d5	8.636	63	163968	100.864	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.860%
56) 1,1,2,2-Tetrachloroeth...	10.761	84	209215	45.801	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	12.198	152	127006	51.367	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.740%
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.581	96	3070	1.472	ug/L	# 1
17) trans-1,2-Dichloroethene	3.359	96	14069	6.405	ug/L	99
20) cis-1,2-Dichloroethene	4.671	96	480258	198.406	ug/L	97
34) Trichloroethene	6.546	95	981712	425.041	ug/L	99
42) Toluene	7.973	91	5466	0.559	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044785.D
Acq On : 23 Sep 2021 15:26
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Time: Sep 24 05:38:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 24 05:26:38 2021
Response via : Initial Calibration

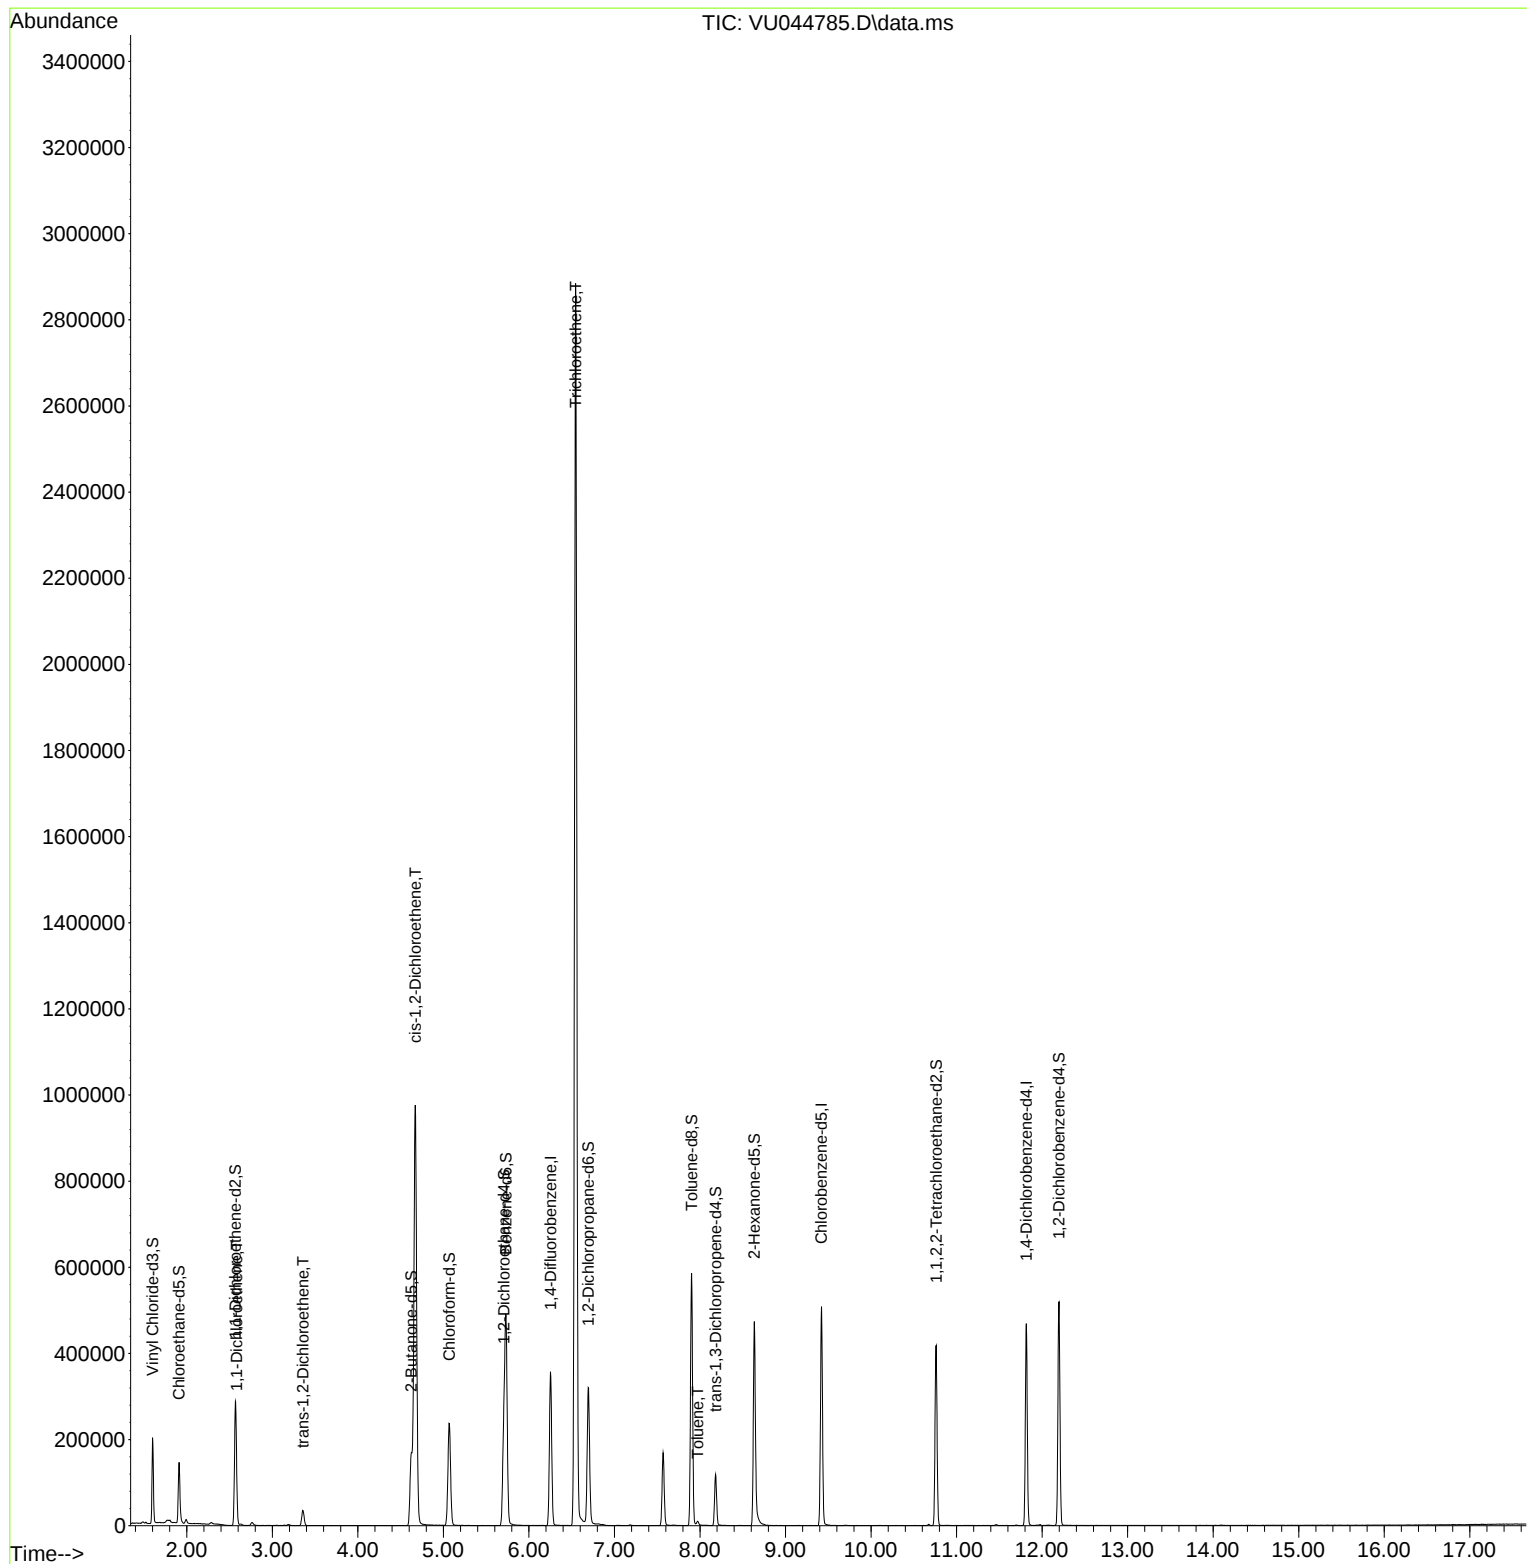

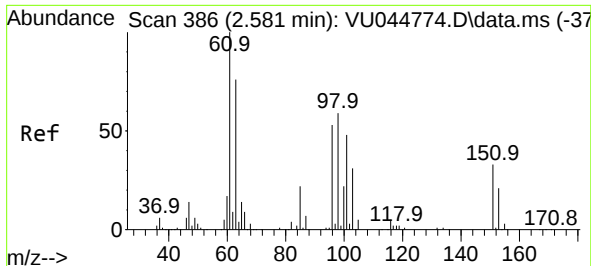

#12

1,1-Dichloroethene

Concen: 1.472 ug/L

RT: 2.581 min Scan# 386

Delta R.T. -0.000 min

Lab File: VU044785.D

Acq: 23 Sep 2021 15:26

Instrument :





MSVOA_U

ClientSampleId :

EW7X6

Tgt Ion: 96 Resp: 3070

Ion	Ratio	Lower	Upper
96	100		
61	588.4	131.3	243.9#
63	3619.3	102.5	190.3#

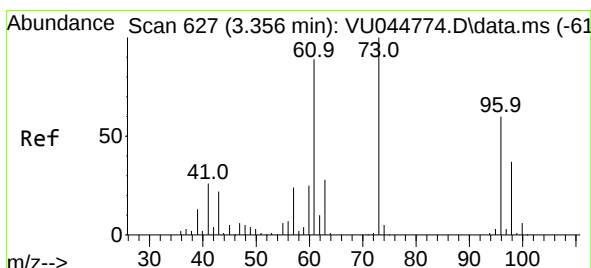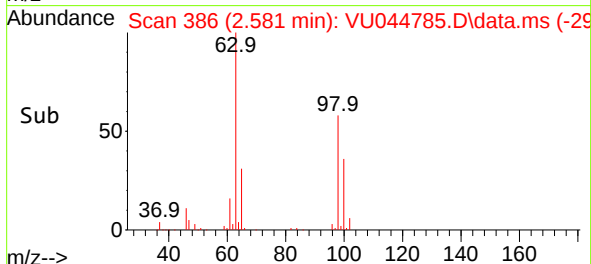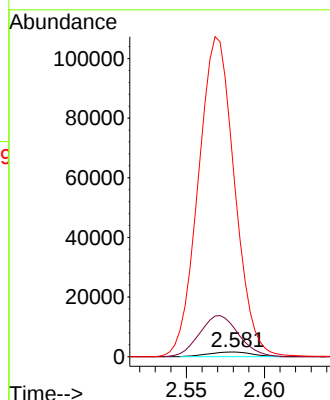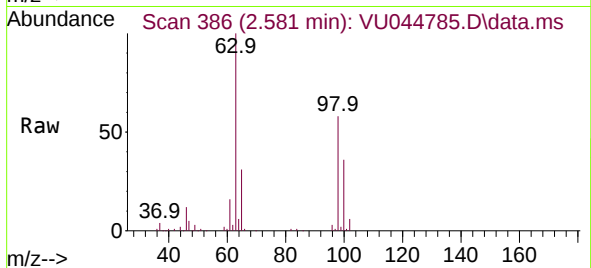

#17

trans-1,2-Dichloroethene

Concen: 6.405 ug/L

RT: 3.359 min Scan# 628




Delta R.T. 0.003 min


Lab File: VU044785.D

Acq: 23 Sep 2021 15:26

Tgt Ion: 96 Resp: 14069

Ion	Ratio	Lower	Upper
96	100		
61	151.3	105.1	195.3
98	63.0	43.0	79.8

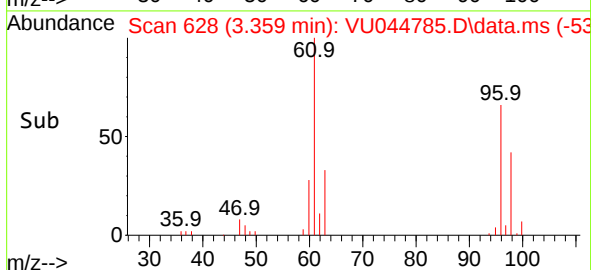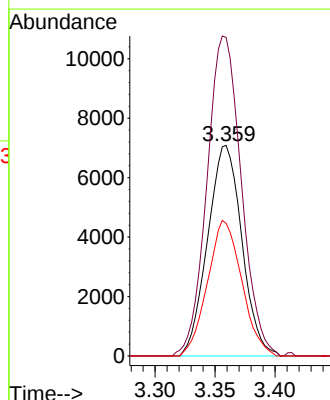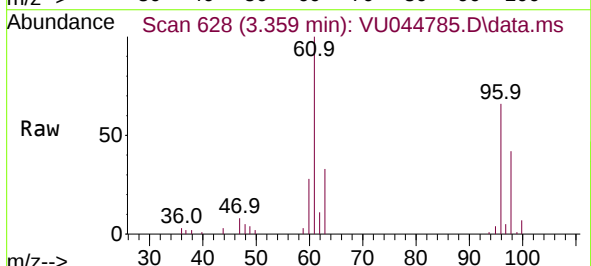

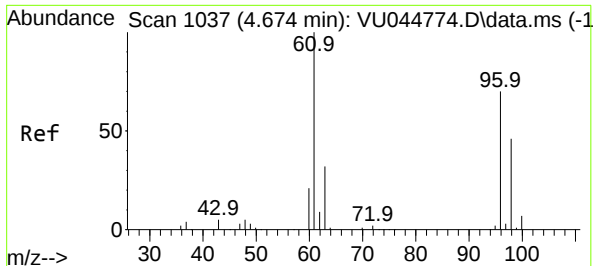

#20

cis-1,2-Dichloroethene

Concen: 198.406 ug/L

RT: 4.671 min Scan# 1036

Delta R.T. -0.003 min

Lab File: VU044785.D

Acq: 23 Sep 2021 15:26

Instrument :

MSVOA_U

ClientSampleId :

EW7X6





Tgt Ion: 96 Resp: 480258

Ion Ratio Lower Upper

96 100

61 139.3 100.2 186.0

68 0.0 0.0 0.0

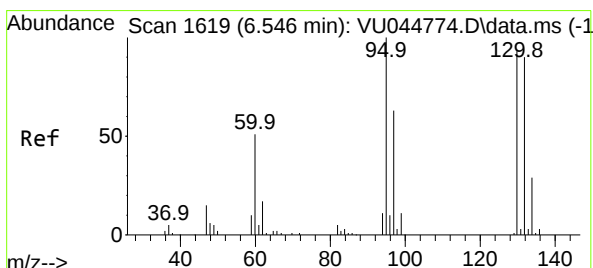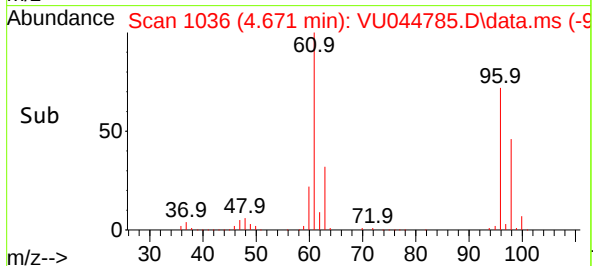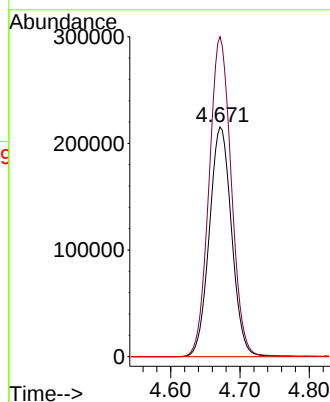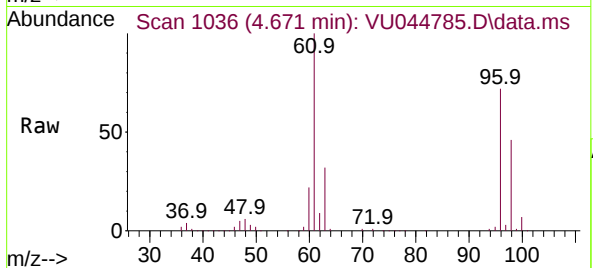

#34

Trichloroethene

Concen: 425.041 ug/L

RT: 6.546 min Scan# 1619

Delta R.T. -0.000 min

Lab File: VU044785.D

Acq: 23 Sep 2021 15:26

Tgt Ion: 95 Resp: 981712




Ion Ratio Lower Upper


95 100

97 63.9 44.4 82.4

132 89.1 62.9 116.9

130 92.0 65.0 120.8

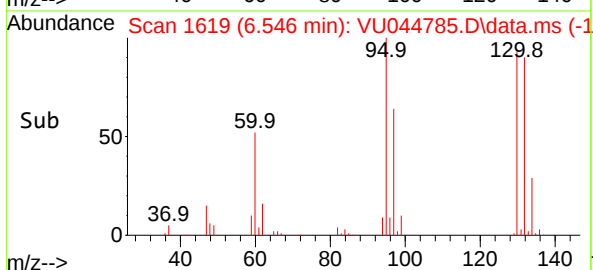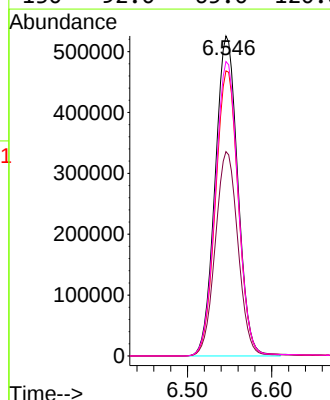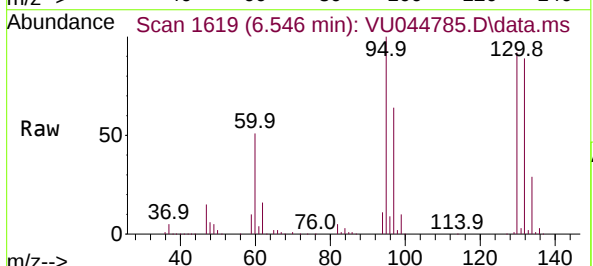

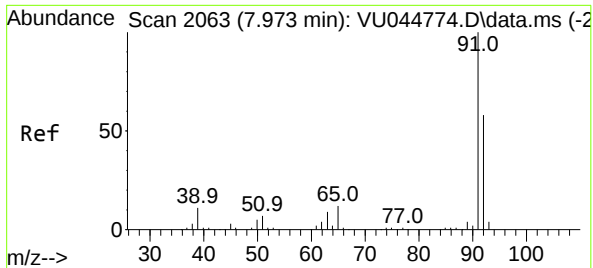

#42
Toluene
Concen: 0.559 ug/L
RT: 7.973 min Scan# 2063
Delta R.T. -0.000 min
Lab File: VU044785.D
Acq: 23 Sep 2021 15:26

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Tgt Ion: 91 Resp: 5466
Ion Ratio Lower Upper
91 100
92 51.6 40.5 75.1

