

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044779.D
 Acq On : 23 Sep 2021 13:07
 Operator : SY/MD
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rBV	201646	230526	16.68%	2.268%
2	1.909	169	177	197	rVB	146807	205991	14.90%	2.026%
3	2.568	370	382	402	rBV	297171	493682	35.72%	4.857%
4	2.796	445	453	463	rBV2	1525	2248	0.16%	0.022%
5	2.909	484	488	494	rBV2	307	225	0.02%	0.002%
6	2.948	495	500	501	rBV	366	331	0.02%	0.003%
7	3.012	516	520	524	rBV2	152	170	0.01%	0.002%
8	3.054	524	533	541	rVV3	2067	3654	0.26%	0.036%
9	3.189	565	575	585	rBV2	2216	4518	0.33%	0.044%
10	3.350	622	625	629	rBV2	496	418	0.03%	0.004%
11	3.671	722	725	727	rBV2	193	155	0.01%	0.002%
12	3.919	797	802	805	rBV2	219	252	0.02%	0.002%
13	3.993	821	825	829	rBV2	206	251	0.02%	0.002%
14	4.099	853	858	862	rVB2	206	274	0.02%	0.003%
15	4.128	862	867	870	rBV2	201	239	0.02%	0.002%
16	4.202	887	890	895	rVB2	196	196	0.01%	0.002%
17	4.231	895	899	902	rBV2	256	243	0.02%	0.002%
18	4.298	915	920	924	rBV2	190	187	0.01%	0.002%
19	4.391	945	949	952	rBV	107	105	0.01%	0.001%
20	4.555	996	1000	1006	rBV	161	151	0.01%	0.001%
21	4.626	1006	1022	1060	rBV	170053	407699	29.50%	4.011%
22	5.070	1142	1160	1181	rBV	243082	530682	38.40%	5.220%
23	5.234	1209	1211	1214	rBV3	272	172	0.01%	0.002%
24	5.292	1225	1229	1231	rBV2	502	444	0.03%	0.004%
25	5.388	1256	1259	1262	rVB2	143	107	0.01%	0.001%
26	5.459	1276	1281	1285	rBV2	141	149	0.01%	0.001%
27	5.481	1285	1288	1293	rBV2	128	156	0.01%	0.002%
28	5.729	1343	1365	1399	rBV2	505215	1382148	100.00%	13.597%
29	6.041	1460	1462	1466	rVB2	355	257	0.02%	0.003%
30	6.118	1481	1486	1488	rBV	338	273	0.02%	0.003%
31	6.253	1514	1528	1547	rBV	351397	657526	47.57%	6.468%
32	6.529	1607	1614	1625	rBV5	3501	6136	0.44%	0.060%
33	6.597	1630	1635	1639	rBV	207	297	0.02%	0.003%
34	6.616	1639	1641	1646	rVB3	228	174	0.01%	0.002%
35	6.697	1651	1666	1684	rBV	326509	635910	46.01%	6.256%
36	6.902	1727	1730	1733	rVB	218	118	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044779.D
 Acq On : 23 Sep 2021 13:07
 Operator : SY/MD
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.941	1740	1742	1746	rVB	195	141	0.01%	0.001%
38	6.967	1746	1750	1759	rVB2	116	162	0.01%	0.002%
39	7.005	1759	1762	1768	rBV2	123	107	0.01%	0.001%
40	7.050	1768	1776	1783	rVB3	803	1197	0.09%	0.012%
41	7.185	1811	1818	1829	rBV2	1147	1697	0.12%	0.017%
42	7.266	1834	1843	1844	rBV2	310	482	0.03%	0.005%
43	7.365	1867	1874	1877	rBV2	161	211	0.02%	0.002%
44	7.401	1882	1885	1889	rVB2	291	246	0.02%	0.002%
45	7.443	1889	1898	1901	rBV	277	467	0.03%	0.005%
46	7.510	1915	1919	1920	rBV	171	146	0.01%	0.001%
47	7.523	1921	1923	1925	rVV	195	112	0.01%	0.001%
48	7.571	1925	1938	1961	rVV	172612	302587	21.89%	2.977%
49	7.684	1969	1973	1974	rBV2	859	598	0.04%	0.006%
50	7.722	1984	1985	1989	rBV	224	109	0.01%	0.001%
51	7.800	2002	2009	2019	rVB3	948	1528	0.11%	0.015%
52	7.845	2019	2023	2027	rBV	130	122	0.01%	0.001%
53	7.902	2027	2041	2056	rBV	606901	1031774	74.65%	10.150%
54	7.973	2057	2063	2075	rVB2	9396	15458	1.12%	0.152%
55	8.182	2116	2128	2146	rBV	121337	202589	14.66%	1.993%
56	8.327	2171	2173	2177	rVB3	205	111	0.01%	0.001%
57	8.478	2217	2220	2224	rBV	184	119	0.01%	0.001%
58	8.500	2224	2227	2229	rBV	163	122	0.01%	0.001%
59	8.565	2244	2247	2249	rBV2	262	151	0.01%	0.001%
60	8.584	2249	2253	2256	rVV3	175	127	0.01%	0.001%
61	8.635	2256	2269	2316	rVV	487902	866982	62.73%	8.529%
62	9.420	2500	2513	2551	rBV	496763	822139	59.48%	8.088%
63	9.571	2556	2560	2573	rVB4	560	845	0.06%	0.008%
64	9.700	2593	2600	2607	rVB2	963	1427	0.10%	0.014%
65	9.825	2635	2639	2642	rBV	136	117	0.01%	0.001%
66	10.034	2701	2704	2707	rBV2	195	137	0.01%	0.001%
67	10.098	2720	2724	2726	rBV2	400	328	0.02%	0.003%
68	10.115	2726	2729	2733	rVB3	377	350	0.03%	0.003%
69	10.269	2773	2777	2784	rBV2	259	275	0.02%	0.003%
70	10.340	2793	2799	2804	rBV2	223	311	0.02%	0.003%
71	10.491	2840	2846	2852	rVB3	356	491	0.04%	0.005%
72	10.610	2880	2883	2888	rBV	148	129	0.01%	0.001%
73	10.648	2892	2895	2896	rBV	265	154	0.01%	0.002%
74	10.677	2896	2904	2911	rVV2	3629	5008	0.36%	0.049%
75	10.761	2917	2930	2948	rBV	433312	699970	50.64%	6.886%
76	10.870	2960	2964	2965	rBV3	568	407	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044779.D
 Acq On : 23 Sep 2021 13:07
 Operator : SY/MD
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.044	3015	3018	3019	rBV	169	120	0.01%	0.001%
78	11.095	3027	3034	3038	rVB3	532	615	0.04%	0.006%
79	11.118	3038	3041	3043	rBV3	472	372	0.03%	0.004%
80	11.153	3049	3052	3056	rVB2	514	394	0.03%	0.004%
81	11.362	3115	3117	3120	rBV	147	107	0.01%	0.001%
82	11.459	3139	3147	3160	rVB3	2602	4657	0.34%	0.046%
83	11.577	3181	3184	3186	rBV2	254	207	0.01%	0.002%
84	11.703	3216	3223	3231	rVB3	1273	1610	0.12%	0.016%
85	11.754	3232	3239	3244	rVB3	1242	1484	0.11%	0.015%
86	11.815	3245	3258	3283	rBV	460324	731916	52.95%	7.200%
87	11.909	3285	3287	3290	rBV3	333	200	0.01%	0.002%
88	11.944	3291	3298	3299	rBV3	785	768	0.06%	0.008%
89	12.121	3351	3353	3356	rVB3	221	112	0.01%	0.001%
90	12.198	3362	3377	3398	rBV	540723	877838	63.51%	8.636%
91	12.327	3415	3417	3420	rBV2	605	495	0.04%	0.005%
92	12.404	3437	3441	3443	rBV	263	160	0.01%	0.002%
93	12.561	3488	3490	3493	rBV2	266	128	0.01%	0.001%
94	13.224	3692	3696	3708	rVB3	1325	1685	0.12%	0.017%
95	13.777	3863	3868	3871	rBV2	264	302	0.02%	0.003%
96	13.848	3884	3890	3899	rVB3	2745	3783	0.27%	0.037%
97	14.092	3958	3966	3980	rBV	5180	8215	0.59%	0.081%
98	14.336	4034	4042	4052	rVB6	2823	4235	0.31%	0.042%
99	14.925	4223	4225	4227	rBV2	304	164	0.01%	0.002%
100	15.021	4253	4255	4260	rBV4	351	313	0.02%	0.003%




Sum of corrected areas: 10165377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044779.D
Acq On : 23 Sep 2021 13:07
Operator : SY/MD
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

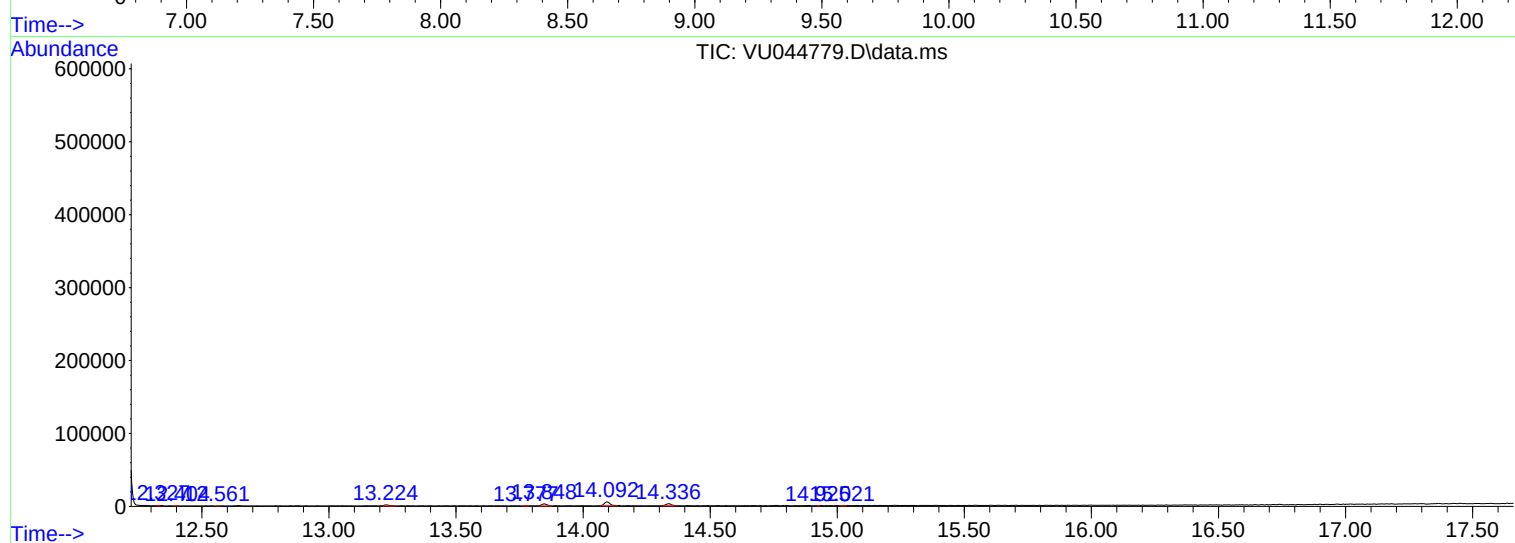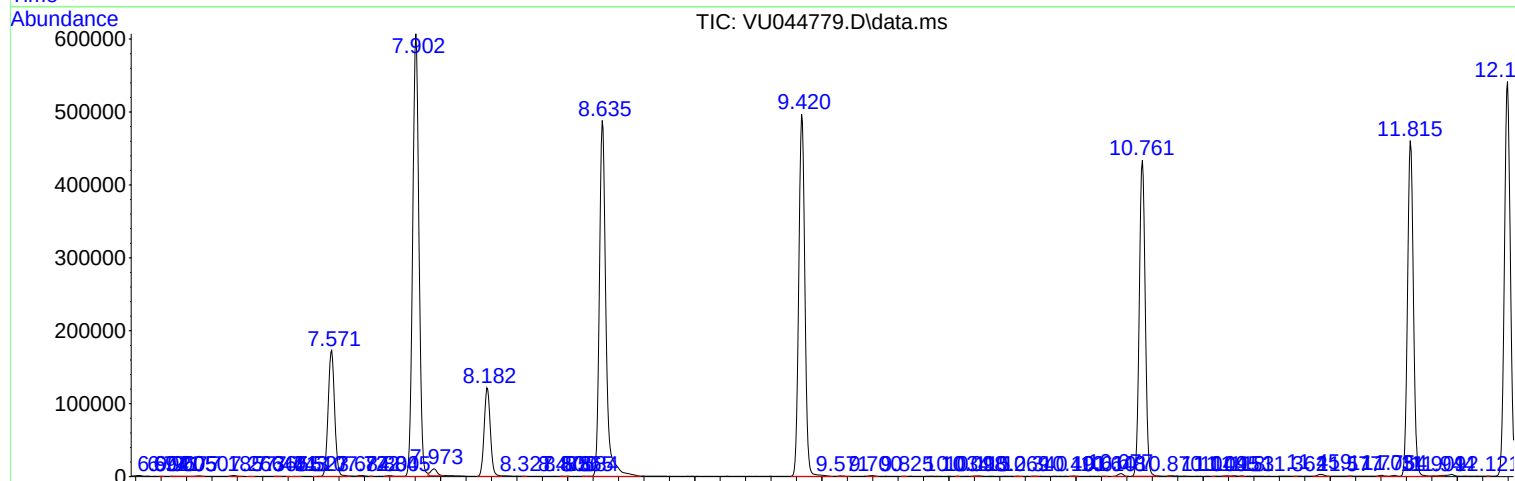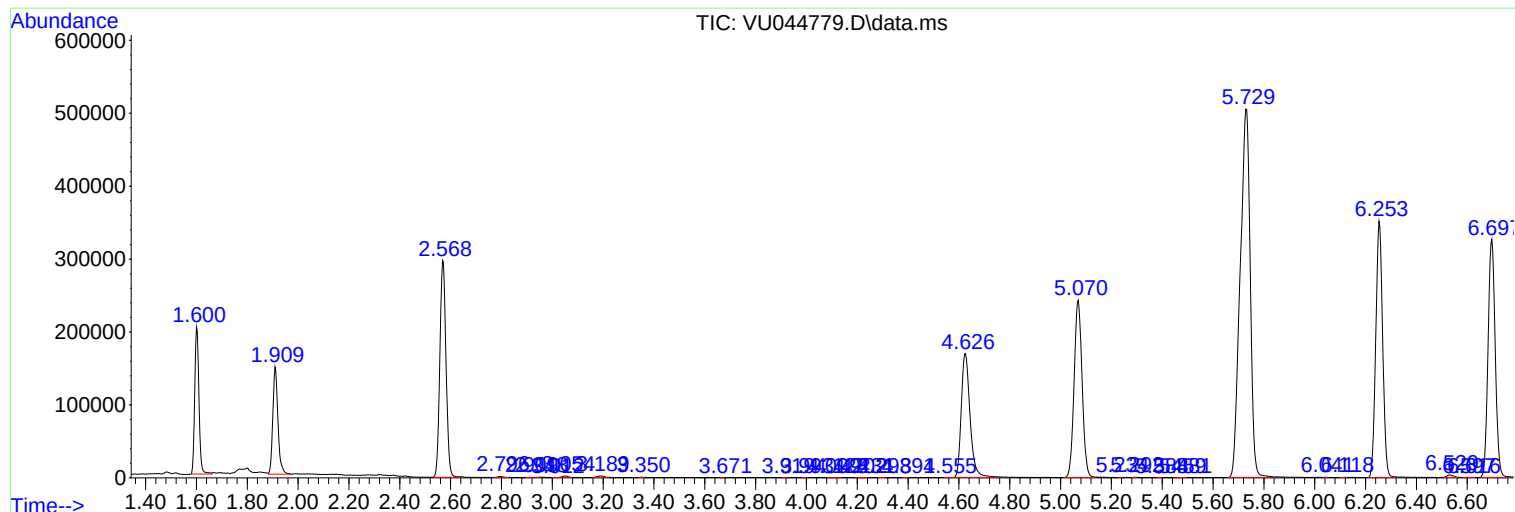

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044779.D
Acq On : 23 Sep 2021 13:07
Operator : SY/MD
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044779.D
Acq On : 23 Sep 2021 13:07
Operator : SY/MD
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
