

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044780.D
 Acq On : 23 Sep 2021 13:31
 Operator : SY/MD
 Sample : M3873-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rBV	217739	250724	5.77%	1.686%
2	1.909	169	177	197	rVB	146837	206790	4.76%	1.391%
3	2.572	370	383	402	rBV	305826	510613	11.75%	3.434%
4	2.674	413	415	417	rBV3	224	139	0.00%	0.001%
5	2.761	433	442	449	rBV2	2978	5373	0.12%	0.036%
6	2.835	463	465	470	rVB	204	116	0.00%	0.001%
7	2.877	475	478	482	rBV2	135	107	0.00%	0.001%
8	2.954	495	502	510	rBV3	756	1034	0.02%	0.007%
9	3.041	526	529	533	rBV4	557	594	0.01%	0.004%
10	3.154	557	564	566	rBV2	134	129	0.00%	0.001%
11	3.189	566	575	588	rBV2	907	2175	0.05%	0.015%
12	3.356	614	627	647	rBV	106319	208816	4.80%	1.404%
13	3.568	687	693	697	rBV	92	127	0.00%	0.001%
14	3.594	698	701	707	rVB	245	294	0.01%	0.002%
15	3.681	723	728	731	rBV2	172	230	0.01%	0.002%
16	3.742	744	747	750	rVB2	195	119	0.00%	0.001%
17	3.845	775	779	786	rVB2	168	167	0.00%	0.001%
18	3.880	787	790	792	rBV	233	135	0.00%	0.001%
19	4.047	839	842	846	rBV	148	172	0.00%	0.001%
20	4.070	846	849	853	rVV	140	124	0.00%	0.001%
21	4.478	970	976	979	rBV2	132	145	0.00%	0.001%
22	4.571	999	1005	1006	rBV2	149	158	0.00%	0.001%
23	4.671	1006	1036	1082	rBV2	1787269	4345807	100.00%	29.228%
24	5.070	1144	1160	1181	rBV	246006	533533	12.28%	3.588%
25	5.272	1220	1223	1225	rVB2	357	203	0.00%	0.001%
26	5.295	1225	1230	1232	rBV3	450	468	0.01%	0.003%
27	5.382	1254	1257	1260	rBV2	209	134	0.00%	0.001%
28	5.411	1261	1266	1270	rVV3	290	270	0.01%	0.002%
29	5.449	1275	1278	1282	rBV3	196	148	0.00%	0.001%
30	5.494	1289	1292	1296	rBV2	215	144	0.00%	0.001%
31	5.533	1301	1304	1311	rVB2	235	223	0.01%	0.001%
32	5.729	1342	1365	1393	rBV2	512326	1403808	32.30%	9.441%
33	5.880	1410	1412	1413	rBV2	238	122	0.00%	0.001%
34	6.044	1460	1463	1470	rVB3	394	374	0.01%	0.003%
35	6.253	1513	1528	1544	rBV	341131	639607	14.72%	4.302%
36	6.546	1605	1619	1639	rBV	316913	593503	13.66%	3.992%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044780.D
 Acq On : 23 Sep 2021 13:31
 Operator : SY/MD
 Sample : M3873-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.697	1651	1666	1685	rBV	326769	637263	14.66%	4.286%
38	6.809	1696	1701	1703	rBV3	587	622	0.01%	0.004%
39	6.848	1711	1713	1714	rBV	318	150	0.00%	0.001%
40	6.877	1719	1722	1726	rVB4	268	221	0.01%	0.001%
41	7.025	1765	1768	1769	rBV2	216	127	0.00%	0.001%
42	7.182	1805	1817	1827	rBV4	1364	2641	0.06%	0.018%
43	7.507	1911	1918	1923	rBV2	320	493	0.01%	0.003%
44	7.568	1923	1937	1960	rBV	175960	308933	7.11%	2.078%
45	7.719	1982	1984	1987	rVB2	197	122	0.00%	0.001%
46	7.796	2002	2008	2018	rVB3	586	1142	0.03%	0.008%
47	7.841	2018	2022	2024	rBV2	143	109	0.00%	0.001%
48	7.903	2027	2041	2055	rBV	609798	1045709	24.06%	7.033%
49	8.182	2115	2128	2151	rBV	121792	208200	4.79%	1.400%
50	8.317	2167	2170	2174	rBV	383	324	0.01%	0.002%
51	8.337	2174	2176	2181	rVB3	368	243	0.01%	0.002%
52	8.398	2192	2195	2200	rVB3	208	184	0.00%	0.001%
53	8.475	2211	2219	2230	rVB2	632	1158	0.03%	0.008%
54	8.636	2256	2269	2304	rBV	475844	840446	19.34%	5.652%
55	8.854	2333	2337	2343	rVB2	232	270	0.01%	0.002%
56	9.214	2447	2449	2454	rVB	184	127	0.00%	0.001%
57	9.243	2454	2458	2461	rBV2	168	143	0.00%	0.001%
58	9.337	2484	2487	2495	rVB	197	164	0.00%	0.001%
59	9.420	2500	2513	2538	rBV	481505	791382	18.21%	5.322%
60	9.571	2557	2560	2568	rVB3	533	676	0.02%	0.005%
61	9.700	2592	2600	2607	rVB	1102	1550	0.04%	0.010%
62	9.767	2618	2621	2625	rVB	200	151	0.00%	0.001%
63	10.102	2719	2725	2727	rBV2	572	579	0.01%	0.004%
64	10.375	2807	2810	2814	rBV	144	116	0.00%	0.001%
65	10.671	2894	2902	2911	rVB4	3547	5209	0.12%	0.035%
66	10.761	2917	2930	2949	rBV	439227	700874	16.13%	4.714%
67	10.845	2954	2956	2959	rBV	234	166	0.00%	0.001%
68	10.867	2960	2963	2964	rBV2	333	214	0.00%	0.001%
69	11.002	3002	3005	3006	rBV2	233	140	0.00%	0.001%
70	11.089	3029	3032	3035	rBV2	324	282	0.01%	0.002%
71	11.111	3036	3039	3040	rVV2	422	270	0.01%	0.002%
72	11.124	3040	3043	3047	rVV3	570	484	0.01%	0.003%
73	11.153	3047	3052	3055	rVB4	433	357	0.01%	0.002%
74	11.176	3055	3059	3062	rBV	209	192	0.00%	0.001%
75	11.205	3066	3068	3071	rBV	158	125	0.00%	0.001%
76	11.272	3086	3089	3093	rBV2	138	143	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044780.D
 Acq On : 23 Sep 2021 13:31
 Operator : SY/MD
 Sample : M3873-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.465	3138	3149	3160	rVB3	2559	4376	0.10%	0.029%
78	11.700	3216	3222	3228	rVB2	1514	1625	0.04%	0.011%
79	11.745	3232	3236	3237	rBV2	561	311	0.01%	0.002%
80	11.816	3245	3258	3276	rBV	445131	702833	16.17%	4.727%
81	11.906	3283	3286	3289	rBV2	308	200	0.00%	0.001%
82	11.947	3293	3299	3302	rBV4	1250	1447	0.03%	0.010%
83	12.063	3332	3335	3339	rBV2	459	369	0.01%	0.002%
84	12.195	3361	3376	3392	rBV	552620	885720	20.38%	5.957%
85	12.333	3415	3419	3423	rBV4	815	803	0.02%	0.005%
86	12.568	3490	3492	3495	rBV2	198	115	0.00%	0.001%
87	12.619	3505	3508	3509	rBV	267	141	0.00%	0.001%
88	12.671	3521	3524	3527	rBV2	283	203	0.00%	0.001%
89	12.722	3537	3540	3542	rBV	205	127	0.00%	0.001%
90	12.771	3552	3555	3557	rBV	276	162	0.00%	0.001%
91	12.934	3604	3606	3609	rBV	195	124	0.00%	0.001%
92	13.143	3667	3671	3677	rBV2	307	337	0.01%	0.002%
93	13.224	3691	3696	3702	rVB3	705	810	0.02%	0.005%
94	13.844	3883	3889	3902	rVB3	1796	2308	0.05%	0.016%
95	13.899	3903	3906	3908	rBV2	259	153	0.00%	0.001%
96	14.092	3959	3966	3978	rBV2	2987	4775	0.11%	0.032%
97	14.336	4036	4042	4052	rBV4	1941	2577	0.06%	0.017%
98	14.391	4057	4059	4062	rBV	304	175	0.00%	0.001%
99	14.864	4204	4206	4212	rBV3	359	283	0.01%	0.002%
100	15.118	4281	4285	4290	rBV	402	506	0.01%	0.003%




Sum of corrected areas: 14868806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044780.D
Acq On : 23 Sep 2021 13:31
Operator : SY/MD
Sample : M3873-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

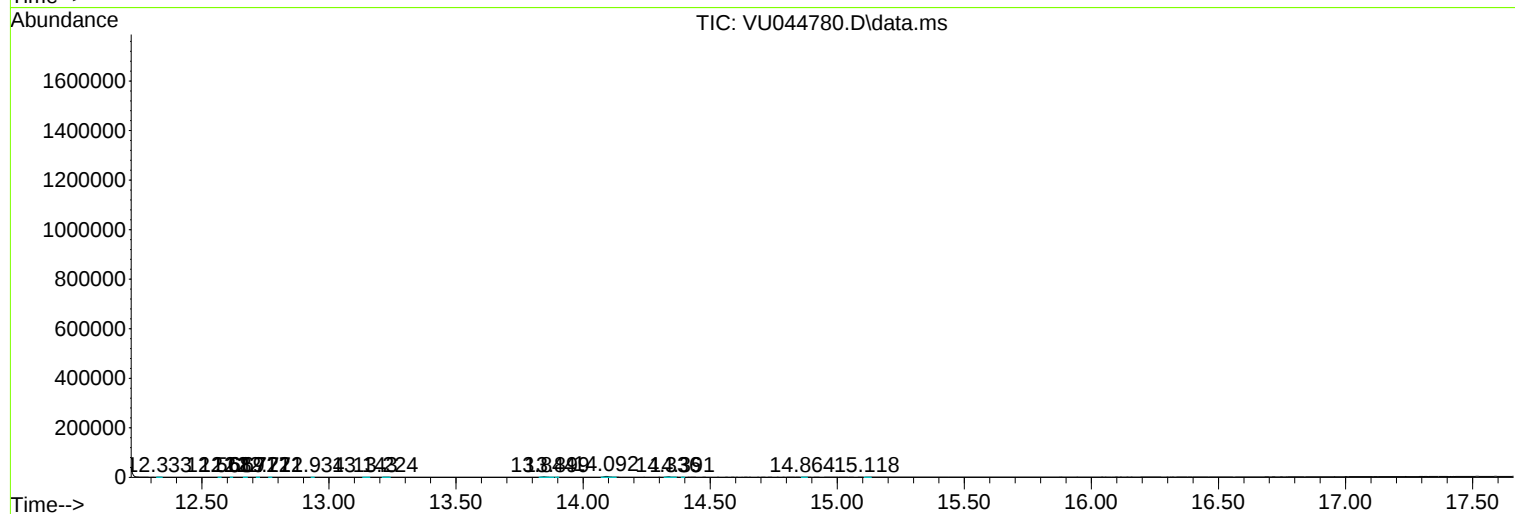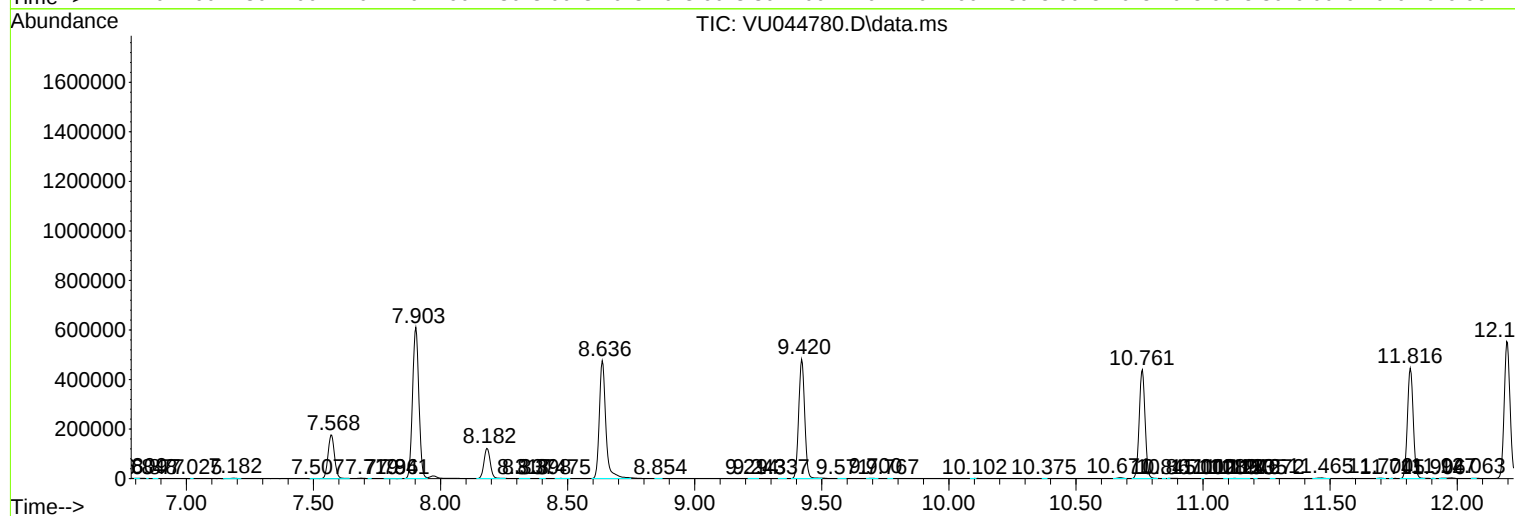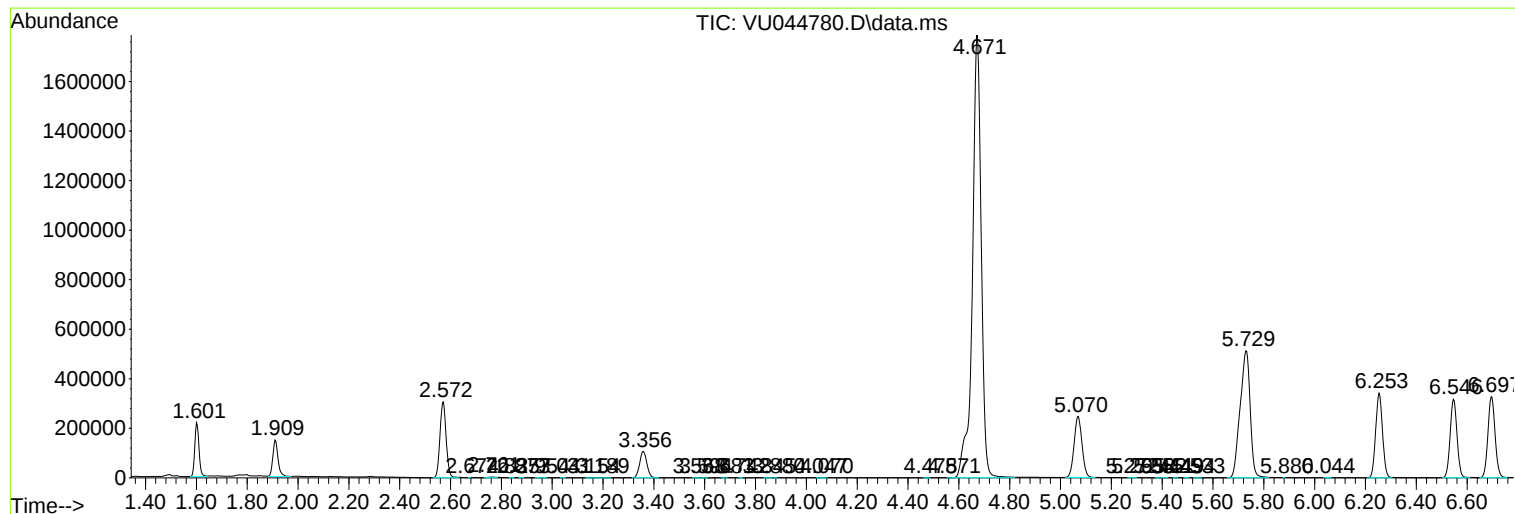

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044780.D
Acq On : 23 Sep 2021 13:31
Operator : SY/MD
Sample : M3873-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044780.D
Acq On : 23 Sep 2021 13:31
Operator : SY/MD
Sample : M3873-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
