

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044783.D
 Acq On : 23 Sep 2021 14:41
 Operator : SY/MD
 Sample : M3873-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	196717	227958	3.30%	1.299%
2	1.909	169	177	193	rVB	144352	196031	2.84%	1.117%
3	2.453	342	346	353	rVB3	588	703	0.01%	0.004%
4	2.572	370	383	398	rBV2	284557	482697	6.99%	2.751%
5	2.707	421	425	426	rBV2	207	154	0.00%	0.001%
6	2.790	437	451	473	rBV3	6508	20549	0.30%	0.117%
7	2.887	479	481	485	rVB2	306	181	0.00%	0.001%
8	2.925	491	493	497	rVB2	285	161	0.00%	0.001%
9	2.951	497	501	510	rBV3	530	1009	0.01%	0.006%
10	3.047	526	531	539	rVB3	935	1395	0.02%	0.008%
11	3.141	557	560	562	rBV	279	151	0.00%	0.001%
12	3.195	566	577	589	rVV4	734	1879	0.03%	0.011%
13	3.359	614	628	644	rBV	77683	150452	2.18%	0.857%
14	3.482	661	666	672	rBV2	124	126	0.00%	0.001%
15	3.527	676	680	687	rVB3	191	189	0.00%	0.001%
16	3.800	758	765	768	rBV2	141	197	0.00%	0.001%
17	4.099	856	858	863	rVB2	173	166	0.00%	0.001%
18	4.517	986	988	991	rVB2	223	147	0.00%	0.001%
19	4.539	991	995	999	rBV	206	251	0.00%	0.001%
20	4.671	1004	1036	1071	rBV	2946947	6903426	100.00%	39.341%
21	5.070	1144	1160	1182	rVB	233734	506011	7.33%	2.884%
22	5.362	1248	1251	1254	rBV2	141	128	0.00%	0.001%
23	5.391	1255	1260	1265	rBV3	371	497	0.01%	0.003%
24	5.481	1284	1288	1294	rBV2	95	128	0.00%	0.001%
25	5.578	1314	1318	1325	rVB2	210	193	0.00%	0.001%
26	5.620	1325	1331	1335	rBV2	197	239	0.00%	0.001%
27	5.729	1343	1365	1394	rBV2	489944	1327927	19.24%	7.568%
28	6.099	1477	1480	1483	rBV	170	150	0.00%	0.001%
29	6.121	1484	1487	1492	rVV2	286	219	0.00%	0.001%
30	6.163	1492	1500	1503	rBV4	633	818	0.01%	0.005%
31	6.253	1510	1528	1547	rBV	348840	656966	9.52%	3.744%
32	6.546	1604	1619	1638	rBV	597758	1104807	16.00%	6.296%
33	6.697	1651	1666	1686	rBV	309243	602557	8.73%	3.434%
34	6.796	1695	1697	1703	rVB4	564	341	0.00%	0.002%
35	7.041	1767	1773	1775	rBV3	589	554	0.01%	0.003%
36	7.121	1796	1798	1802	rVB	219	152	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044783.D
 Acq On : 23 Sep 2021 14:41
 Operator : SY/MD
 Sample : M3873-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.192	1811	1820	1830	rVB4	1250	2020	0.03%	0.012%
38	7.314	1851	1858	1861	rBV2	171	230	0.00%	0.001%
39	7.417	1888	1890	1895	rVB2	256	154	0.00%	0.001%
40	7.568	1925	1937	1956	rBV	167966	292772	4.24%	1.668%
41	7.690	1969	1975	1982	rVB4	827	1237	0.02%	0.007%
42	7.755	1990	1995	1999	rVB3	206	240	0.00%	0.001%
43	7.787	2002	2005	2006	rBV2	281	179	0.00%	0.001%
44	7.796	2006	2008	2012	rVB3	416	216	0.00%	0.001%
45	7.903	2026	2041	2056	rBV	577015	975567	14.13%	5.560%
46	8.182	2116	2128	2149	rBV	115438	194048	2.81%	1.106%
47	8.295	2161	2163	2167	rVV2	247	180	0.00%	0.001%
48	8.337	2174	2176	2178	rBV2	241	129	0.00%	0.001%
49	8.401	2193	2196	2199	rBV2	176	120	0.00%	0.001%
50	8.475	2212	2219	2221	rBV2	614	699	0.01%	0.004%
51	8.520	2231	2233	2238	rVB2	203	122	0.00%	0.001%
52	8.562	2243	2246	2251	rBV3	249	201	0.00%	0.001%
53	8.639	2256	2270	2298	rBV	475619	839348	12.16%	4.783%
54	8.864	2336	2340	2343	rBV3	218	223	0.00%	0.001%
55	8.903	2348	2352	2355	rBV	135	119	0.00%	0.001%
56	8.935	2359	2362	2364	rBV	258	153	0.00%	0.001%
57	9.169	2431	2435	2437	rBV	250	193	0.00%	0.001%
58	9.420	2499	2513	2535	rBV	491225	809411	11.72%	4.613%
59	9.575	2554	2561	2568	rVB2	779	913	0.01%	0.005%
60	9.645	2581	2583	2587	rVB2	282	155	0.00%	0.001%
61	9.700	2591	2600	2609	rVB3	1347	2010	0.03%	0.011%
62	9.964	2680	2682	2690	rVB2	309	213	0.00%	0.001%
63	10.005	2692	2695	2701	rVV2	163	130	0.00%	0.001%
64	10.102	2719	2725	2727	rBV3	760	850	0.01%	0.005%
65	10.153	2737	2741	2744	rBV	215	171	0.00%	0.001%
66	10.173	2744	2747	2751	rBV	154	125	0.00%	0.001%
67	10.484	2841	2844	2850	rBV	398	319	0.00%	0.002%
68	10.677	2895	2904	2911	rBV3	2620	3806	0.06%	0.022%
69	10.761	2916	2930	2949	rBV	410288	665642	9.64%	3.793%
70	10.874	2958	2965	2969	rBV4	711	902	0.01%	0.005%
71	10.893	2969	2971	2980	rVB3	693	784	0.01%	0.004%
72	11.037	3013	3016	3019	rBV	150	125	0.00%	0.001%
73	11.095	3029	3034	3038	rVV2	471	619	0.01%	0.004%
74	11.128	3038	3044	3048	rVV4	592	708	0.01%	0.004%
75	11.156	3051	3053	3060	rVB3	248	187	0.00%	0.001%
76	11.375	3118	3121	3125	rVB3	187	167	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044783.D
 Acq On : 23 Sep 2021 14:41
 Operator : SY/MD
 Sample : M3873-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.459	3140	3147	3150	rBV2	1896	2429	0.04%	0.014%
78	11.578	3181	3184	3189	rVB3	413	383	0.01%	0.002%
79	11.703	3217	3223	3229	rVB4	897	1187	0.02%	0.007%
80	11.748	3234	3237	3242	rBV2	414	354	0.01%	0.002%
81	11.816	3246	3258	3280	rBV	451303	713125	10.33%	4.064%
82	11.928	3289	3293	3294	rBV2	526	326	0.00%	0.002%
83	11.947	3294	3299	3303	rVV4	1395	1749	0.03%	0.010%
84	11.973	3303	3307	3317	rVB4	2084	2901	0.04%	0.017%
85	12.060	3329	3334	3335	rBV3	1363	1018	0.01%	0.006%
86	12.127	3350	3355	3359	rVB2	380	370	0.01%	0.002%
87	12.153	3359	3363	3364	rBV	337	251	0.00%	0.001%
88	12.195	3364	3376	3394	rVV	517811	833011	12.07%	4.747%
89	12.336	3415	3420	3425	rVB2	645	621	0.01%	0.004%
90	12.391	3435	3437	3441	rBV2	225	165	0.00%	0.001%
91	12.410	3441	3443	3445	rVV	240	118	0.00%	0.001%
92	12.439	3448	3452	3457	rVB3	266	272	0.00%	0.002%
93	12.645	3511	3516	3518	rBV2	338	290	0.00%	0.002%
94	13.848	3884	3890	3891	rBV3	542	457	0.01%	0.003%
95	14.095	3961	3967	3973	rVB	1117	1412	0.02%	0.008%
96	14.153	3982	3985	3987	rBV	310	173	0.00%	0.001%
97	14.259	4015	4018	4021	rBV	307	262	0.00%	0.001%
98	14.333	4036	4041	4047	rBV2	763	885	0.01%	0.005%
99	15.102	4276	4280	4285	rBV4	525	580	0.01%	0.003%
100	16.159	4607	4609	4613	rBV2	469	383	0.01%	0.002%




Sum of corrected areas: 17547618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044783.D
Acq On : 23 Sep 2021 14:41
Operator : SY/MD
Sample : M3873-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

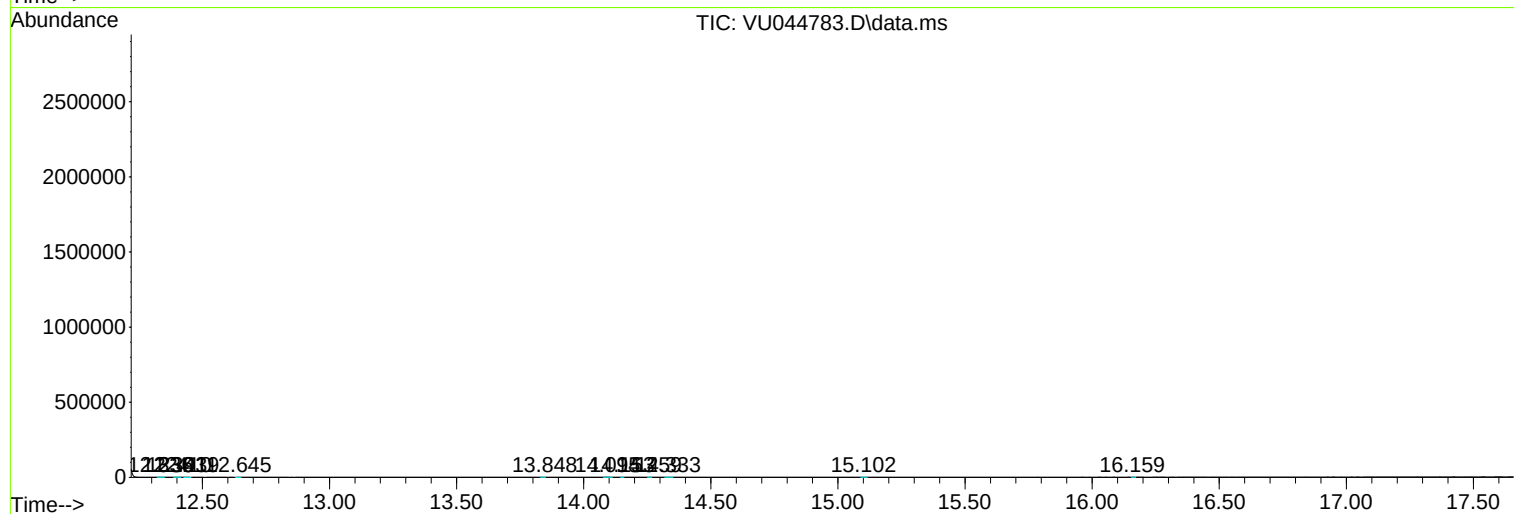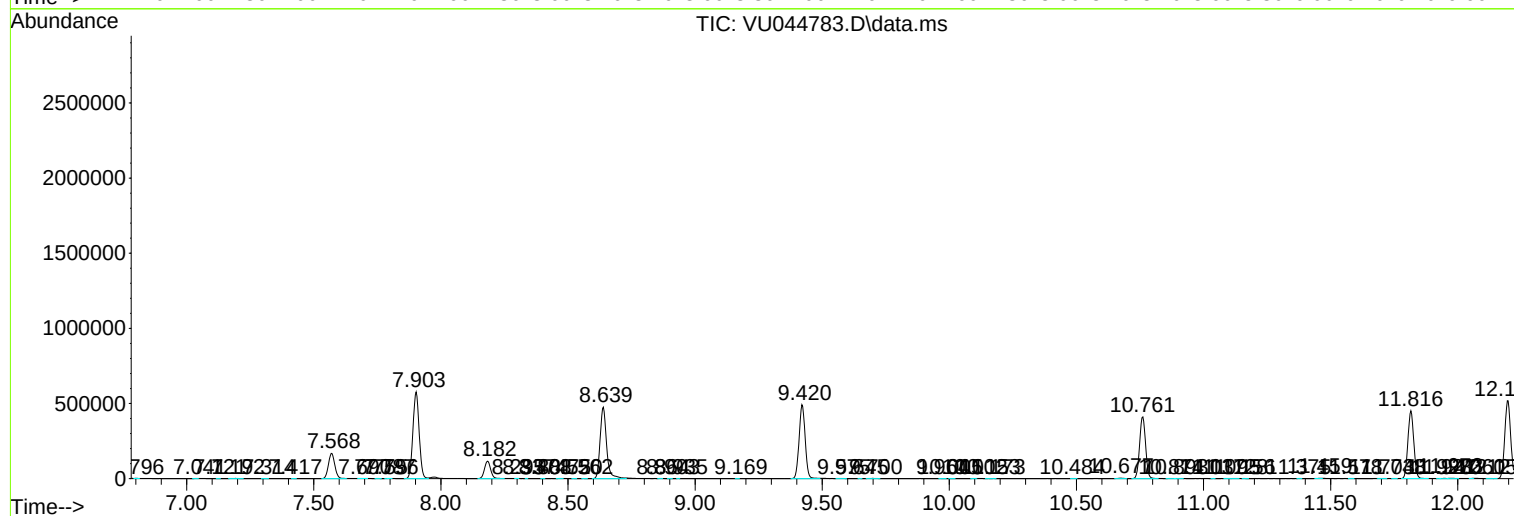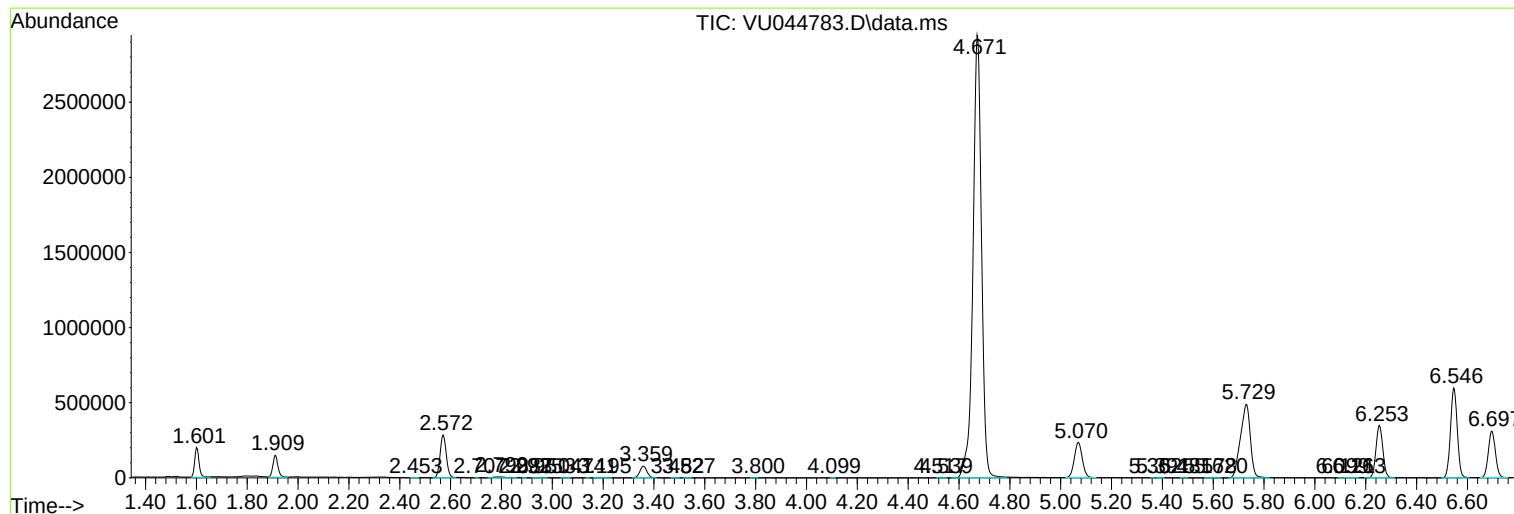

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044783.D
Acq On : 23 Sep 2021 14:41
Operator : SY/MD
Sample : M3873-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044783.D
Acq On : 23 Sep 2021 14:41
Operator : SY/MD
Sample : M3873-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
