

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044785.D
 Acq On : 23 Sep 2021 15:26
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	94	rBV	199036	227406	4.19%	1.303%
2	1.909	169	177	194	rVB	141487	195790	3.61%	1.121%
3	2.568	369	382	398	rBV	288390	481015	8.86%	2.755%
4	2.761	432	442	461	rBV2	6767	14401	0.27%	0.082%
5	2.887	477	481	490	rVB2	317	415	0.01%	0.002%
6	2.938	491	497	498	rBV2	428	347	0.01%	0.002%
7	2.977	506	509	512	rVB3	378	279	0.01%	0.002%
8	3.057	526	534	540	rVB4	744	1216	0.02%	0.007%
9	3.092	541	545	549	rVV	335	267	0.00%	0.002%
10	3.144	552	561	565	rVV5	1070	1398	0.03%	0.008%
11	3.192	567	576	587	rVV4	2324	5034	0.09%	0.029%
12	3.356	615	627	642	rVB	35298	68401	1.26%	0.392%
13	3.700	730	734	738	rBV2	364	310	0.01%	0.002%
14	3.803	760	766	770	rVV2	121	151	0.00%	0.001%
15	3.912	797	800	805	rBV2	145	119	0.00%	0.001%
16	3.954	810	813	818	rBV2	157	168	0.00%	0.001%
17	4.031	832	837	843	rBV2	140	209	0.00%	0.001%
18	4.092	850	856	860	rBV2	147	181	0.00%	0.001%
19	4.131	864	868	871	rBV2	165	175	0.00%	0.001%
20	4.224	891	897	902	rBV	182	234	0.00%	0.001%
21	4.382	943	946	950	rVV2	163	143	0.00%	0.001%
22	4.443	962	965	968	rBV2	175	141	0.00%	0.001%
23	4.526	987	991	997	rVB	152	145	0.00%	0.001%
24	4.626	1007	1022	1024	rBV	169796	269267	4.96%	1.542%
25	4.671	1027	1036	1064	rVB	973773	2147387	39.56%	12.300%
26	5.067	1143	1159	1184	rBV	236974	516843	9.52%	2.960%
27	5.208	1201	1203	1206	rBV2	276	165	0.00%	0.001%
28	5.253	1215	1217	1219	rBV	250	142	0.00%	0.001%
29	5.295	1225	1230	1235	rBV4	441	491	0.01%	0.003%
30	5.343	1241	1245	1248	rBV2	201	153	0.00%	0.001%
31	5.369	1251	1253	1258	rVV2	134	121	0.00%	0.001%
32	5.423	1266	1270	1277	rVB2	183	236	0.00%	0.001%
33	5.456	1277	1280	1285	rVB	289	160	0.00%	0.001%
34	5.729	1343	1365	1401	rBV2	490777	1340309	24.69%	7.677%
35	5.893	1414	1416	1418	rBV2	415	174	0.00%	0.001%
36	6.047	1458	1464	1471	rBV4	311	442	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044785.D
 Acq On : 23 Sep 2021 15:26
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.157	1493	1498	1500	rBV	242	263	0.00%	0.002%
38	6.253	1513	1528	1552	rBV	356865	669853	12.34%	3.837%
39	6.378	1565	1567	1571	rBV	274	206	0.00%	0.001%
40	6.546	1602	1619	1652	rBV	2883995	5428775	100.00%	31.095%
41	6.694	1653	1665	1687	rVB	316284	625225	11.52%	3.581%
42	6.912	1731	1733	1740	rVB2	260	249	0.00%	0.001%
43	6.944	1740	1743	1747	rBV	151	149	0.00%	0.001%
44	7.185	1809	1818	1830	rVB6	1539	2785	0.05%	0.016%
45	7.317	1855	1859	1862	rBV2	287	222	0.00%	0.001%
46	7.449	1896	1900	1903	rBV2	174	195	0.00%	0.001%
47	7.494	1912	1914	1918	rVB2	278	176	0.00%	0.001%
48	7.526	1918	1924	1925	rBV2	258	226	0.00%	0.001%
49	7.568	1925	1937	1954	rBV	169027	291765	5.37%	1.671%
50	7.796	2006	2008	2012	rVB3	240	137	0.00%	0.001%
51	7.816	2012	2014	2017	rBV2	169	131	0.00%	0.001%
52	7.902	2025	2041	2055	rBV	585645	996535	18.36%	5.708%
53	7.973	2058	2063	2073	rVB2	8710	13171	0.24%	0.075%
54	8.182	2113	2128	2141	rBV	118461	194437	3.58%	1.114%
55	8.359	2180	2183	2186	rBV	207	128	0.00%	0.001%
56	8.472	2215	2218	2226	rBV4	423	534	0.01%	0.003%
57	8.533	2235	2237	2241	rVV2	168	139	0.00%	0.001%
58	8.584	2251	2253	2256	rBV2	193	115	0.00%	0.001%
59	8.636	2256	2269	2313	rBV	473776	838744	15.45%	4.804%
60	8.890	2345	2348	2351	rBV2	220	131	0.00%	0.001%
61	9.144	2425	2427	2430	rBV2	262	155	0.00%	0.001%
62	9.160	2430	2432	2446	rVB2	251	317	0.01%	0.002%
63	9.420	2500	2513	2539	rBV	508216	829271	15.28%	4.750%
64	9.574	2556	2561	2570	rVB4	446	692	0.01%	0.004%
65	9.697	2592	2599	2606	rBV3	806	1245	0.02%	0.007%
66	10.102	2717	2725	2730	rBV3	293	459	0.01%	0.003%
67	10.353	2800	2803	2807	rBV2	150	137	0.00%	0.001%
68	10.513	2848	2853	2856	rBV	282	280	0.01%	0.002%
69	10.674	2895	2903	2910	rVB3	2733	3704	0.07%	0.021%
70	10.761	2916	2930	2947	rBV	418236	679748	12.52%	3.894%
71	10.857	2956	2960	2961	rBV2	399	267	0.00%	0.002%
72	11.044	3014	3018	3021	rBV	205	151	0.00%	0.001%
73	11.092	3030	3033	3035	rBV	307	224	0.00%	0.001%
74	11.124	3041	3043	3048	rBV2	307	206	0.00%	0.001%
75	11.169	3053	3057	3061	rBV3	161	162	0.00%	0.001%
76	11.208	3066	3069	3074	rVB2	223	176	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044785.D
 Acq On : 23 Sep 2021 15:26
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.333	3105	3108	3111	rVB2	226	172	0.00%	0.001%
78	11.353	3111	3114	3115	rBV	351	170	0.00%	0.001%
79	11.394	3124	3127	3132	rBV	180	173	0.00%	0.001%
80	11.426	3135	3137	3140	rVV2	260	140	0.00%	0.001%
81	11.459	3140	3147	3160	rVB4	2067	3788	0.07%	0.022%
82	11.510	3160	3163	3167	rBV	243	246	0.00%	0.001%
83	11.581	3180	3185	3194	rVB3	547	801	0.01%	0.005%
84	11.613	3194	3195	3201	rVB	132	135	0.00%	0.001%
85	11.645	3201	3205	3206	rBV	195	161	0.00%	0.001%
86	11.700	3215	3222	3228	rBV5	991	1518	0.03%	0.009%
87	11.816	3245	3258	3278	rBV	468644	735829	13.55%	4.215%
88	11.944	3294	3298	3303	rBV4	860	1064	0.02%	0.006%
89	11.976	3303	3308	3314	rVB2	2021	2333	0.04%	0.013%
90	12.066	3330	3336	3341	rBV5	726	951	0.02%	0.005%
91	12.198	3360	3377	3394	rBV	519438	851434	15.68%	4.877%
92	12.333	3414	3419	3424	rBV4	642	670	0.01%	0.004%
93	12.401	3438	3440	3444	rBV2	611	426	0.01%	0.002%
94	12.751	3545	3549	3552	rBV	213	223	0.00%	0.001%
95	13.147	3669	3672	3683	rVB3	381	610	0.01%	0.003%
96	13.391	3745	3748	3750	rBV2	228	140	0.00%	0.001%
97	13.848	3886	3890	3893	rBV3	440	351	0.01%	0.002%
98	14.098	3961	3968	3975	rBV2	945	1344	0.02%	0.008%
99	14.484	4085	4088	4093	rBV3	298	252	0.00%	0.001%
100	14.745	4166	4169	4171	rVB2	401	220	0.00%	0.001%




Sum of corrected areas: 17458471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044785.D
Acq On : 23 Sep 2021 15:26
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

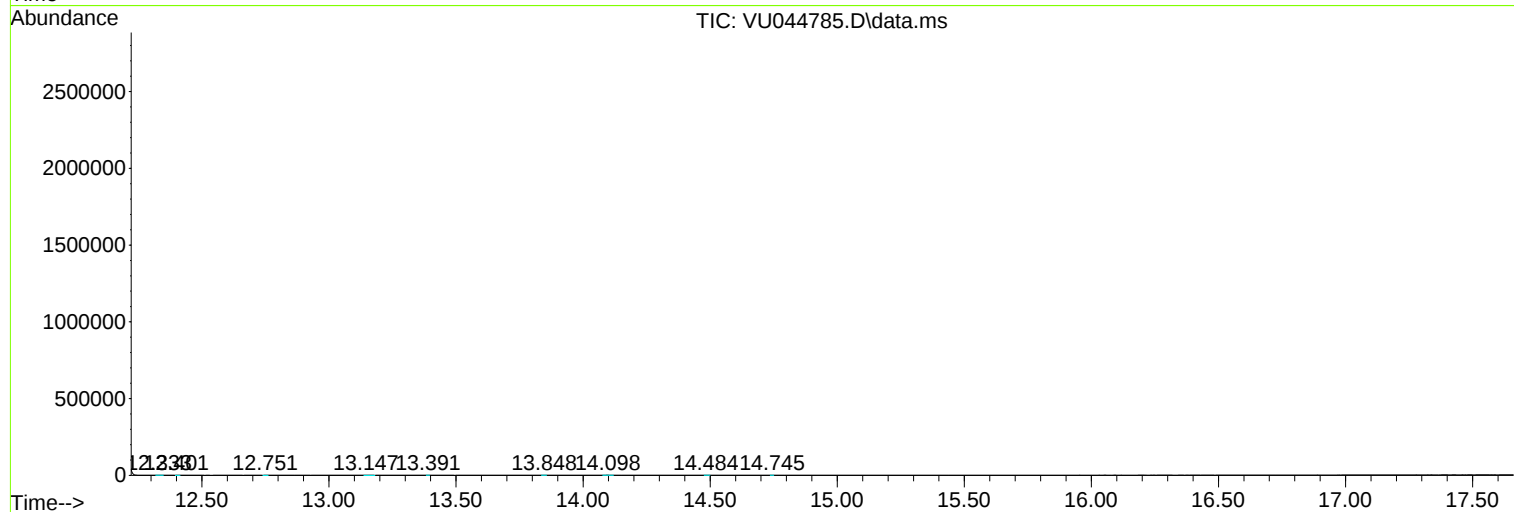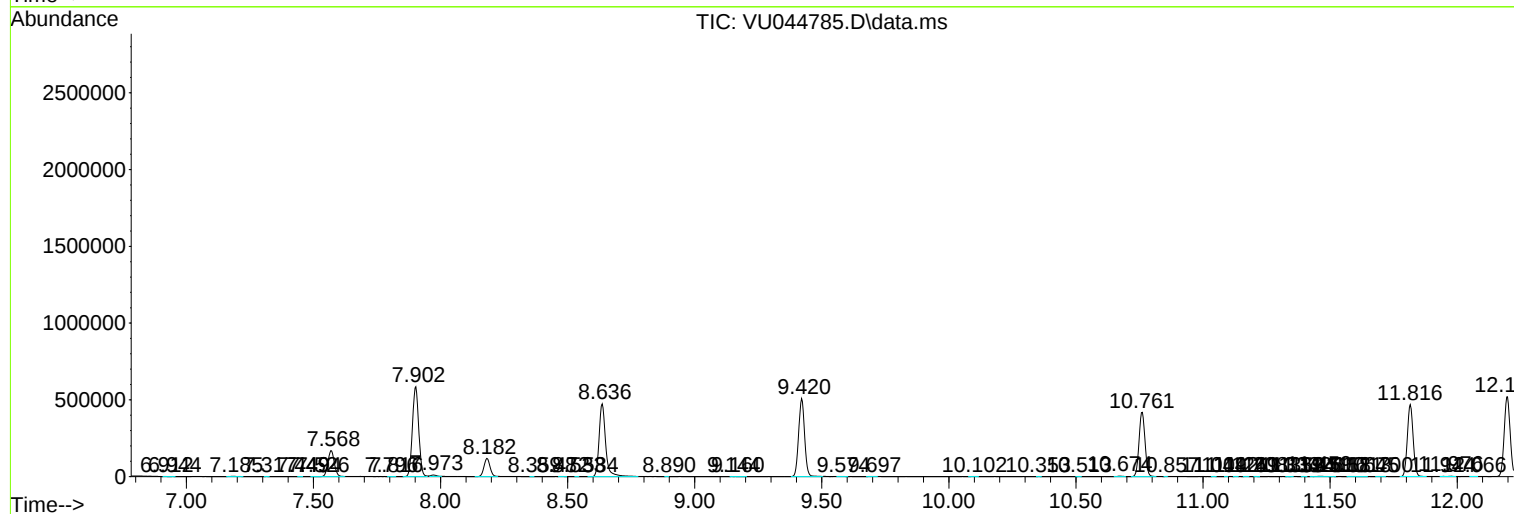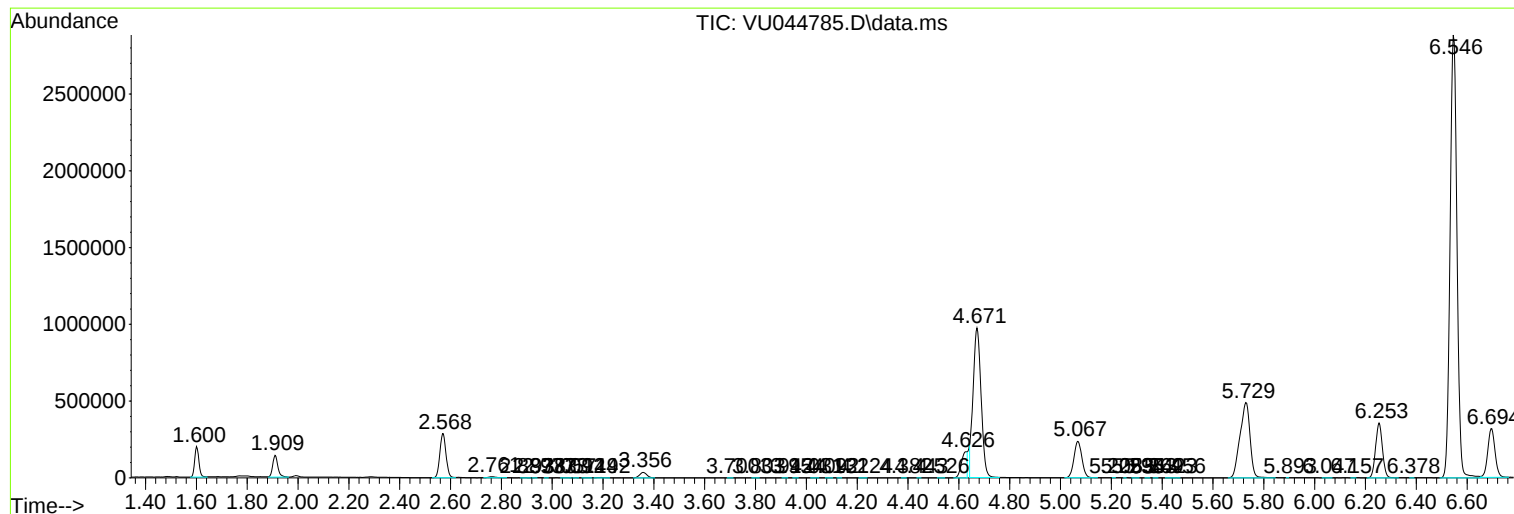

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044785.D
Acq On : 23 Sep 2021 15:26
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044785.D
Acq On : 23 Sep 2021 15:26
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
