

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044788.D
 Acq On : 23 Sep 2021 16:36
 Operator : SY/MD
 Sample : M3873-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.362	3	7	15	rVB2	5857	5795	0.07%	0.025%
2	1.604	74	82	95	rBV2	235084	285173	3.67%	1.242%
3	1.909	169	177	195	rVB	147887	200697	2.58%	0.874%
4	2.571	370	383	400	rBV	285795	478134	6.15%	2.082%
5	2.790	440	451	462	rVV5	1597	3832	0.05%	0.017%
6	2.864	471	474	479	rVB2	319	225	0.00%	0.001%
7	2.890	479	482	489	rBV2	264	305	0.00%	0.001%
8	2.960	497	504	510	rVB2	333	459	0.01%	0.002%
9	3.047	526	531	532	rBV2	455	334	0.00%	0.001%
10	3.083	537	542	548	rBV2	509	692	0.01%	0.003%
11	3.189	570	575	580	rBV4	505	670	0.01%	0.003%
12	3.359	615	628	645	rBV	38792	74938	0.96%	0.326%
13	3.510	672	675	679	rBV2	169	182	0.00%	0.001%
14	3.562	685	691	694	rBV2	122	139	0.00%	0.001%
15	3.681	722	728	733	rVV2	140	177	0.00%	0.001%
16	3.838	770	777	779	rBV2	131	162	0.00%	0.001%
17	3.877	780	789	795	rVV	538	913	0.01%	0.004%
18	3.951	807	812	817	rBV	128	128	0.00%	0.001%
19	4.407	951	954	958	rBV	156	127	0.00%	0.001%
20	4.488	974	979	987	rBV2	192	275	0.00%	0.001%
21	4.575	1003	1006	1008	rBV3	208	128	0.00%	0.001%
22	4.671	1008	1036	1069	rBV2	2272212	5420811	69.69%	23.600%
23	5.070	1144	1160	1183	rVB	238826	517477	6.65%	2.253%
24	5.247	1212	1215	1218	rBV2	403	327	0.00%	0.001%
25	5.382	1253	1257	1261	rBV3	322	224	0.00%	0.001%
26	5.497	1289	1293	1296	rVB2	279	215	0.00%	0.001%
27	5.603	1322	1326	1331	rBV2	170	168	0.00%	0.001%
28	5.729	1341	1365	1400	rBV2	493728	1343928	17.28%	5.851%
29	5.976	1440	1442	1448	rVB3	489	308	0.00%	0.001%
30	6.005	1449	1451	1454	rBV2	182	130	0.00%	0.001%
31	6.253	1513	1528	1551	rBV	365618	688508	8.85%	2.997%
32	6.362	1559	1562	1566	rBV4	345	364	0.00%	0.002%
33	6.549	1602	1620	1652	rBV	4165594	7778122	100.00%	33.862%
34	6.697	1654	1666	1688	rVB	322025	629171	8.09%	2.739%
35	7.050	1772	1776	1781	rVB4	798	748	0.01%	0.003%
36	7.179	1812	1816	1824	rVV4	1635	2111	0.03%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044788.D
 Acq On : 23 Sep 2021 16:36
 Operator : SY/MD
 Sample : M3873-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.224	1827	1830	1835	rVB2	232	144	0.00%	0.001%
38	7.346	1864	1868	1870	rVB	204	160	0.00%	0.001%
39	7.362	1870	1873	1877	rVB2	181	169	0.00%	0.001%
40	7.423	1890	1892	1897	rVB2	334	265	0.00%	0.001%
41	7.449	1897	1900	1902	rBV	277	153	0.00%	0.001%
42	7.494	1909	1914	1917	rVB	275	256	0.00%	0.001%
43	7.571	1925	1938	1952	rBV	165846	291631	3.75%	1.270%
44	7.690	1969	1975	1978	rBV4	920	1056	0.01%	0.005%
45	7.722	1978	1985	1993	rVB4	2324	3792	0.05%	0.017%
46	7.809	2007	2012	2017	rBV4	329	411	0.01%	0.002%
47	7.902	2026	2041	2056	rBV	571741	984283	12.65%	4.285%
48	7.973	2058	2063	2076	rVB	9478	15039	0.19%	0.065%
49	8.182	2117	2128	2151	rBV	116592	194329	2.50%	0.846%
50	8.298	2162	2164	2169	rVB3	339	244	0.00%	0.001%
51	8.369	2182	2186	2187	rBV2	218	131	0.00%	0.001%
52	8.414	2195	2200	2202	rBV2	207	220	0.00%	0.001%
53	8.475	2214	2219	2220	rBV2	490	379	0.00%	0.002%
54	8.523	2231	2234	2237	rVV2	203	136	0.00%	0.001%
55	8.555	2240	2244	2248	rBV4	353	291	0.00%	0.001%
56	8.639	2257	2270	2300	rBV	489878	868179	11.16%	3.780%
57	8.893	2346	2349	2353	rVB2	318	206	0.00%	0.001%
58	8.938	2359	2363	2367	rVB2	209	167	0.00%	0.001%
59	9.008	2382	2385	2388	rBV	266	241	0.00%	0.001%
60	9.102	2411	2414	2419	rVB2	161	158	0.00%	0.001%
61	9.131	2419	2423	2425	rBV2	161	143	0.00%	0.001%
62	9.240	2454	2457	2459	rBV	206	168	0.00%	0.001%
63	9.420	2499	2513	2536	rBV	511781	850827	10.94%	3.704%
64	9.568	2555	2559	2563	rVV2	618	587	0.01%	0.003%
65	9.597	2566	2568	2571	rVB3	232	132	0.00%	0.001%
66	9.632	2576	2579	2582	rVB2	197	136	0.00%	0.001%
67	9.674	2586	2592	2593	rBV	201	212	0.00%	0.001%
68	9.693	2593	2598	2607	rVV3	942	1406	0.02%	0.006%
69	9.809	2632	2634	2637	rVB2	248	149	0.00%	0.001%
70	9.928	2663	2671	2676	rBV2	243	435	0.01%	0.002%
71	10.677	2896	2904	2911	rBV3	2591	3619	0.05%	0.016%
72	10.761	2917	2930	2950	rBV	432467	685878	8.82%	2.986%
73	10.867	2959	2963	2965	rBV2	604	516	0.01%	0.002%
74	11.118	3038	3041	3051	rVB4	854	1268	0.02%	0.006%
75	11.163	3051	3055	3058	rBV	234	259	0.00%	0.001%
76	11.465	3140	3149	3156	rBV4	1660	2973	0.04%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044788.D
 Acq On : 23 Sep 2021 16:36
 Operator : SY/MD
 Sample : M3873-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.703	3214	3223	3226	rBV6	1146	1577	0.02%	0.007%
78	11.767	3240	3243	3245	rBV	334	185	0.00%	0.001%
79	11.815	3245	3258	3279	rVV	479904	757906	9.74%	3.300%
80	11.944	3295	3298	3301	rBV3	481	383	0.00%	0.002%
81	12.066	3327	3336	3347	rBV5	2675	5203	0.07%	0.023%
82	12.121	3351	3353	3356	rVB2	399	185	0.00%	0.001%
83	12.198	3360	3377	3393	rBV	527614	852744	10.96%	3.712%
84	12.278	3399	3402	3406	rVB3	863	604	0.01%	0.003%
85	12.333	3414	3419	3424	rVB4	751	951	0.01%	0.004%
86	12.362	3424	3428	3429	rBV	188	139	0.00%	0.001%
87	12.642	3511	3515	3519	rBV2	377	356	0.00%	0.002%
88	13.008	3626	3629	3631	rBV2	193	126	0.00%	0.001%
89	13.143	3670	3671	3676	rVB2	326	200	0.00%	0.001%
90	13.185	3681	3684	3688	rVB3	259	172	0.00%	0.001%
91	13.844	3886	3889	3890	rBV	450	265	0.00%	0.001%
92	13.957	3921	3924	3927	rBV	277	165	0.00%	0.001%
93	14.066	3955	3958	3960	rBV2	207	140	0.00%	0.001%
94	14.204	3999	4001	4004	rBV	342	236	0.00%	0.001%
95	14.249	4013	4015	4017	rBV	258	124	0.00%	0.001%
96	14.343	4042	4044	4049	rBV3	237	209	0.00%	0.001%
97	14.738	4165	4167	4172	rVB4	370	257	0.00%	0.001%
98	14.986	4241	4244	4247	rBV3	320	289	0.00%	0.001%
99	15.005	4248	4250	4253	rVV2	371	210	0.00%	0.001%
100	15.256	4322	4328	4330	rBV3	454	490	0.01%	0.002%




Sum of corrected areas: 22969961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044788.D
Acq On : 23 Sep 2021 16:36
Operator : SY/MD
Sample : M3873-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

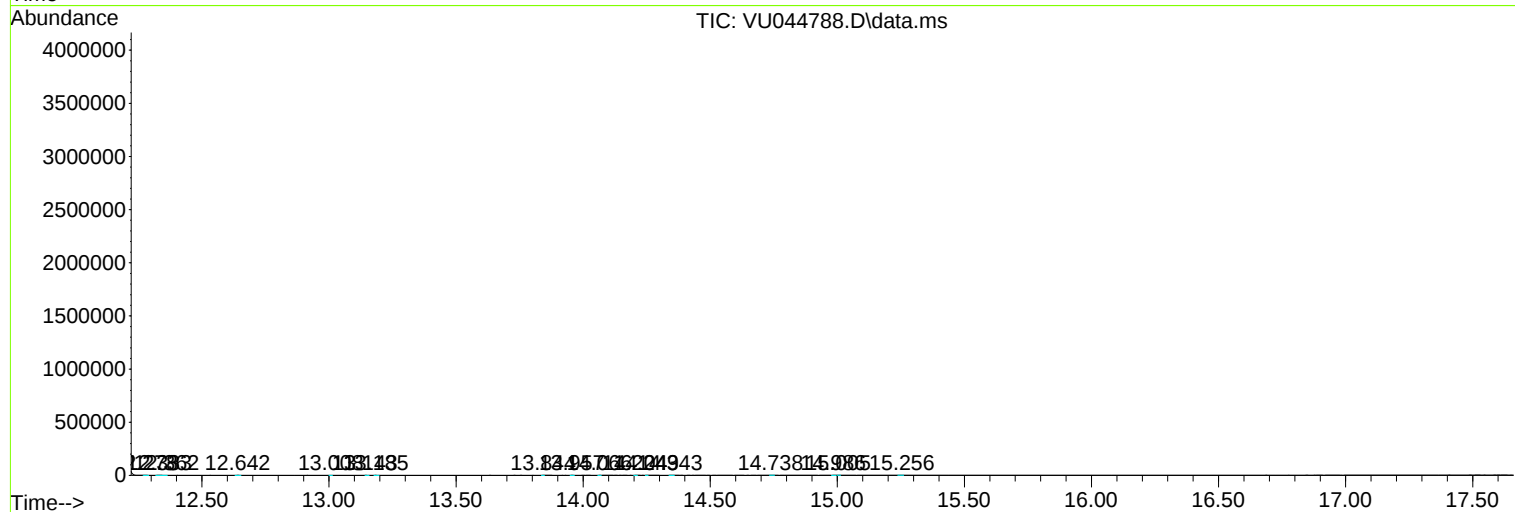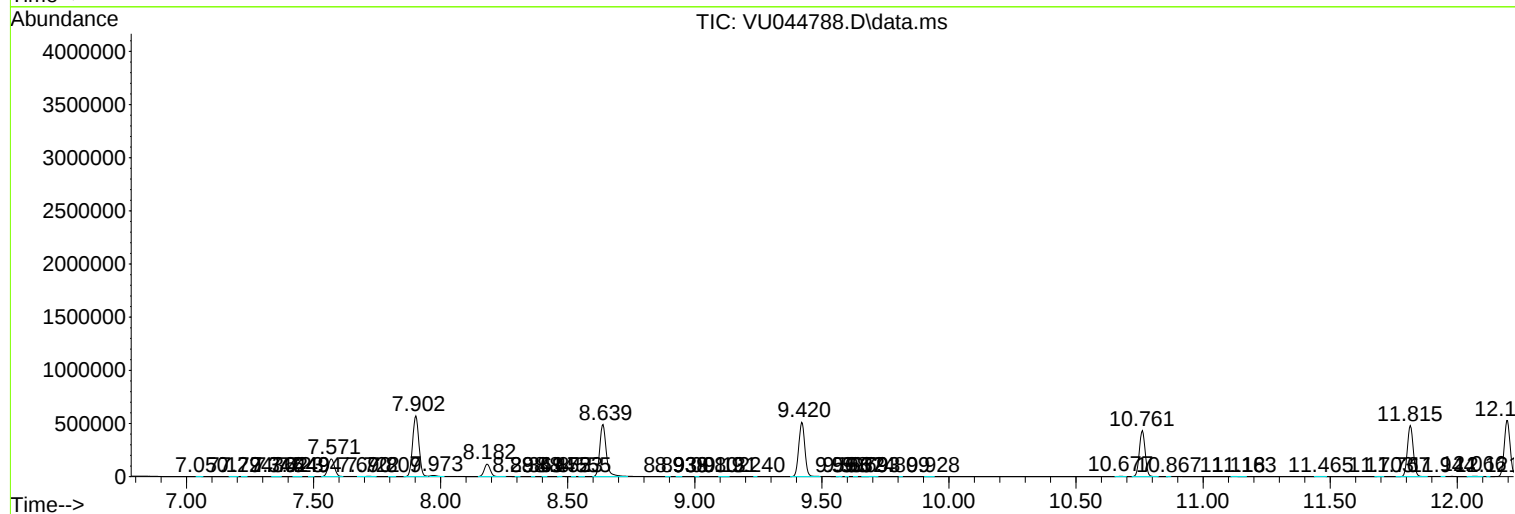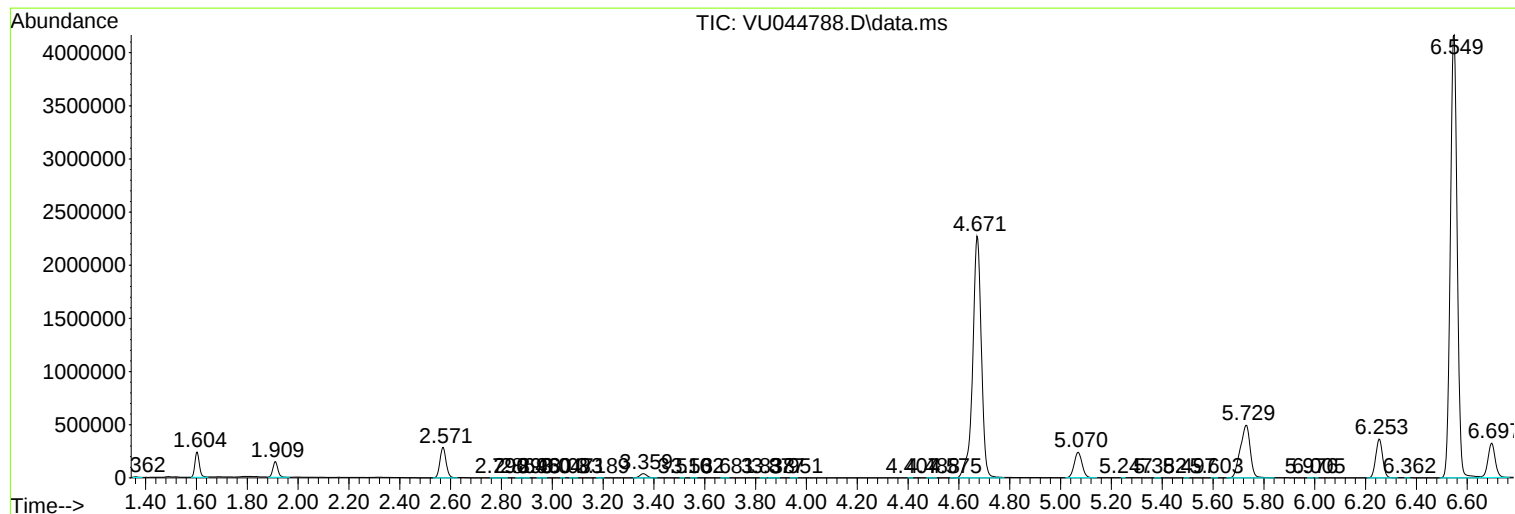

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044788.D
Acq On : 23 Sep 2021 16:36
Operator : SY/MD
Sample : M3873-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044788.D
Acq On : 23 Sep 2021 16:36
Operator : SY/MD
Sample : M3873-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
