

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044790.D
 Acq On : 23 Sep 2021 17:23
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rBV	178225	201789	16.34%	2.160%
2	1.909	169	177	194	rVB	135709	184236	14.92%	1.972%
3	2.568	370	382	397	rBV	260168	431422	34.93%	4.618%
4	2.678	414	416	421	rBV2	195	165	0.01%	0.002%
5	2.777	435	447	473	rVB	11031	30901	2.50%	0.331%
6	2.954	496	502	504	rBV3	350	353	0.03%	0.004%
7	3.051	526	532	533	rBV2	726	731	0.06%	0.008%
8	3.092	542	545	550	rVB2	259	221	0.02%	0.002%
9	3.144	557	561	562	rBV	202	174	0.01%	0.002%
10	3.195	564	577	596	rVV	8337	21485	1.74%	0.230%
11	3.282	601	604	606	rVB2	173	108	0.01%	0.001%
12	3.359	618	628	629	rBV3	1534	2094	0.17%	0.022%
13	3.401	637	641	645	rBV	188	106	0.01%	0.001%
14	3.424	645	648	650	rBV	171	141	0.01%	0.002%
15	3.462	657	660	664	rVB2	318	226	0.02%	0.002%
16	3.488	664	668	669	rBV	184	118	0.01%	0.001%
17	3.498	669	671	674	rVB2	258	150	0.01%	0.002%
18	3.520	674	678	680	rBV2	270	233	0.02%	0.002%
19	3.565	689	692	697	rBV2	193	228	0.02%	0.002%
20	3.600	701	703	709	rVB2	284	239	0.02%	0.003%
21	3.629	709	712	717	rBV	275	264	0.02%	0.003%
22	3.735	741	745	747	rBV2	173	112	0.01%	0.001%
23	3.768	752	755	758	rVB	172	109	0.01%	0.001%
24	3.793	761	763	767	rVB2	188	97	0.01%	0.001%
25	3.851	778	781	785	rVB2	157	116	0.01%	0.001%
26	3.961	807	815	818	rBV2	116	160	0.01%	0.002%
27	4.012	828	831	833	rBV2	138	99	0.01%	0.001%
28	4.054	840	844	853	rBV2	390	573	0.05%	0.006%
29	4.301	916	921	925	rBV2	159	173	0.01%	0.002%
30	4.629	1007	1023	1032	rBV	157320	380509	30.81%	4.073%
31	4.986	1129	1134	1136	rBV3	229	191	0.02%	0.002%
32	5.002	1136	1139	1142	rVV	126	125	0.01%	0.001%
33	5.070	1143	1160	1184	rVV	222124	480100	38.87%	5.139%
34	5.179	1191	1194	1200	rVB4	393	423	0.03%	0.005%
35	5.208	1200	1203	1204	rBV	236	159	0.01%	0.002%
36	5.224	1207	1208	1211	rVB	246	113	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044790.D
 Acq On : 23 Sep 2021 17:23
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.292	1226	1229	1233	rVB3	396	352	0.03%	0.004%
38	5.562	1309	1313	1317	rBV2	186	238	0.02%	0.003%
39	5.729	1343	1365	1386	rBV2	452756	1235138	100.00%	13.220%
40	5.925	1423	1426	1428	rBV2	218	144	0.01%	0.002%
41	5.967	1437	1439	1442	rVB	307	185	0.01%	0.002%
42	6.112	1481	1484	1486	rBV2	193	113	0.01%	0.001%
43	6.253	1513	1528	1549	rBV	343367	647501	52.42%	6.930%
44	6.546	1607	1619	1633	rBV4	32201	63078	5.11%	0.675%
45	6.697	1650	1666	1695	rBV	296574	571852	46.30%	6.121%
46	6.813	1698	1702	1708	rVB5	1005	1151	0.09%	0.012%
47	6.845	1708	1712	1715	rVB2	130	110	0.01%	0.001%
48	6.864	1715	1718	1720	rBV3	161	143	0.01%	0.002%
49	7.028	1767	1769	1770	rBV	252	113	0.01%	0.001%
50	7.047	1770	1775	1783	rVB2	649	831	0.07%	0.009%
51	7.182	1808	1817	1827	rVB4	1228	2131	0.17%	0.023%
52	7.253	1833	1839	1845	rBV2	178	249	0.02%	0.003%
53	7.571	1925	1938	1958	rBV	147130	262081	21.22%	2.805%
54	7.687	1967	1974	1989	rVB5	1106	2140	0.17%	0.023%
55	7.793	2002	2007	2010	rBV2	249	272	0.02%	0.003%
56	7.902	2026	2041	2056	rBV	527847	895249	72.48%	9.582%
57	7.970	2058	2062	2076	rVB2	7887	12672	1.03%	0.136%
58	8.182	2114	2128	2151	rBV	104363	176284	14.27%	1.887%
59	8.295	2160	2163	2165	rBV2	253	135	0.01%	0.001%
60	8.330	2172	2174	2177	rVB2	179	105	0.01%	0.001%
61	8.349	2177	2180	2184	rBV2	148	176	0.01%	0.002%
62	8.394	2191	2194	2200	rBV3	195	203	0.02%	0.002%
63	8.472	2212	2218	2219	rBV2	281	293	0.02%	0.003%
64	8.636	2256	2269	2309	rBV	457897	811335	65.69%	8.684%
65	8.896	2347	2350	2353	rBV	177	118	0.01%	0.001%
66	8.992	2377	2380	2386	rBV2	174	226	0.02%	0.002%
67	9.211	2446	2448	2451	rVB2	209	114	0.01%	0.001%
68	9.420	2500	2513	2552	rBV	483988	799247	64.71%	8.554%
69	9.693	2593	2598	2606	rBV3	652	899	0.07%	0.010%
70	9.854	2643	2648	2653	rBV2	182	201	0.02%	0.002%
71	9.880	2653	2656	2659	rBV	170	114	0.01%	0.001%
72	9.973	2681	2685	2691	rBV2	272	331	0.03%	0.004%
73	10.105	2720	2726	2729	rBV3	325	302	0.02%	0.003%
74	10.224	2760	2763	2765	rBV2	209	171	0.01%	0.002%
75	10.288	2780	2783	2785	rBV	137	103	0.01%	0.001%
76	10.304	2785	2788	2792	rVV	176	162	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044790.D
 Acq On : 23 Sep 2021 17:23
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.484	2842	2844	2848	rVB2	163	98	0.01%	0.001%
78	10.578	2871	2873	2876	rBV	173	132	0.01%	0.001%
79	10.674	2896	2903	2912	rVB3	2060	2873	0.23%	0.031%
80	10.761	2917	2930	2949	rBV	396506	635662	51.46%	6.804%
81	10.870	2961	2964	2967	rBV3	207	159	0.01%	0.002%
82	11.102	3034	3036	3040	rVV2	182	103	0.01%	0.001%
83	11.124	3040	3043	3046	rVV2	254	227	0.02%	0.002%
84	11.385	3121	3124	3127	rBV	227	144	0.01%	0.002%
85	11.459	3142	3147	3158	rVB4	1435	2283	0.18%	0.024%
86	11.574	3180	3183	3188	rVB3	268	264	0.02%	0.003%
87	11.697	3216	3221	3225	rBV3	761	841	0.07%	0.009%
88	11.816	3245	3258	3277	rBV	441240	695219	56.29%	7.441%
89	11.944	3296	3298	3302	rBV4	433	333	0.03%	0.004%
90	11.976	3304	3308	3317	rVB4	1594	1865	0.15%	0.020%
91	12.111	3347	3350	3355	rBV2	273	220	0.02%	0.002%
92	12.195	3364	3376	3396	rBV	483221	776339	62.85%	8.309%
93	12.336	3416	3420	3423	rBV2	513	436	0.04%	0.005%
94	12.410	3440	3443	3444	rBV2	336	143	0.01%	0.002%
95	12.635	3511	3513	3514	rBV2	366	190	0.02%	0.002%
96	13.140	3668	3670	3672	rBV	220	135	0.01%	0.001%
97	13.883	3898	3901	3904	rBV2	282	192	0.02%	0.002%
98	14.272	4020	4022	4024	rBV	245	168	0.01%	0.002%
99	14.288	4025	4027	4030	rVB	334	172	0.01%	0.002%
100	14.761	4172	4174	4175	rBV	267	137	0.01%	0.001%




Sum of corrected areas: 9343040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044790.D
Acq On : 23 Sep 2021 17:23
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

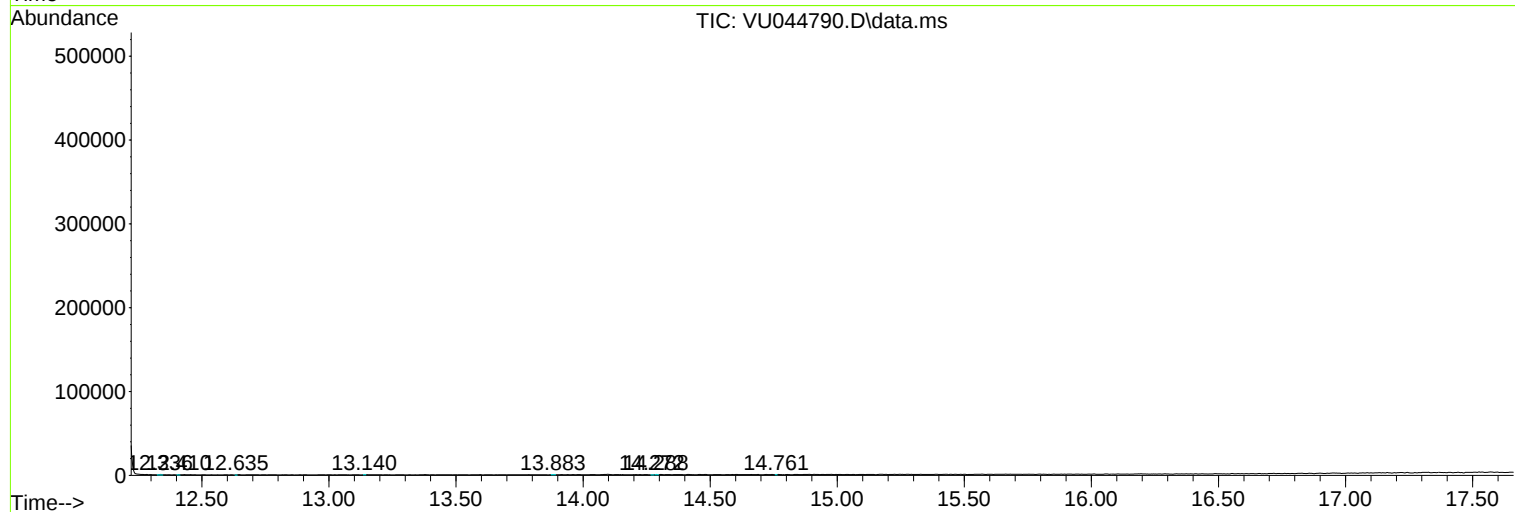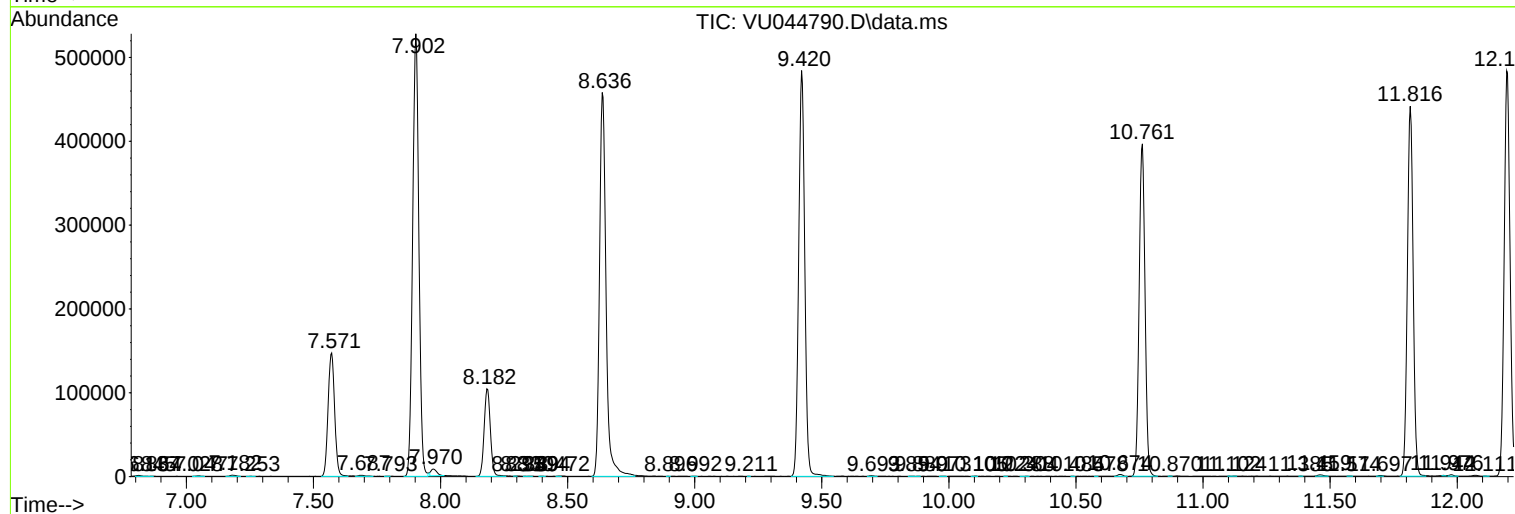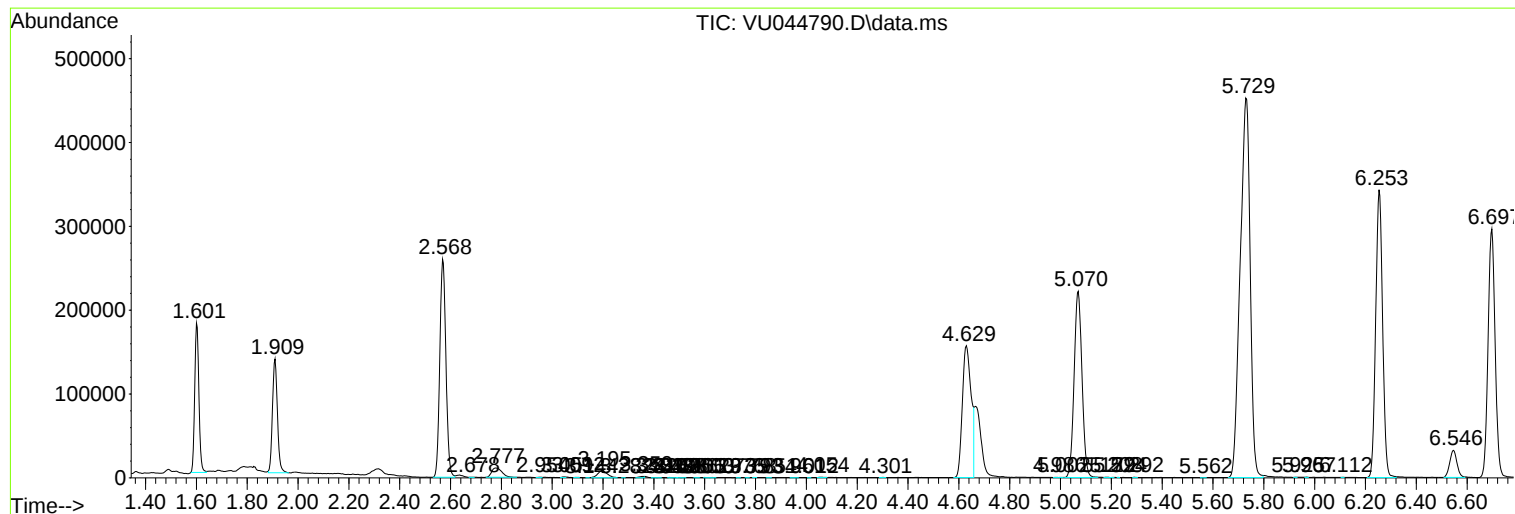

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044790.D
Acq On : 23 Sep 2021 17:23
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
Data File : VU044790.D
Acq On : 23 Sep 2021 17:23
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
