
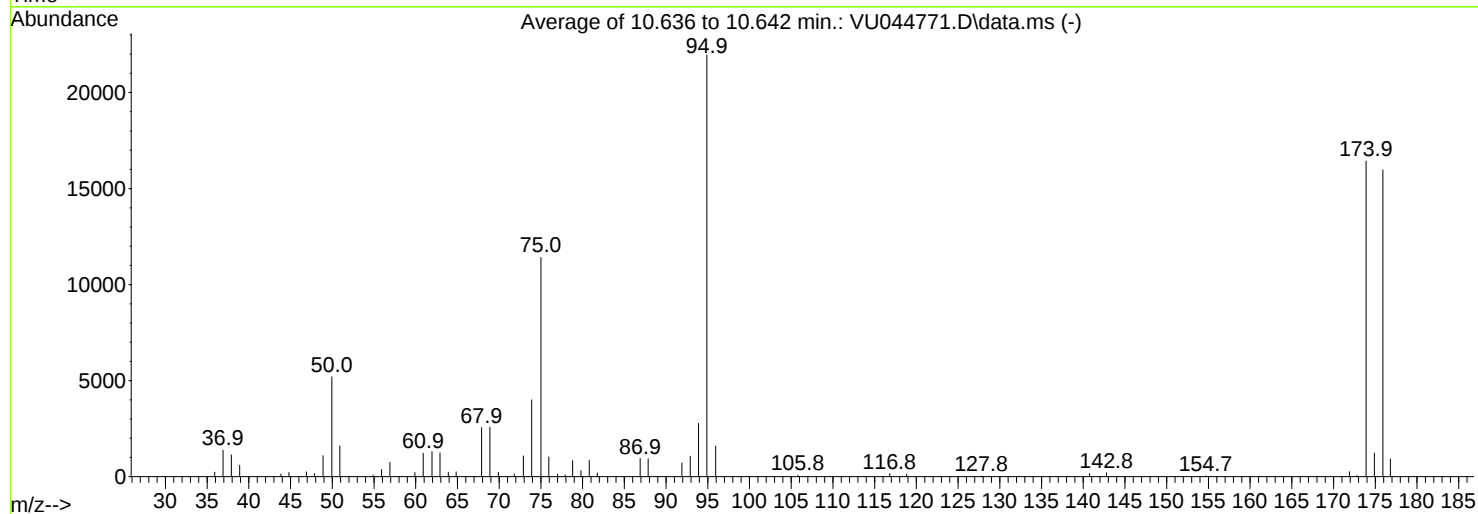


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092321\
 Data File : VU044771.D
 Acq On : 23 Sep 2021 08:54
 Operator : SY/MD
 Sample : BFB003
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB003

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 25 02:36:00 2021

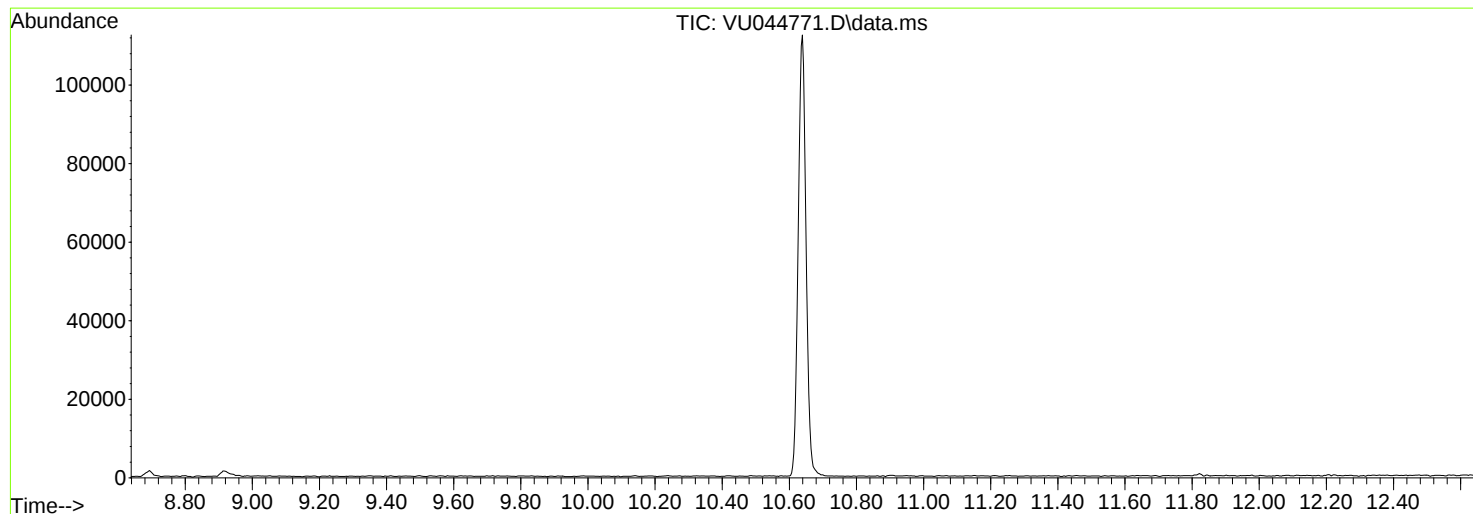

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	5196	PASS
75	95	30	80	52.0	11414	PASS
95	95	100	100	100.0	21963	PASS
96	95	5	9	7.3	1593	PASS
173	174	0.00	2	0.4	62	PASS
174	95	50	120	74.8	16426	PASS
175	174	5	9	7.5	1224	PASS
176	174	95	101	97.2	15968	PASS
177	176	5	9	5.7	918	PASS

Scan 2879 (10.597 min): VU044771.D\data.ms
BFB003

m/z	Abundance
39.80	172.0
43.90	316.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	234.0
36.90	1459.0
37.90	1180.0
38.90	525.0
39.80	134.0
43.90	437.0
44.80	232.0
46.90	232.0
47.80	193.0
48.90	1150.0
50.00	5474.0
50.90	1605.0
54.90	136.0
55.90	369.0
56.90	761.0
59.90	222.0
60.90	1267.0
62.00	1251.0
62.90	1264.0
63.90	213.0
64.80	236.0
67.90	2591.0
68.90	2647.0
69.90	227.0
71.80	129.0
72.90	1115.0
73.90	3995.0
75.00	11564.0
76.00	1024.0
77.00	127.0
77.90	160.0
78.80	844.0
79.80	327.0
80.80	838.0
81.70	208.0
86.90	997.0
87.90	965.0
91.90	711.0
92.90	1027.0
93.90	2839.0
94.90	22136.0
95.90	1713.0
105.80	106.0
116.70	170.0
118.90	145.0
140.80	173.0
142.80	192.0
171.90	258.0
173.90	16384.0
174.90	1173.0
175.90	15614.0
176.80	948.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	245.0
36.90	1441.0
37.90	1167.0
38.90	617.0
39.80	134.0
43.90	461.0
44.80	224.0
46.90	234.0
47.90	164.0
48.90	1106.0
49.90	5379.0
50.90	1682.0
54.90	109.0
55.90	391.0
56.90	769.0
59.90	228.0
60.90	1277.0
61.90	1359.0
62.90	1307.0
63.90	240.0
64.90	250.0
67.90	2618.0
68.90	2639.0
69.90	233.0
71.80	138.0
72.90	1123.0
73.90	4124.0
75.00	11722.0
76.00	1030.0
77.00	126.0
77.90	126.0
78.80	860.0
79.80	333.0
80.80	856.0
81.70	189.0
86.90	968.0
87.80	940.0
91.90	738.0
92.90	1103.0
93.90	2858.0
94.90	22680.0
95.90	1644.0
105.80	101.0
116.80	157.0
118.80	132.0
127.80	106.0
140.70	165.0
142.80	211.0
154.70	103.0
171.90	272.0
173.90	16936.0
174.90	1271.0
175.90	16504.0
176.80	936.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.90	222.0
36.90	1232.0
37.90	1056.0
38.90	631.0
39.80	134.0
43.80	466.0
44.80	198.0
46.90	280.0
47.90	145.0
48.90	1019.0
49.90	4736.0
50.90	1511.0
55.90	376.0
56.90	702.0
59.90	189.0
60.90	1142.0
61.90	1318.0
62.90	1158.0
63.90	234.0
64.90	259.0
67.90	2450.0
68.90	2434.0
69.90	216.0
71.80	142.0
72.90	1004.0
73.90	3879.0
75.00	10957.0
75.90	1014.0
77.00	141.0
78.80	806.0
79.80	285.0
80.80	854.0
81.80	168.0
86.90	876.0
87.80	904.0
91.90	684.0
92.90	1071.0
93.90	2628.0
94.90	21072.0
96.00	1423.0
116.90	162.0
118.80	115.0
140.80	163.0
142.80	220.0
171.90	239.0
172.80	186.0
173.90	15958.0
174.90	1228.0
175.90	15787.0
176.80	869.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003