

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092324\
 Data File : VU060975.D
 Acq On : 23 Sep 2024 15:35
 Operator : MD/SY
 Sample : VIBLK140
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK140

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU060975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	65	71	77	rBV2	3490	4871	1.08%	0.132%
2	1.596	86	95	115	rVB	74614	89956	19.94%	2.431%
3	1.911	183	193	206	rBV	53386	75789	16.80%	2.048%
4	2.557	380	394	410	rVB	110687	183470	40.67%	4.958%
5	3.036	535	543	556	rVB3	3067	5534	1.23%	0.150%
6	3.174	575	586	603	rBV	3824	8070	1.79%	0.218%
7	4.644	1029	1043	1078	rBV2	51200	154077	34.16%	4.164%
8	5.055	1156	1171	1192	rBV2	87531	193373	42.87%	5.226%
9	5.718	1354	1377	1402	rBV3	174004	451081	100.00%	12.190%
10	6.242	1527	1540	1560	rBV	160548	309873	68.70%	8.374%
11	6.538	1622	1632	1647	rBV6	11818	23985	5.32%	0.648%
12	6.682	1664	1677	1699	rBV	107377	209823	46.52%	5.670%
13	7.560	1934	1950	1964	rBV	48146	85982	19.06%	2.324%
14	7.891	2041	2053	2078	rBV	192123	345488	76.59%	9.336%
15	8.177	2127	2142	2159	rBV3	28301	50664	11.23%	1.369%
16	8.634	2273	2284	2321	rBV2	182361	407005	90.23%	10.999%
17	9.412	2514	2526	2553	rBV	224829	394241	87.40%	10.654%
18	10.750	2927	2942	2957	rBV	79697	131442	29.14%	3.552%
19	10.888	2971	2985	2995	rVB2	3197	5461	1.21%	0.148%
20	11.807	3259	3271	3290	rBV	183131	298920	66.27%	8.078%
21	12.187	3376	3389	3410	rBV	154247	259741	57.58%	7.019%
22	12.762	3558	3568	3578	rBV3	3153	4646	1.03%	0.126%
23	14.569	4120	4130	4140	rVB2	4311	6968	1.54%	0.188%




Sum of corrected areas: 3700460

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092324\
Data File : VU060975.D
Acq On : 23 Sep 2024 15:35
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

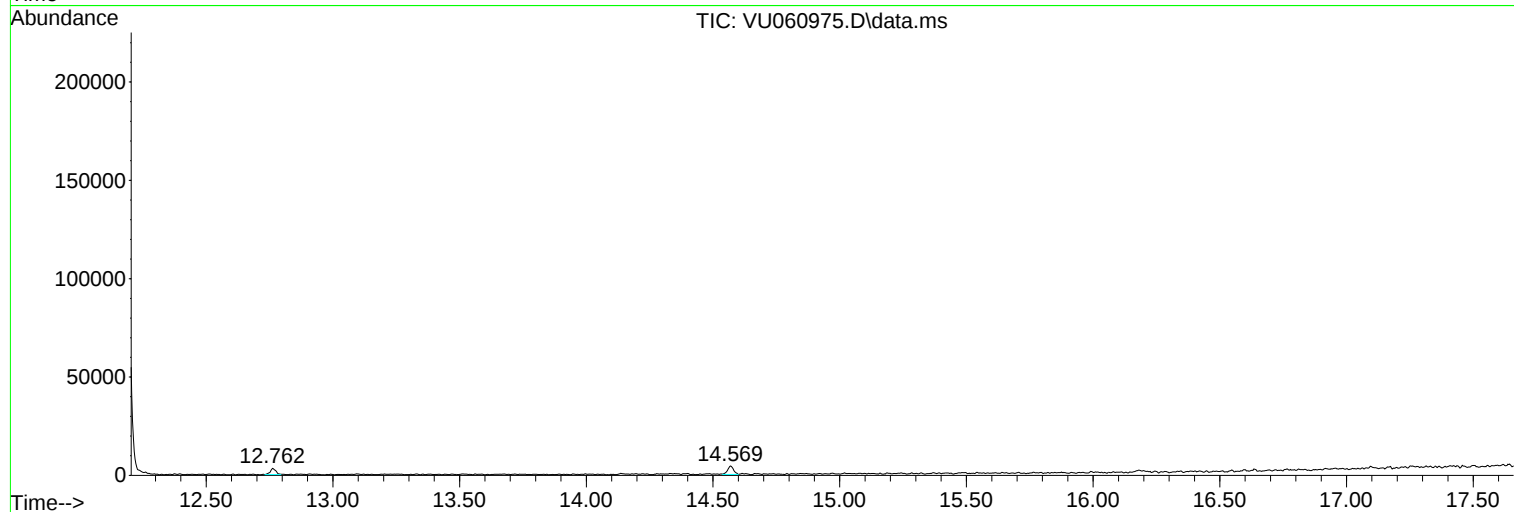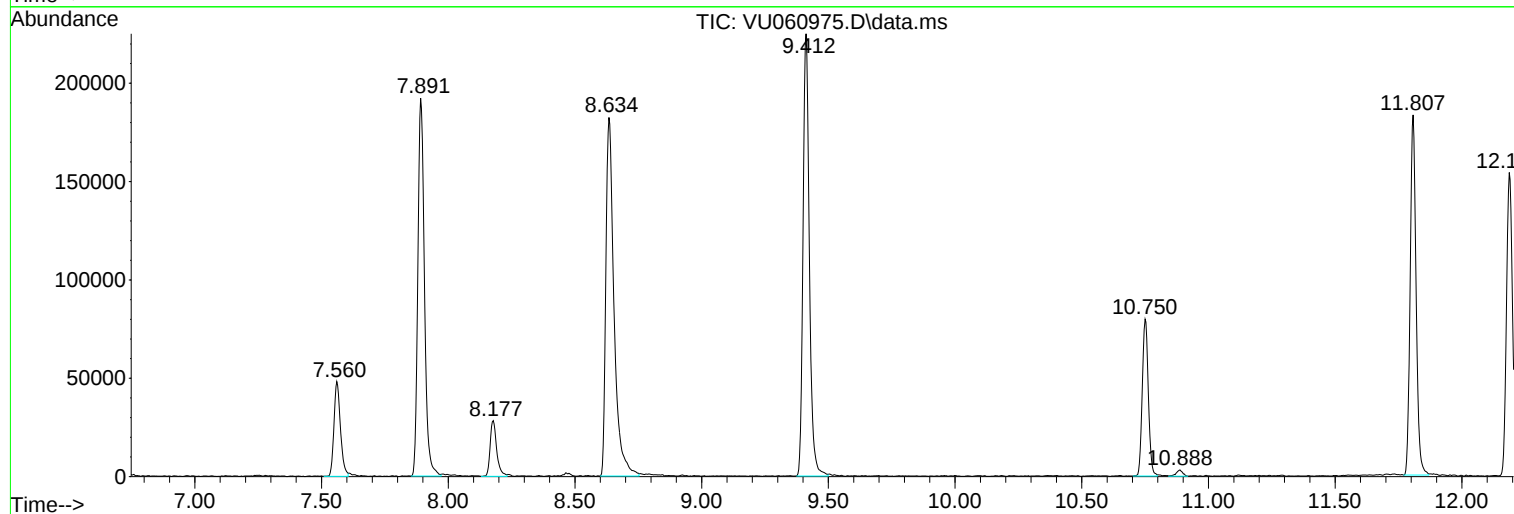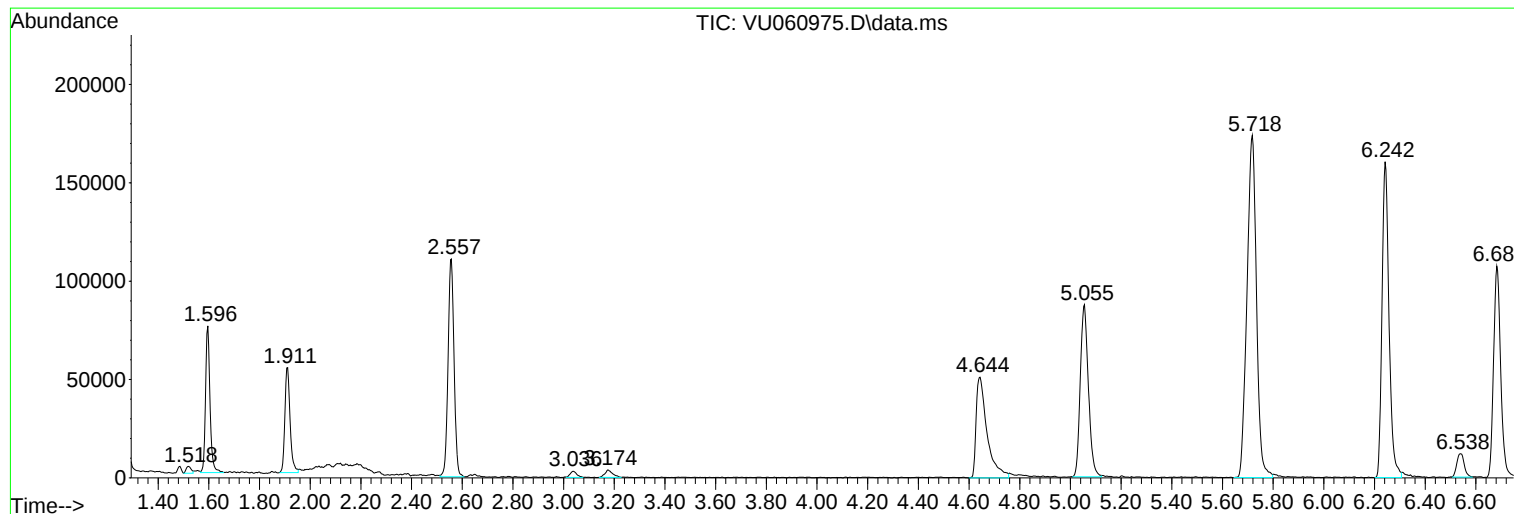

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092324\
Data File : VU060975.D
Acq On : 23 Sep 2024 15:35
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092324\
Data File : VU060975.D
Acq On : 23 Sep 2024 15:35
Operator : MD/SY
Sample : VIBLK140
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK140

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------