


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092324\
Data File : VU060963.D
Acq On : 23 Sep 2024 08:20
Operator : MD/SY
Sample : BFB003
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB003

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 25 04:46:41 2024

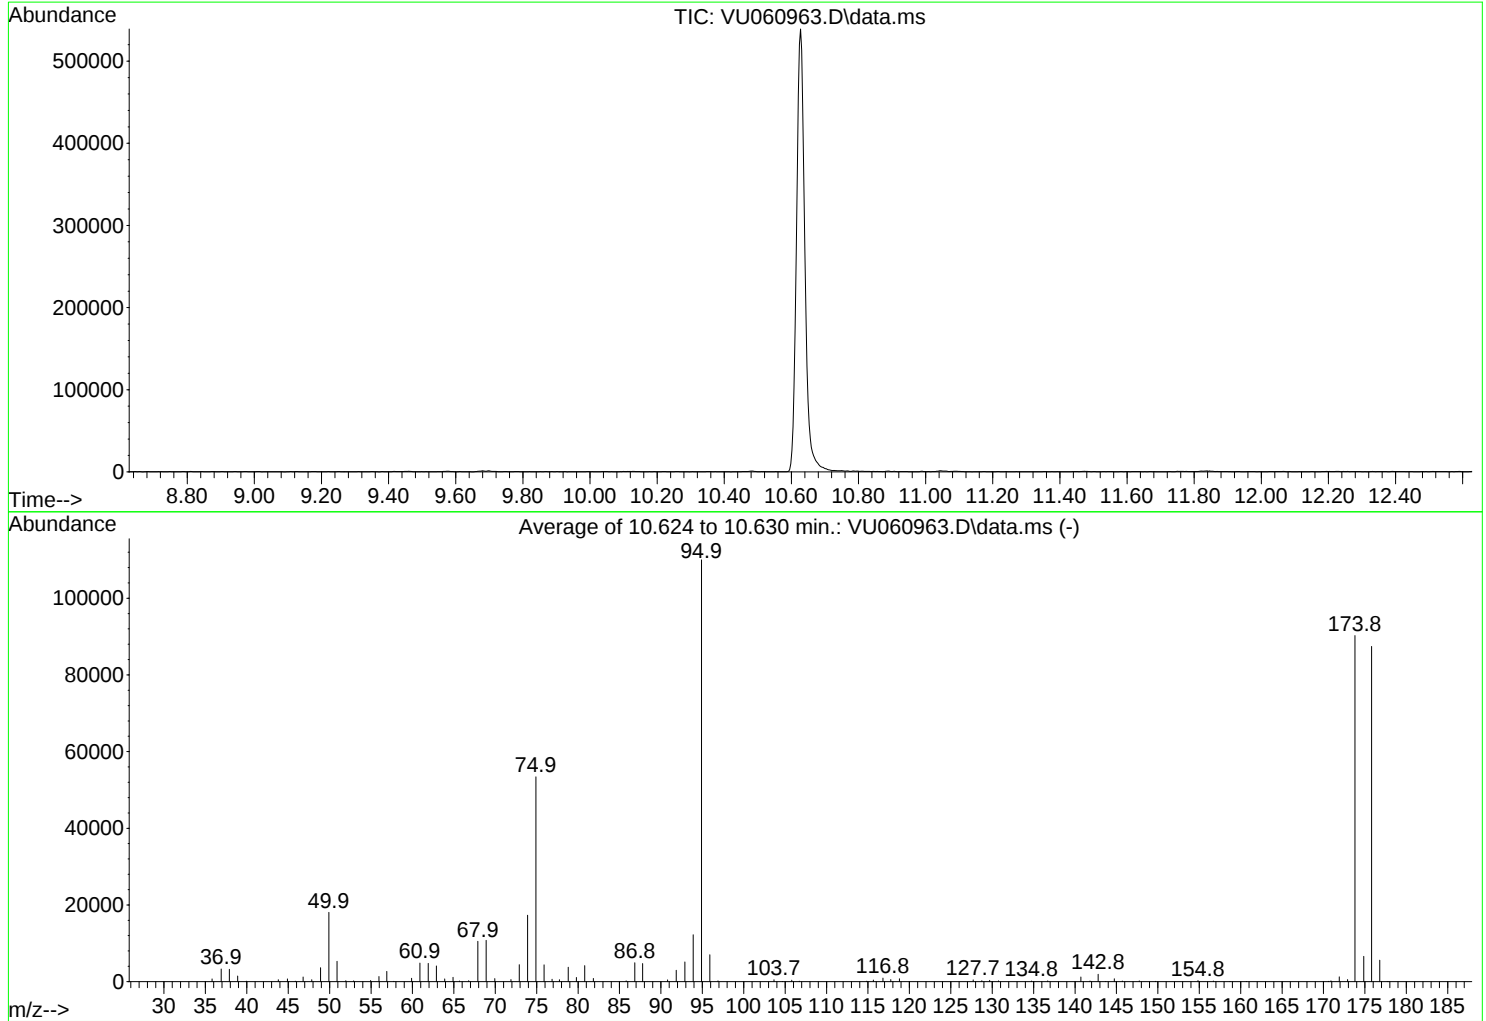

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.4	18064	PASS
75	95	30	80	48.6	53432	PASS
95	95	100	100	100.0	110013	PASS
96	95	5	9	6.4	7020	PASS
173	174	0.00	2	0.6	545	PASS
174	95	50	120	82.1	90277	PASS
175	174	5	9	7.3	6603	PASS
176	174	95	101	96.8	87408	PASS
177	176	5	9	6.4	5584	PASS

m/z	Abundance
43.80	216.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.80	726.0
36.90	3555.0
37.90	3318.0
38.90	1439.0
39.90	180.0
43.90	809.0
44.90	714.0
45.90	106.0
46.80	1468.0
47.80	543.0
48.90	3548.0
49.90	18304.0
50.90	5547.0
51.90	276.0
52.90	138.0
55.00	312.0
55.90	1393.0
56.90	2562.0
57.80	113.0
59.90	879.0
60.90	4643.0
61.90	4605.0
62.90	4429.0
63.90	779.0
64.90	1192.0
65.70	121.0
66.80	263.0
67.90	10665.0
68.90	10572.0
70.00	822.0
71.90	571.0
72.90	4356.0
73.90	17872.0
74.90	53152.0
75.90	4273.0
76.90	685.0
77.70	502.0
78.80	3810.0
79.80	1099.0
80.80	3987.0
81.80	751.0
85.80	200.0
86.90	4824.0
87.80	4641.0
90.80	448.0
91.90	2884.0
92.90	4885.0
93.90	12575.0
94.90	108160.0
95.90	7175.0
96.90	199.0
103.60	576.0
104.70	107.0
105.80	385.0
106.80	122.0
114.80	106.0
115.70	447.0
116.80	907.0
117.70	508.0
118.80	738.0
127.70	425.0
128.80	276.0
129.70	367.0
130.70	192.0
134.70	189.0
136.70	221.0
140.70	1253.0
141.80	154.0
142.80	1803.0
144.80	680.0
145.70	179.0
147.80	211.0
154.90	300.0
156.70	158.0
170.90	283.0
171.90	1295.0
172.90	1634.0
173.80	87848.0
174.90	6410.0
175.80	85840.0
176.80	5768.0
177.70	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.80	739.0
36.90	3360.0
37.90	3291.0
38.90	1505.0
39.90	126.0
43.90	701.0
44.90	762.0
45.80	112.0
46.80	1287.0
47.90	500.0
48.90	3779.0
49.90	18696.0
50.90	5434.0
51.90	229.0
52.90	215.0
54.90	322.0
56.00	1356.0
56.90	2773.0
57.70	121.0
59.90	911.0
60.90	4915.0
61.90	4929.0
62.90	4223.0
63.90	775.0
64.90	1126.0
65.70	180.0
66.80	243.0
67.90	10868.0
68.90	11032.0
69.90	800.0
71.90	537.0
72.90	4587.0
73.90	17696.0
74.90	55016.0
75.90	4422.0
76.80	655.0
77.70	506.0
78.80	3795.0
79.80	1090.0
80.80	4287.0
81.80	858.0
85.80	229.0
86.90	5135.0
87.80	4944.0
90.80	467.0
91.80	3059.0
92.90	5364.0
93.90	12469.0
94.90	113488.0
95.90	7196.0
96.90	203.0
103.70	494.0
105.80	367.0
106.70	124.0
114.80	126.0
115.60	405.0
116.80	979.0
117.70	563.0
118.80	744.0
127.70	460.0
128.70	278.0
129.70	338.0
130.70	234.0
134.70	183.0
136.70	222.0
140.70	1259.0
141.80	160.0
142.80	2019.0
144.70	782.0
145.70	174.0
147.70	203.0
149.70	117.0
154.90	324.0
156.70	177.0
158.70	107.0
170.90	339.0
171.90	1250.0
173.80	92808.0
174.80	6759.0
175.80	89856.0
176.80	5792.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003

m/z	Abundance
35.80	631.0
36.90	2968.0
37.90	3007.0
38.90	1486.0
40.00	102.0
43.80	638.0
44.90	710.0
45.80	119.0
46.80	948.0
47.90	444.0
48.90	3603.0
49.90	17192.0
50.90	4905.0
52.00	238.0
52.90	233.0
54.90	260.0
56.00	1259.0
56.90	2648.0
59.90	815.0
60.90	4927.0
61.90	4704.0
62.90	3641.0
63.90	631.0
64.90	1045.0
65.70	159.0
66.80	245.0
67.90	9985.0
68.90	10665.0
69.90	782.0
71.90	515.0
72.90	4352.0
73.90	16416.0
74.90	52128.0
75.90	4464.0
76.80	585.0
77.80	480.0
78.80	3683.0
79.80	1029.0
80.80	4273.0
81.90	888.0
85.80	198.0
86.80	4787.0
87.80	4582.0
90.80	461.0
91.90	2994.0
92.90	5174.0
93.90	11614.0
94.90	108392.0
95.90	6688.0
96.90	175.0
103.70	441.0
105.80	369.0
106.60	118.0
114.90	120.0
115.60	352.0
116.80	884.0
117.80	511.0
118.80	726.0
127.70	434.0
128.70	212.0
129.70	325.0
130.80	201.0
134.80	183.0
136.70	227.0
140.70	1118.0
141.80	150.0
142.80	2000.0
143.70	107.0
144.80	777.0
145.70	138.0
147.70	213.0
149.70	108.0
154.80	322.0
156.70	207.0
160.70	158.0
170.60	317.0
171.90	1191.0
173.80	90176.0
174.80	6639.0
175.80	86528.0
176.80	5191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB003