

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063625.D
 Acq On : 23 Sep 2025 10:31
 Operator : MD/SY
 Sample : VU0923MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M

Title : VOC Analysis

Signal : TIC: VU063625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	104	rBV	117763	129353	15.03%	1.964%
2	1.779	138	152	159	rBV2	27087	50535	5.87%	0.767%
3	1.898	180	189	202	rVB	94759	129085	15.00%	1.960%
4	2.554	380	393	413	rBV	162041	275047	31.95%	4.177%
5	2.692	433	436	440	rVB2	380	358	0.04%	0.005%
6	2.714	440	443	448	rVB3	562	360	0.04%	0.005%
7	2.759	453	457	458	rBV2	831	519	0.06%	0.008%
8	2.972	518	523	526	rBV	392	375	0.04%	0.006%
9	3.033	533	542	552	rVB3	2734	5182	0.60%	0.079%
10	3.078	552	556	561	rVB2	222	214	0.02%	0.003%
11	3.139	572	575	578	rBV	291	240	0.03%	0.004%
12	3.181	578	588	593	rVV3	787	1338	0.16%	0.020%
13	3.296	620	624	625	rBV	268	205	0.02%	0.003%
14	3.351	636	641	648	rBV4	479	680	0.08%	0.010%
15	3.499	683	687	690	rVB3	213	171	0.02%	0.003%
16	3.521	692	694	701	rVB	265	246	0.03%	0.004%
17	3.566	705	708	712	rVB2	264	172	0.02%	0.003%
18	3.592	713	716	719	rBV	252	175	0.02%	0.003%
19	3.740	759	762	767	rVB2	280	185	0.02%	0.003%
20	3.917	813	817	819	rBV	369	278	0.03%	0.004%
21	3.933	819	822	828	rVV3	368	396	0.05%	0.006%
22	4.132	881	884	888	rVB2	267	196	0.02%	0.003%
23	4.242	915	918	923	rVB2	266	195	0.02%	0.003%
24	4.447	978	982	986	rBV	344	274	0.03%	0.004%
25	4.615	1025	1034	1067	rBV	68599	181466	21.08%	2.756%
26	5.045	1153	1168	1200	rBV	149449	344782	40.05%	5.236%
27	5.258	1231	1234	1237	rVB	385	252	0.03%	0.004%
28	5.280	1237	1241	1242	rBV	247	168	0.02%	0.003%
29	5.357	1257	1265	1267	rBV2	478	452	0.05%	0.007%
30	5.386	1270	1274	1276	rVV3	413	329	0.04%	0.005%
31	5.467	1291	1299	1305	rVB2	346	466	0.05%	0.007%
32	5.499	1305	1309	1314	rBV2	363	323	0.04%	0.005%
33	5.534	1316	1320	1323	rVV2	313	273	0.03%	0.004%
34	5.711	1355	1375	1408	rBV2	290126	860804	100.00%	13.073%
35	5.991	1460	1462	1467	rVB	454	269	0.03%	0.004%
36	6.013	1467	1469	1474	rBV2	272	169	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063625.D
 Acq On : 23 Sep 2025 10:31
 Operator : MD/SY
 Sample : VU0923MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
 Title : VOC Analysis

37	6.042	1475	1478	1481	rBV3	398	221	0.03%	0.003%
38	6.126	1501	1504	1507	rVB2	412	281	0.03%	0.004%
39	6.142	1507	1509	1511	rBV2	307	167	0.02%	0.003%
40	6.238	1525	1539	1580	rBV	264352	563976	65.52%	8.565%
41	6.531	1620	1630	1646	rVB10	4227	8915	1.04%	0.135%
42	6.634	1658	1662	1663	rBV2	297	190	0.02%	0.003%
43	6.679	1663	1676	1703	rBV	188911	391035	45.43%	5.939%
44	6.798	1711	1713	1715	rBV2	568	331	0.04%	0.005%
45	6.875	1735	1737	1740	rVB2	435	196	0.02%	0.003%
46	7.071	1793	1798	1802	rBV	367	290	0.03%	0.004%
47	7.148	1819	1822	1825	rBV2	344	242	0.03%	0.004%
48	7.196	1833	1837	1838	rBV2	457	218	0.03%	0.003%
49	7.415	1903	1905	1911	rVB2	385	332	0.04%	0.005%
50	7.447	1912	1915	1917	rBV	265	188	0.02%	0.003%
51	7.553	1938	1948	1969	rBV	75066	141864	16.48%	2.155%
52	7.692	1989	1991	1995	rVB2	325	166	0.02%	0.003%
53	7.795	2020	2023	2024	rBV	403	230	0.03%	0.003%
54	7.888	2040	2052	2085	rBV	344429	660022	76.68%	10.024%
55	8.171	2129	2140	2156	rBV	47892	86396	10.04%	1.312%
56	8.376	2200	2204	2206	rBV2	240	180	0.02%	0.003%
57	8.393	2206	2209	2213	rVV2	259	261	0.03%	0.004%
58	8.412	2213	2215	2221	rVB2	427	372	0.04%	0.006%
59	8.441	2221	2224	2230	rBV2	232	213	0.02%	0.003%
60	8.534	2250	2253	2258	rBV	252	177	0.02%	0.003%
61	8.553	2258	2259	2267	rVB2	243	170	0.02%	0.003%
62	8.624	2271	2281	2332	rBV2	174937	389047	45.20%	5.908%
63	8.987	2391	2394	2398	rBV3	298	279	0.03%	0.004%
64	9.135	2438	2440	2446	rVB2	317	214	0.02%	0.003%
65	9.187	2454	2456	2460	rBV3	318	219	0.03%	0.003%
66	9.409	2512	2525	2568	rBV	376565	702598	81.62%	10.670%
67	9.672	2604	2607	2610	rBV	330	286	0.03%	0.004%
68	9.936	2683	2689	2695	rBV2	352	454	0.05%	0.007%
69	10.065	2726	2729	2734	rBV	281	208	0.02%	0.003%
70	10.100	2737	2740	2746	rVB2	541	418	0.05%	0.006%
71	10.293	2797	2800	2802	rBV2	340	226	0.03%	0.003%
72	10.386	2823	2829	2833	rBV	370	350	0.04%	0.005%
73	10.492	2859	2862	2866	rVB2	578	412	0.05%	0.006%
74	10.663	2912	2915	2922	rBV2	209	182	0.02%	0.003%
75	10.746	2928	2941	2960	rBV	262840	440746	51.20%	6.694%
76	10.926	2994	2997	2999	rVB	346	232	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063625.D
 Acq On : 23 Sep 2025 10:31
 Operator : MD/SY
 Sample : VU0923MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
 Title : VOC Analysis

77	10.952	2999	3005	3009	rVB2	316	304	0.04%	0.005%
78	11.087	3043	3047	3048	rBV2	530	339	0.04%	0.005%
79	11.135	3060	3062	3068	rVB2	372	326	0.04%	0.005%
80	11.257	3097	3100	3103	rVB	295	192	0.02%	0.003%
81	11.280	3104	3107	3110	rBV2	303	218	0.03%	0.003%
82	11.753	3247	3254	3258	rVB4	1344	1619	0.19%	0.025%
83	11.804	3258	3270	3297	rBV	356387	617986	71.79%	9.385%
84	12.016	3334	3336	3345	rVB2	607	500	0.06%	0.008%
85	12.061	3348	3350	3355	rVV2	421	374	0.04%	0.006%
86	12.183	3376	3388	3410	rBV	327135	564455	65.57%	8.572%
87	12.515	3488	3491	3496	rVB2	242	188	0.02%	0.003%
88	12.608	3517	3520	3525	rBV2	239	208	0.02%	0.003%
89	12.679	3539	3542	3545	rVB2	475	374	0.04%	0.006%
90	12.794	3574	3578	3581	rBV2	250	228	0.03%	0.003%
91	13.132	3681	3683	3688	rVB2	427	283	0.03%	0.004%
92	13.154	3688	3690	3693	rBV	403	178	0.02%	0.003%
93	13.235	3708	3715	3724	rVB5	959	1630	0.19%	0.025%
94	13.457	3781	3784	3787	rVB	346	171	0.02%	0.003%
95	13.855	3902	3908	3923	rVB7	2309	4130	0.48%	0.063%
96	14.106	3980	3986	4005	rVB4	3601	7699	0.89%	0.117%
97	14.222	4020	4022	4024	rBV2	405	223	0.03%	0.003%
98	14.334	4050	4057	4071	rBV4	2562	4286	0.50%	0.065%
99	14.894	4228	4231	4232	rBV	382	209	0.02%	0.003%
100	14.955	4247	4250	4253	rBV	586	375	0.04%	0.006%




Sum of corrected areas: 6584531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063625.D
Acq On : 23 Sep 2025 10:31
Operator : MD/SY
Sample : VU0923MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

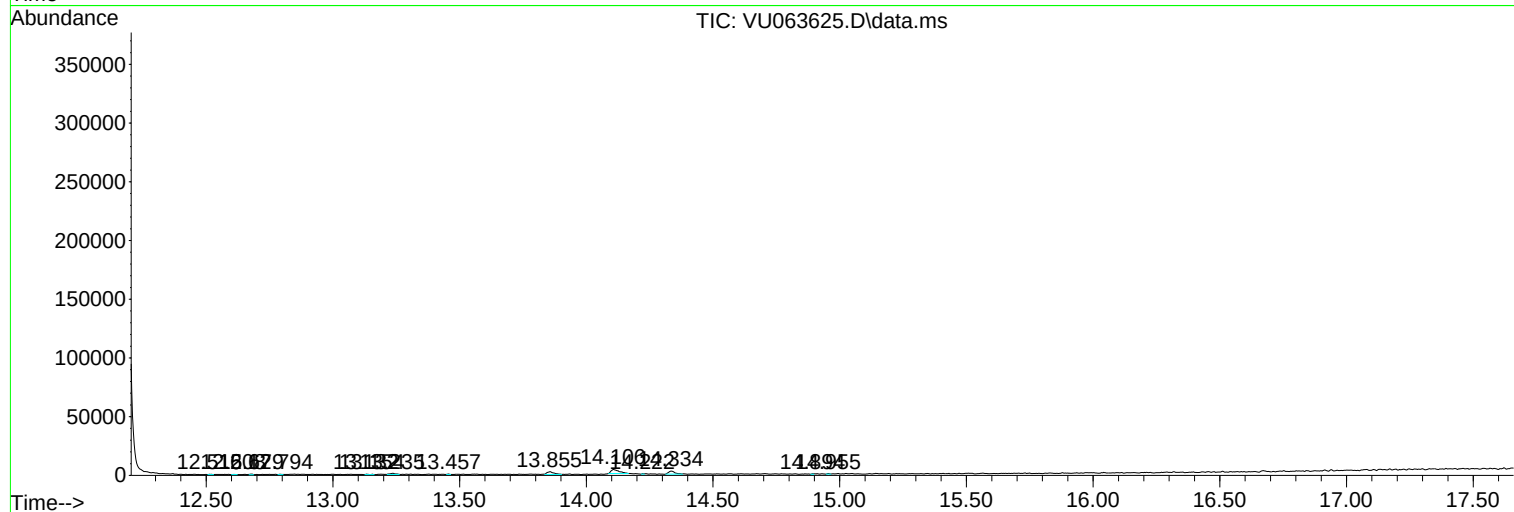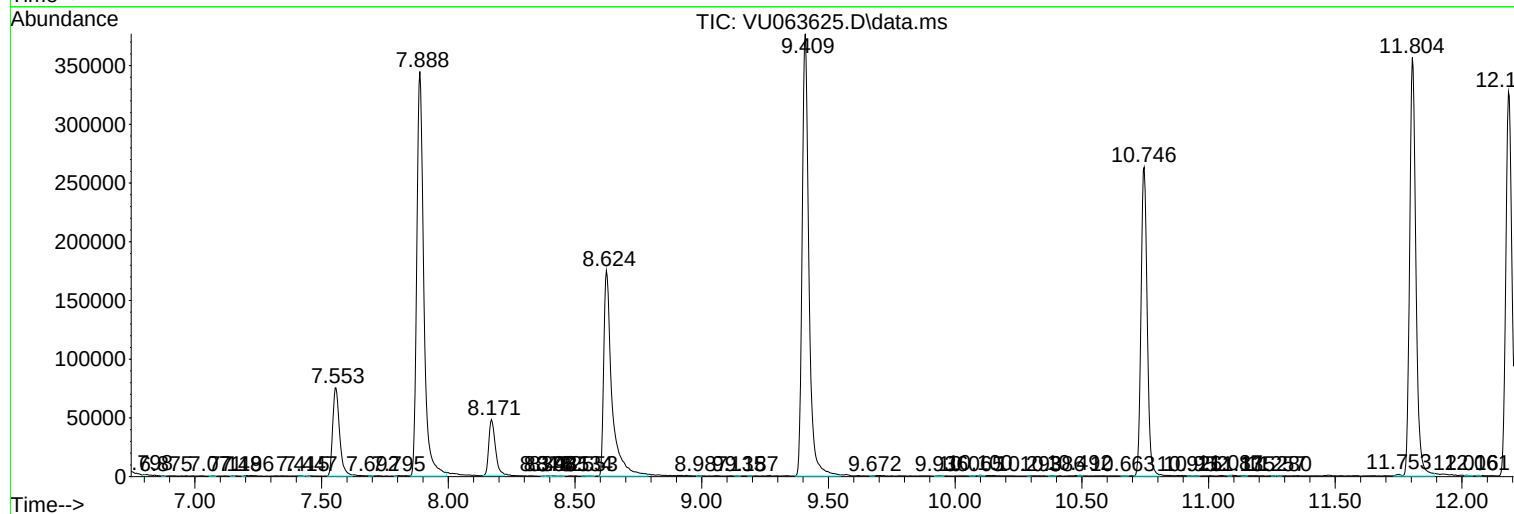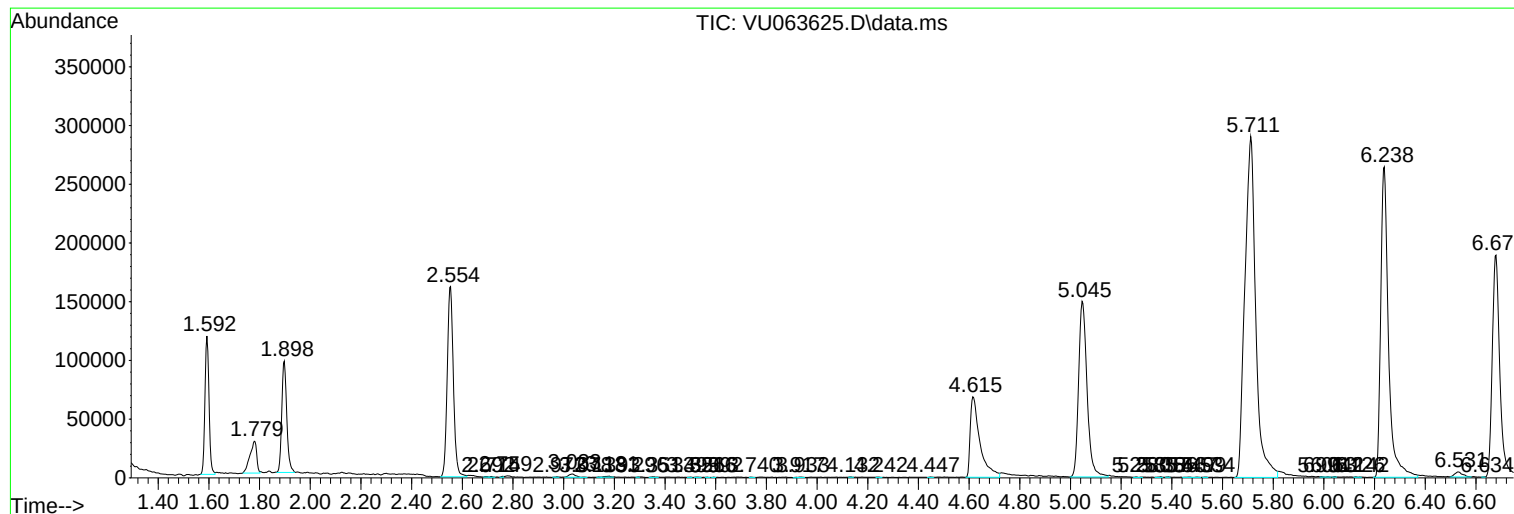

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063625.D
Acq On : 23 Sep 2025 10:31
Operator : MD/SY
Sample : VU0923MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063625.D
Acq On : 23 Sep 2025 10:31
Operator : MD/SY
Sample : VU0923MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc