

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063626.D
 Acq On : 23 Sep 2025 10:56
 Operator : MD/SY
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M

Title : VOC Analysis

Signal : TIC: VU063626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	104	rBV	112326	123402	14.69%	1.903%
2	1.782	140	153	161	rVB	24455	47264	5.63%	0.729%
3	1.895	181	188	205	rVB	92469	126931	15.11%	1.957%
4	2.551	379	392	410	rBV	159307	267442	31.83%	4.124%
5	2.721	442	445	449	rBV2	326	232	0.03%	0.004%
6	2.776	455	462	466	rBV3	734	860	0.10%	0.013%
7	2.924	505	508	512	rBV2	329	227	0.03%	0.004%
8	2.978	523	525	530	rVB2	323	212	0.03%	0.003%
9	3.030	532	541	552	rVV4	2991	5333	0.63%	0.082%
10	3.174	576	586	597	rVB4	1265	2565	0.31%	0.040%
11	3.409	655	659	664	rBV2	175	207	0.02%	0.003%
12	3.454	669	673	676	rBV2	341	304	0.04%	0.005%
13	3.772	768	772	775	rBV	314	258	0.03%	0.004%
14	3.898	804	811	814	rBV2	198	266	0.03%	0.004%
15	4.149	883	889	893	rBV2	239	281	0.03%	0.004%
16	4.239	913	917	923	rBV2	205	232	0.03%	0.004%
17	4.615	1026	1034	1076	rBV	69733	193030	22.97%	2.976%
18	4.920	1126	1129	1132	rVB3	629	369	0.04%	0.006%
19	4.943	1132	1136	1139	rBV4	572	406	0.05%	0.006%
20	5.049	1153	1169	1202	rBV	142997	329363	39.20%	5.078%
21	5.258	1230	1234	1236	rBV	305	209	0.02%	0.003%
22	5.528	1313	1318	1321	rVB3	267	227	0.03%	0.004%
23	5.711	1355	1375	1407	rBV2	282280	840230	100.00%	12.956%
24	5.959	1449	1452	1455	rBV2	404	297	0.04%	0.005%
25	5.997	1460	1464	1466	rBV	387	300	0.04%	0.005%
26	6.103	1494	1497	1502	rVB3	388	351	0.04%	0.005%
27	6.136	1502	1507	1510	rBV2	231	228	0.03%	0.004%
28	6.158	1510	1514	1517	rBV2	285	220	0.03%	0.003%
29	6.238	1527	1539	1569	rBV	257547	537589	63.98%	8.289%
30	6.467	1608	1610	1615	rVB	470	219	0.03%	0.003%
31	6.528	1619	1629	1633	rBV3	4342	7336	0.87%	0.113%
32	6.679	1663	1676	1711	rVV2	182264	381115	45.36%	5.876%
33	7.055	1788	1793	1799	rBV2	295	396	0.05%	0.006%
34	7.168	1820	1828	1831	rVB3	377	418	0.05%	0.006%
35	7.206	1836	1840	1842	rBV2	273	203	0.02%	0.003%
36	7.258	1852	1856	1863	rVB3	321	371	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063626.D
 Acq On : 23 Sep 2025 10:56
 Operator : MD/SY
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
 Title : VOC Analysis

37	7.303	1868	1870	1873	rBV3	430	340	0.04%	0.005%
38	7.338	1877	1881	1885	rBV2	287	215	0.03%	0.003%
39	7.557	1937	1949	1971	rBV2	75204	139851	16.64%	2.156%
40	7.804	2023	2026	2031	rVV2	343	255	0.03%	0.004%
41	7.888	2039	2052	2074	rBV	342206	642410	76.46%	9.905%
42	8.171	2130	2140	2159	rVV2	49111	85565	10.18%	1.319%
43	8.502	2238	2243	2245	rBV2	353	325	0.04%	0.005%
44	8.553	2257	2259	2264	rVB3	531	251	0.03%	0.004%
45	8.589	2264	2270	2271	rBV2	251	224	0.03%	0.003%
46	8.624	2271	2281	2318	rBV2	182616	396816	47.23%	6.119%
47	8.943	2377	2380	2385	rVB	486	361	0.04%	0.006%
48	9.004	2396	2399	2401	rBV3	410	204	0.02%	0.003%
49	9.033	2405	2408	2414	rBV2	329	360	0.04%	0.006%
50	9.148	2442	2444	2447	rVB2	475	202	0.02%	0.003%
51	9.161	2447	2448	2453	rVB2	454	258	0.03%	0.004%
52	9.190	2453	2457	2459	rBV2	386	331	0.04%	0.005%
53	9.348	2503	2506	2511	rVB3	351	254	0.03%	0.004%
54	9.409	2511	2525	2561	rBV	380488	693040	82.48%	10.686%
55	9.698	2609	2615	2618	rBV4	698	718	0.09%	0.011%
56	9.795	2641	2645	2647	rBV	281	214	0.03%	0.003%
57	9.875	2668	2670	2674	rBV2	279	254	0.03%	0.004%
58	9.962	2694	2697	2701	rVB	281	212	0.03%	0.003%
59	10.078	2730	2733	2737	rVB	360	245	0.03%	0.004%
60	10.113	2737	2744	2747	rBV4	497	565	0.07%	0.009%
61	10.135	2747	2751	2754	rVB2	254	253	0.03%	0.004%
62	10.161	2754	2759	2762	rBV3	279	255	0.03%	0.004%
63	10.245	2782	2785	2790	rVB	293	228	0.03%	0.004%
64	10.489	2859	2861	2863	rVV3	495	321	0.04%	0.005%
65	10.743	2928	2940	2962	rBV	263437	441275	52.52%	6.804%
66	10.926	2995	2997	3003	rVB4	348	314	0.04%	0.005%
67	11.090	3045	3048	3049	rBV	435	229	0.03%	0.004%
68	11.100	3049	3051	3055	rVB	448	293	0.03%	0.005%
69	11.123	3055	3058	3060	rBV2	266	203	0.02%	0.003%
70	11.168	3069	3072	3075	rBV	337	229	0.03%	0.004%
71	11.235	3087	3093	3098	rBV	299	428	0.05%	0.007%
72	11.267	3098	3103	3107	rVB2	398	453	0.05%	0.007%
73	11.383	3136	3139	3144	rBV	300	269	0.03%	0.004%
74	11.444	3153	3158	3161	rBV2	309	323	0.04%	0.005%
75	11.476	3161	3168	3174	rVB3	857	1263	0.15%	0.019%
76	11.746	3245	3252	3258	rBV4	1172	1432	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
 Data File : VU063626.D
 Acq On : 23 Sep 2025 10:56
 Operator : MD/SY
 Sample : VU0923WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
 Title : VOC Analysis

77	11.804	3258	3270	3295	rBV	361188	624182	74.29%	9.624%
78	12.036	3340	3342	3346	rBV2	312	241	0.03%	0.004%
79	12.184	3376	3388	3414	rBV	322998	569642	67.80%	8.783%
80	12.405	3455	3457	3461	rVB3	341	210	0.02%	0.003%
81	12.431	3461	3465	3468	rBV3	356	283	0.03%	0.004%
82	12.492	3480	3484	3487	rBV4	402	357	0.04%	0.006%
83	12.560	3502	3505	3506	rBV	563	251	0.03%	0.004%
84	12.733	3556	3559	3564	rBV2	252	210	0.02%	0.003%
85	12.846	3591	3594	3600	rBV	361	364	0.04%	0.006%
86	13.164	3687	3693	3698	rBV2	327	474	0.06%	0.007%
87	13.238	3713	3716	3722	rVB2	584	483	0.06%	0.007%
88	13.621	3830	3835	3838	rBV3	261	231	0.03%	0.004%
89	13.852	3904	3907	3918	rBV4	1340	1796	0.21%	0.028%
90	13.984	3945	3948	3952	rBV	396	306	0.04%	0.005%
91	14.058	3965	3971	3974	rBV2	502	606	0.07%	0.009%
92	14.077	3974	3977	3979	rVV3	338	212	0.03%	0.003%
93	14.119	3984	3990	3991	rBV3	1413	1477	0.18%	0.023%
94	14.280	4033	4040	4043	rBV3	391	494	0.06%	0.008%
95	14.338	4053	4058	4062	rBV6	1625	1594	0.19%	0.025%
96	14.524	4113	4116	4121	rVB3	514	389	0.05%	0.006%
97	14.659	4156	4158	4160	rBV2	449	226	0.03%	0.003%
98	15.598	4448	4450	4456	rBV4	545	432	0.05%	0.007%
99	15.730	4488	4491	4497	rVB2	639	538	0.06%	0.008%
100	15.852	4527	4529	4531	rBV2	585	323	0.04%	0.005%




Sum of corrected areas: 6485452

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063626.D
Acq On : 23 Sep 2025 10:56
Operator : MD/SY
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

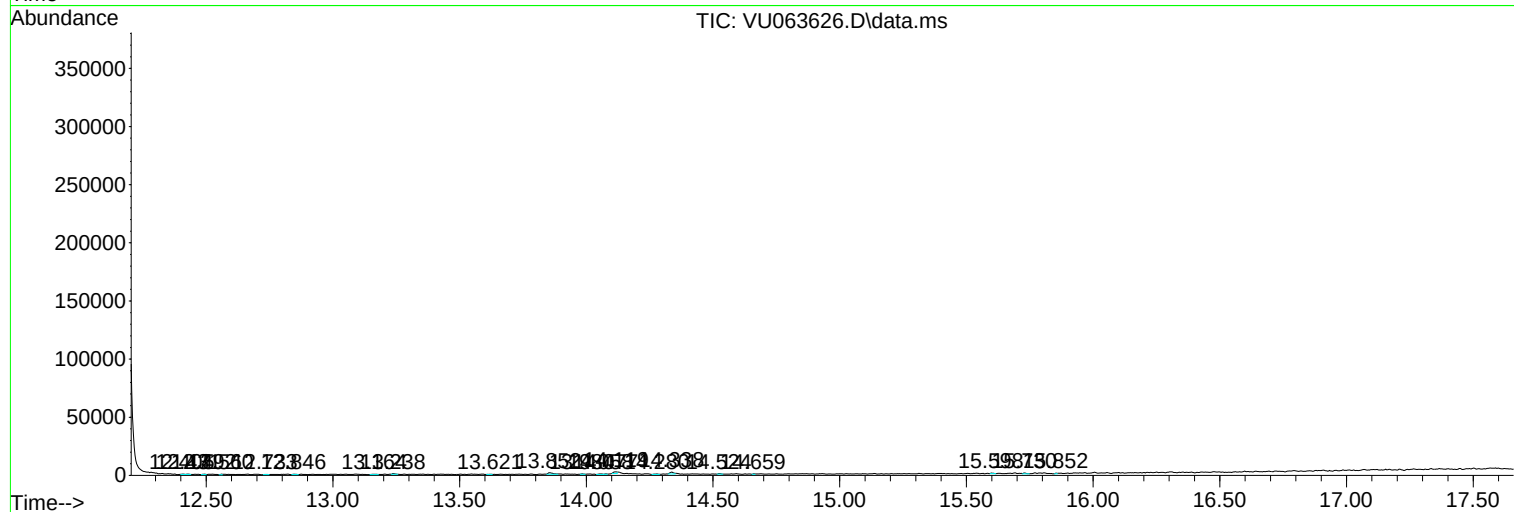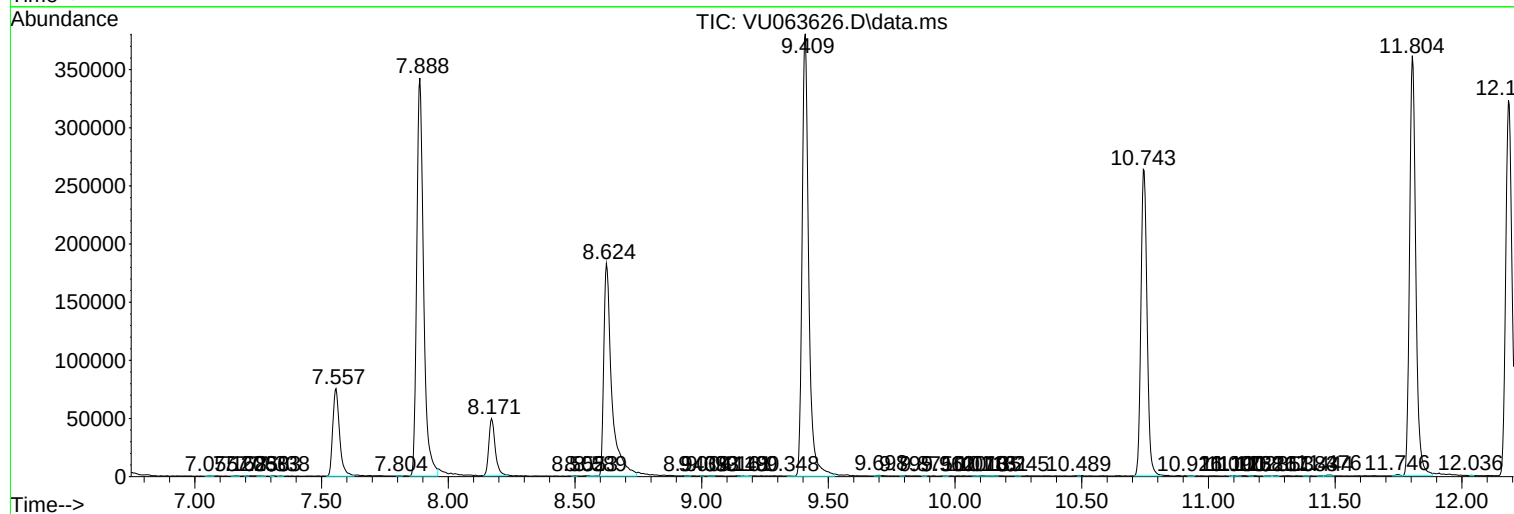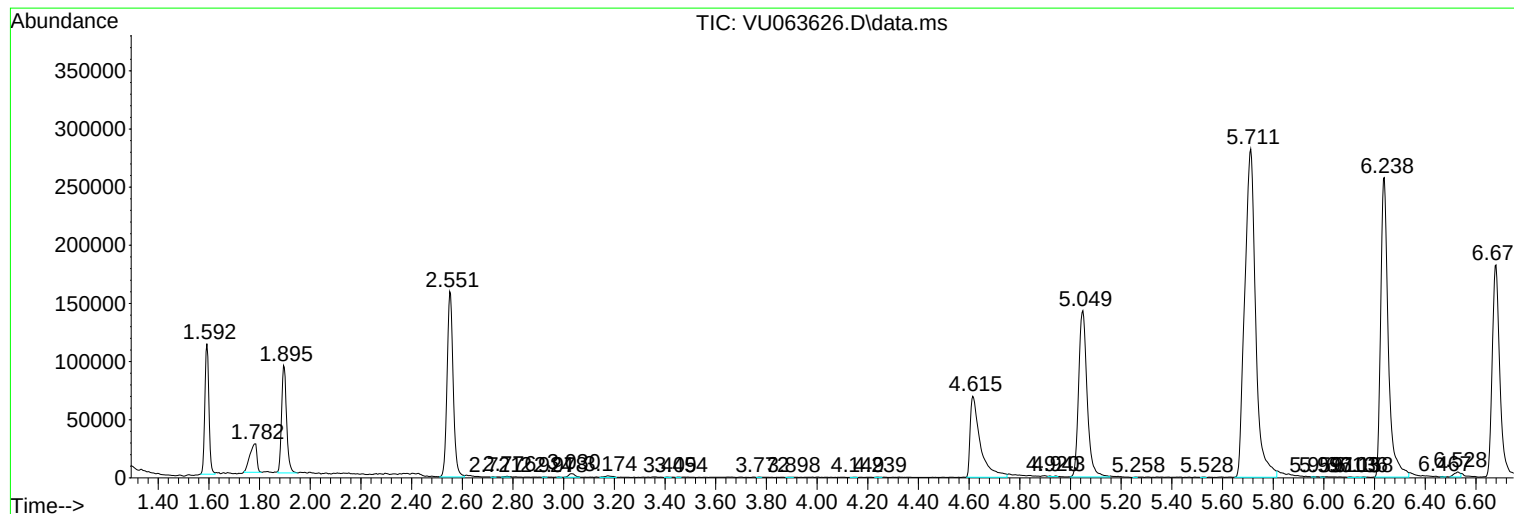

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063626.D
Acq On : 23 Sep 2025 10:56
Operator : MD/SY
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063626.D
Acq On : 23 Sep 2025 10:56
Operator : MD/SY
Sample : VU0923WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc