
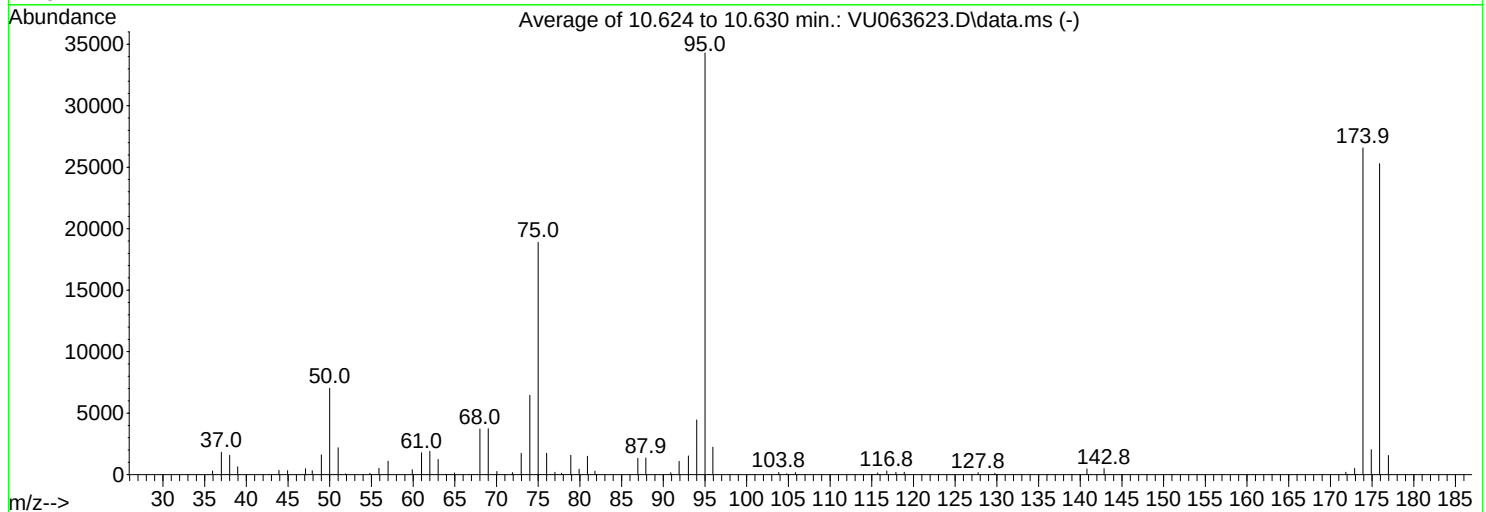


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092325\
Data File : VU063623.D
Acq On : 23 Sep 2025 08:27
Operator : MD/SY
Sample : BFB089
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB089

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092225WMA.M
Title : VOC Analysis
Last Update : Wed Sep 24 01:10:58 2025

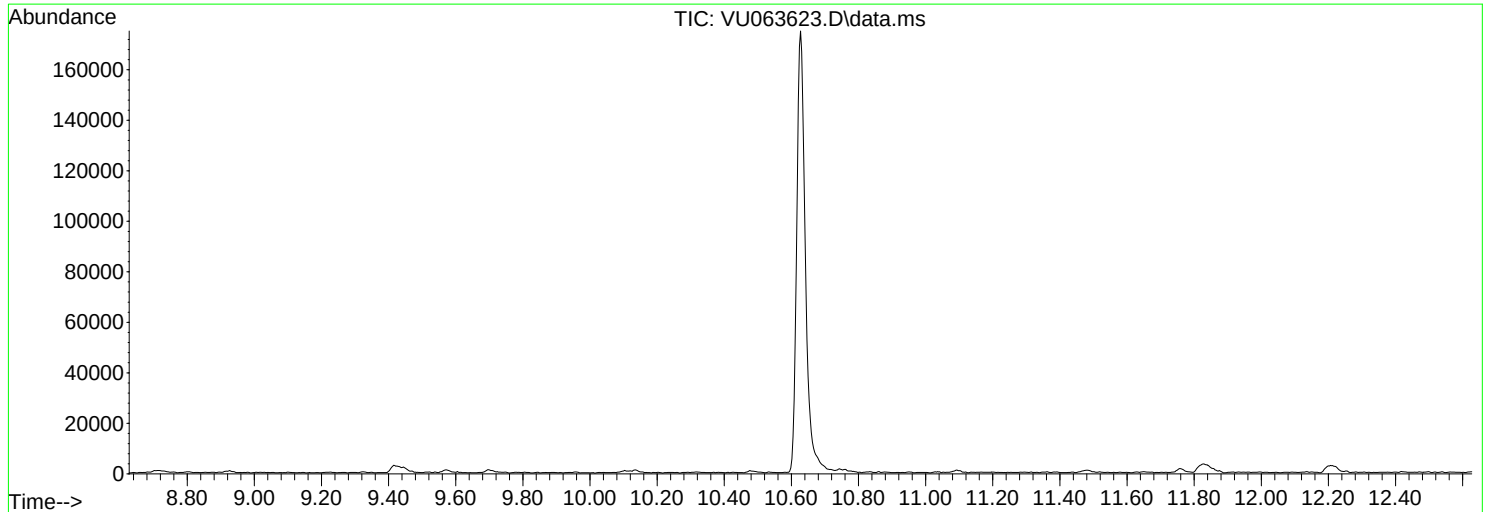

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	7028	PASS
75	95	30	80	55.1	18893	PASS
95	95	100	100	100.0	34299	PASS
96	95	5	9	6.5	2234	PASS
173	174	0.00	2	1.9	504	PASS
174	95	50	120	77.5	26571	PASS
175	174	5	9	7.6	2024	PASS
176	174	95	101	95.2	25291	PASS
177	176	5	9	6.2	1561	PASS

m/z	Abundance
38.80	106.0
39.80	212.0
44.00	330.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
35.90	285.0
37.00	1826.0
38.00	1534.0
39.00	749.0
39.90	162.0
43.90	621.0
45.00	367.0
47.10	466.0
47.90	381.0
49.00	1675.0
50.00	7118.0
51.00	2110.0
54.80	105.0
55.90	597.0
57.00	1075.0
59.90	392.0
61.00	1801.0
62.00	1995.0
63.00	1235.0
63.90	100.0
64.90	150.0
68.00	4048.0
69.00	3886.0
70.10	273.0
71.90	161.0
73.00	1742.0
74.00	6475.0
75.00	18768.0
76.00	1646.0
77.00	208.0
77.80	142.0
78.90	1557.0
79.90	427.0
80.90	1552.0
81.80	314.0
87.00	1287.0
87.90	1376.0
90.90	166.0
91.90	1101.0
93.00	1423.0
94.00	4269.0
95.00	34400.0
95.90	2152.0
103.90	227.0
104.80	121.0
105.90	188.0
115.70	157.0
116.80	294.0
117.90	182.0
118.90	211.0
127.70	192.0
129.80	134.0
140.80	439.0
142.80	426.0
171.90	211.0
172.90	496.0
173.90	25648.0
174.90	1993.0
175.90	24536.0
176.90	1531.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
35.90	302.0
37.00	1824.0
38.00	1646.0
39.00	749.0
39.80	163.0
43.90	695.0
45.00	353.0
47.10	519.0
47.90	349.0
49.00	1675.0
50.00	7225.0
51.00	2221.0
51.90	105.0
54.80	119.0
55.90	520.0
57.00	1095.0
59.90	436.0
61.00	1818.0
62.00	1972.0
63.00	1248.0
64.90	141.0
68.00	3796.0
69.00	3740.0
70.00	259.0
71.90	180.0
72.90	1815.0
74.00	6583.0
75.00	19584.0
76.00	1849.0
77.00	203.0
77.80	128.0
78.90	1635.0
79.90	476.0
80.90	1523.0
81.80	296.0
87.00	1338.0
87.90	1378.0
90.90	163.0
91.90	1098.0
93.00	1566.0
94.00	4546.0
95.00	35304.0
96.00	2295.0
103.90	184.0
104.80	131.0
105.80	181.0
115.70	146.0
116.80	308.0
117.90	217.0
118.90	200.0
127.70	184.0
129.80	100.0
140.80	513.0
142.90	532.0
171.80	208.0
172.90	533.0
173.90	27368.0
174.90	2104.0
175.90	25896.0
176.90	1579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
36.00	310.0
37.00	1800.0
38.00	1543.0
39.00	729.0
39.90	186.0
43.90	713.0
44.90	272.0
47.10	469.0
47.90	245.0
49.00	1494.0
50.00	6742.0
51.00	2229.0
51.90	109.0
54.80	114.0
55.90	433.0
57.00	1116.0
59.90	392.0
61.00	1733.0
62.00	1745.0
63.00	1232.0
65.00	126.0
68.00	3299.0
69.00	3568.0
70.00	240.0
71.90	181.0
72.90	1689.0
74.00	6309.0
75.00	18328.0
76.00	1727.0
77.00	186.0
77.80	102.0
78.90	1533.0
79.90	429.0
80.90	1403.0
81.80	269.0
86.90	1340.0
87.90	1297.0
90.90	143.0
91.90	1024.0
93.00	1589.0
94.00	4543.0
95.00	33192.0
96.00	2255.0
103.80	143.0
105.80	162.0
115.70	122.0
116.80	297.0
117.90	205.0
118.90	172.0
127.80	133.0
129.70	107.0
140.80	465.0
142.90	537.0
171.80	161.0
172.90	482.0
173.90	26696.0
174.90	1976.0
175.90	25440.0
177.00	1573.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089