

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092418\
 Data File : VU027115.D
 Acq On : 24 Sep 2018 17:41
 Operator : MD/SY
 Sample : J4973-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CB-0918-S-TCLP-GRID56-2

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.321	346	357	370	rVB	25047	39418	5.68%	0.869%
2	2.704	465	476	494	rVB	34857	62918	9.07%	1.388%
3	4.884	1138	1154	1171	rBV	99275	224471	32.35%	4.951%
4	4.984	1171	1185	1208	rVB	130114	286464	41.28%	6.318%
5	5.312	1272	1287	1305	rBV	128089	270516	38.98%	5.966%
6	5.550	1347	1361	1379	rBV	80245	168465	24.28%	3.715%
7	5.887	1452	1466	1484	rBV	210840	408991	58.93%	9.020%
8	6.582	1676	1682	1703	rVB2	3397	6971	1.00%	0.154%
9	6.707	1708	1721	1744	rBV	84395	159842	23.03%	3.525%
10	7.566	1975	1988	2003	rBV	397484	693981	100.00%	15.305%
11	8.183	2164	2180	2189	rBV2	19422	50092	7.22%	1.105%
12	8.418	2243	2253	2268	rBV	37491	61549	8.87%	1.357%
13	8.527	2279	2287	2306	rVB2	9071	16564	2.39%	0.365%
14	8.906	2394	2405	2423	rBV2	38836	65890	9.49%	1.453%
15	9.090	2446	2462	2485	rBV	303123	511545	73.71%	11.282%
16	10.308	2829	2841	2862	rBV	255880	412336	59.42%	9.094%
17	10.623	2925	2939	2954	rBV2	23950	47903	6.90%	1.056%
18	11.485	3195	3207	3228	rBV	308441	488267	70.36%	10.768%
19	11.768	3284	3295	3306	rBV4	6862	11447	1.65%	0.252%
20	12.482	3507	3517	3528	rVB	8136	13704	1.97%	0.302%
21	13.122	3707	3716	3728	rVB4	10374	15157	2.18%	0.334%
22	13.742	3895	3909	3934	rBV	287263	447606	64.50%	9.872%
23	14.276	4066	4075	4086	rBV2	4883	7989	1.15%	0.176%
24	14.350	4086	4098	4108	rVB6	3816	7628	1.10%	0.168%
25	14.877	4251	4262	4276	rBV	12486	22105	3.19%	0.488%
26	15.064	4310	4320	4333	rBV	15532	25194	3.63%	0.556%
27	16.742	4833	4842	4850	rBV4	4748	7217	1.04%	0.159%


Sum of corrected areas: 4534230

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092418\
Data File : VU027115.D
Acq On : 24 Sep 2018 17:41
Operator : MD/SY
Sample : J4973-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB-0918-S-TCLP-GRID56-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

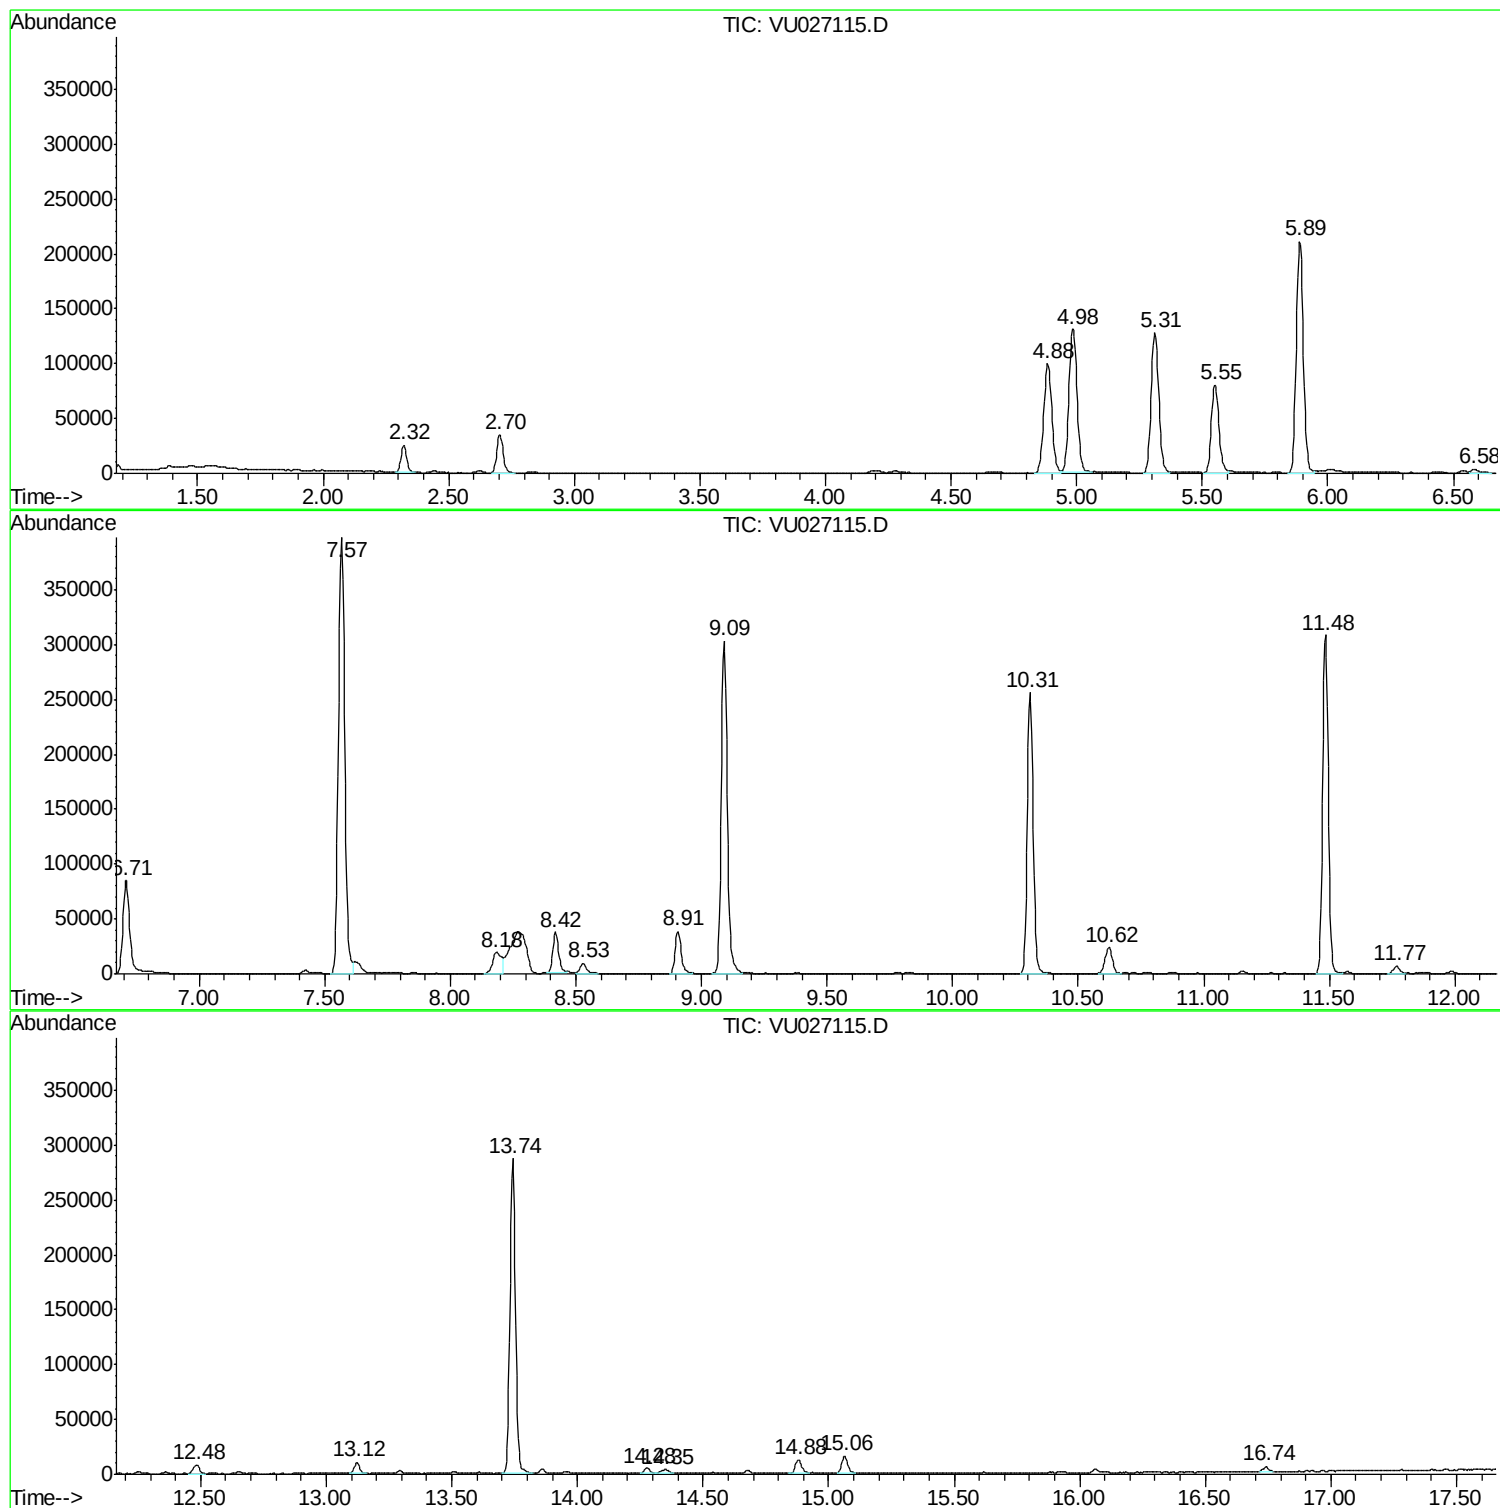

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092418\
Data File : VU027115.D
Acq On : 24 Sep 2018 17:41
Operator : MD/SY
Sample : J4973-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB-0918-S-TCLP-GRID56-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092418\
Data File : VU027115.D
Acq On : 24 Sep 2018 17:41
Operator : MD/SY
Sample : J4973-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CB-0918-S-TCLP-GRID56-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc