


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092418\
Data File : VU027092.D
Acq On : 24 Sep 2018 08:21
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U092218W.M
Title : SW846 8260
Last Update : Sat Sep 22 01:31:57 2018

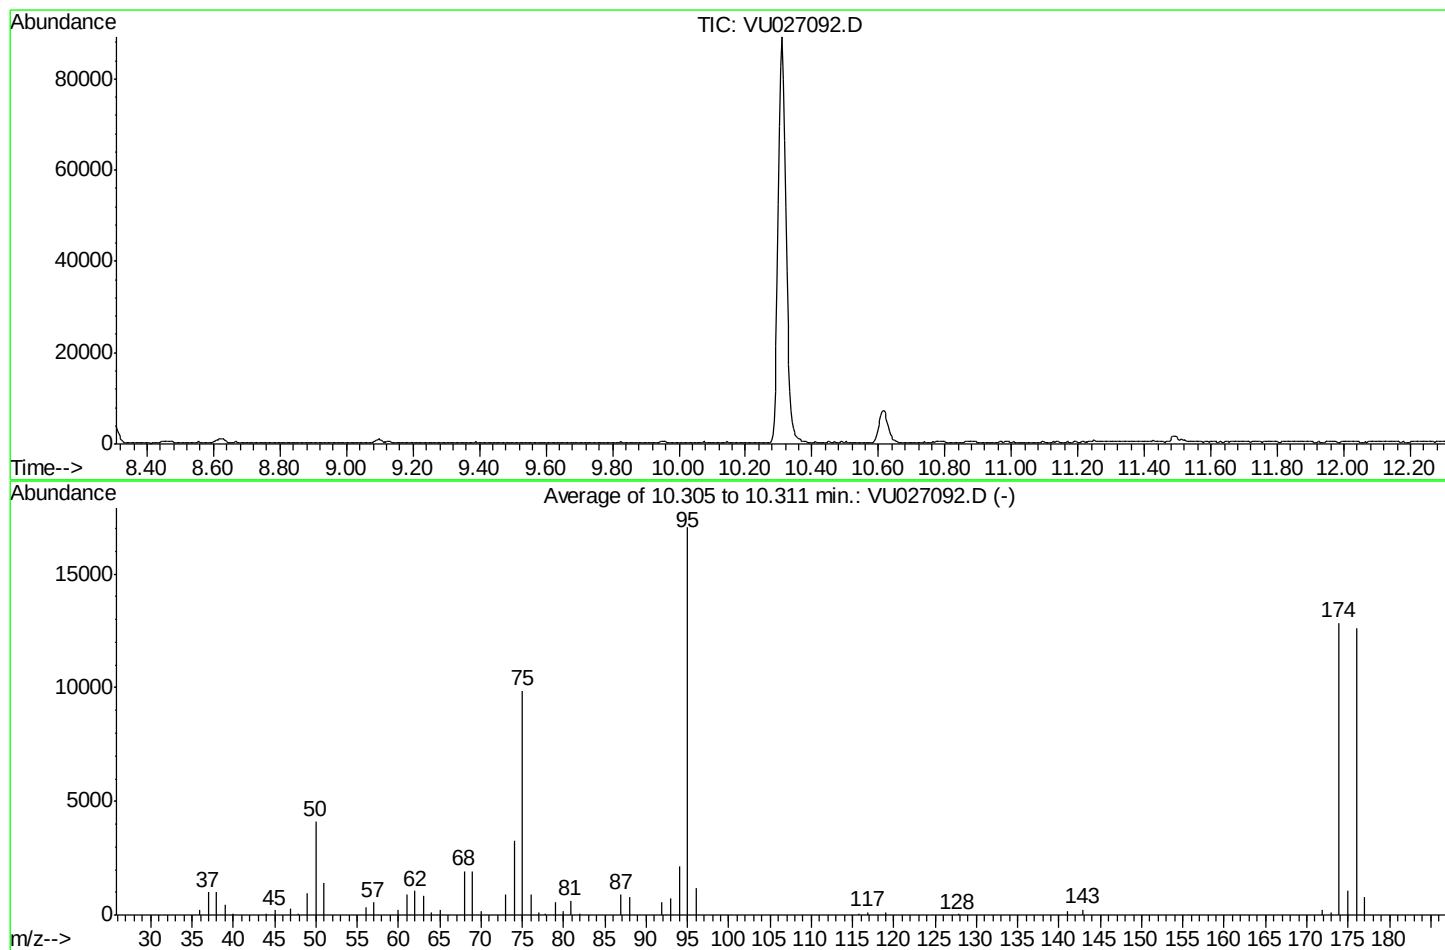

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	4103	PASS
75	95	30	60	57.9	9871	PASS
95	95	100	100	100.0	17058	PASS
96	95	5	9	6.9	1169	PASS
173	174	0.00	2	0.7	95	PASS
174	95	50	100	75.3	12843	PASS
175	174	5	9	8.4	1082	PASS
176	174	95	101	98.3	12629	PASS
177	176	5	9	6.2	781	PASS