
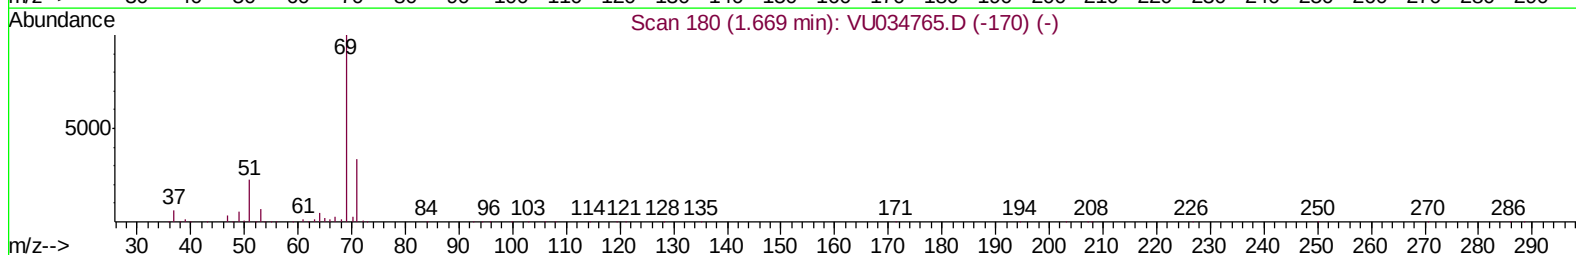
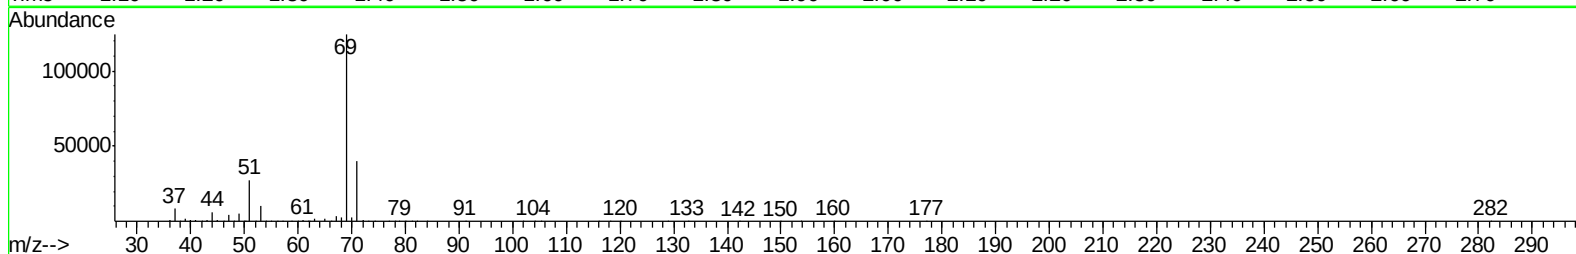


Data File : VU034769.D
Acq On : 24 Sep 2019 14:27
Operator : JC/SP
Sample : K4984-08 10X
Misc : 6.22g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Sep 25 03:02:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 25 02:59:31 2019
Response via : Initial Calibration

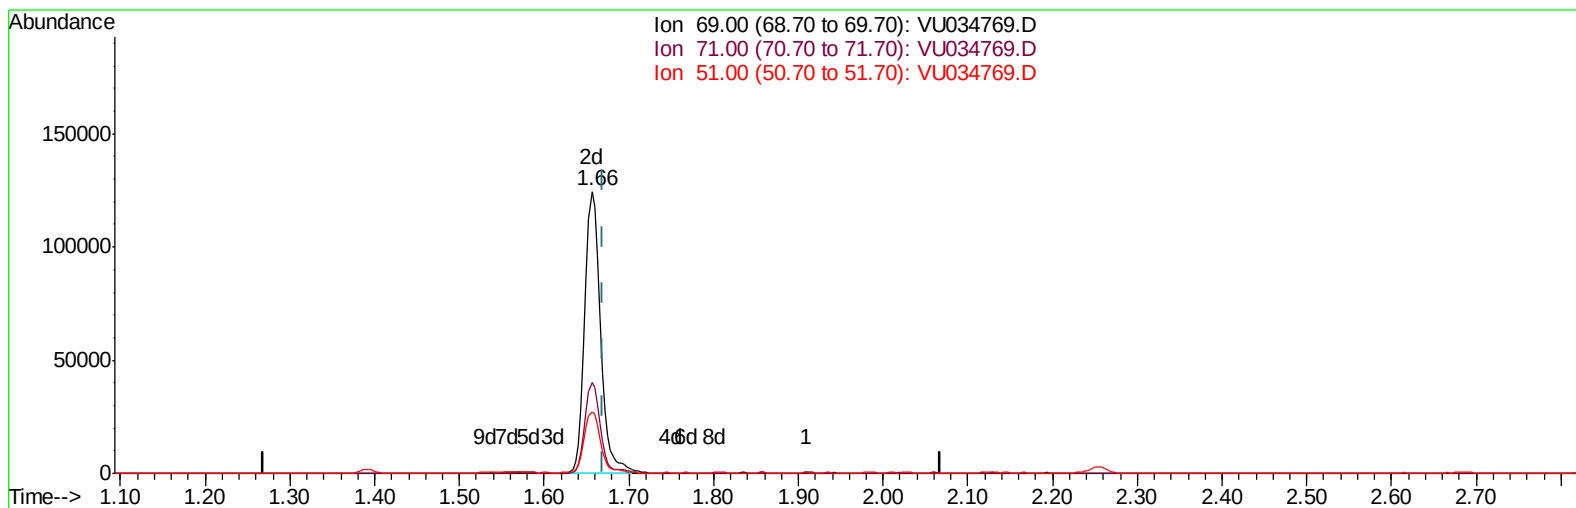

TIC: VU034769.D

(7) Chloroethane-d5 (S)

1.656min (-0.013) 45.61ug/L m

response 161828

Ion	Exp%	Act%
69.00	100	100
71.00	31.80	0.06#
51.00	32.70	0.07#
0.00	0.00	0.00