
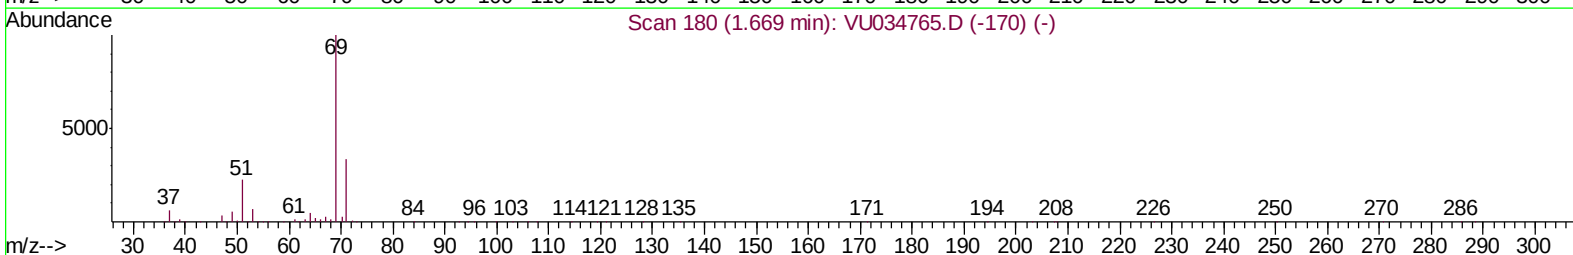
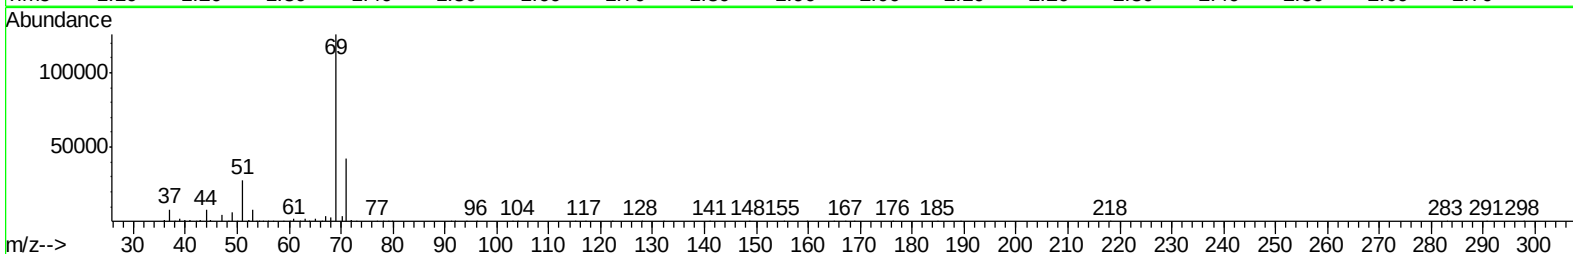


Data File : VU034771.D
Acq On : 24 Sep 2019 15:15
Operator : JC/SP
Sample : K4984-09 10X
Misc : 4.59g/5.0ml/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Sep 25 03:02:59 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 25 02:59:31 2019
Response via : Initial Calibration

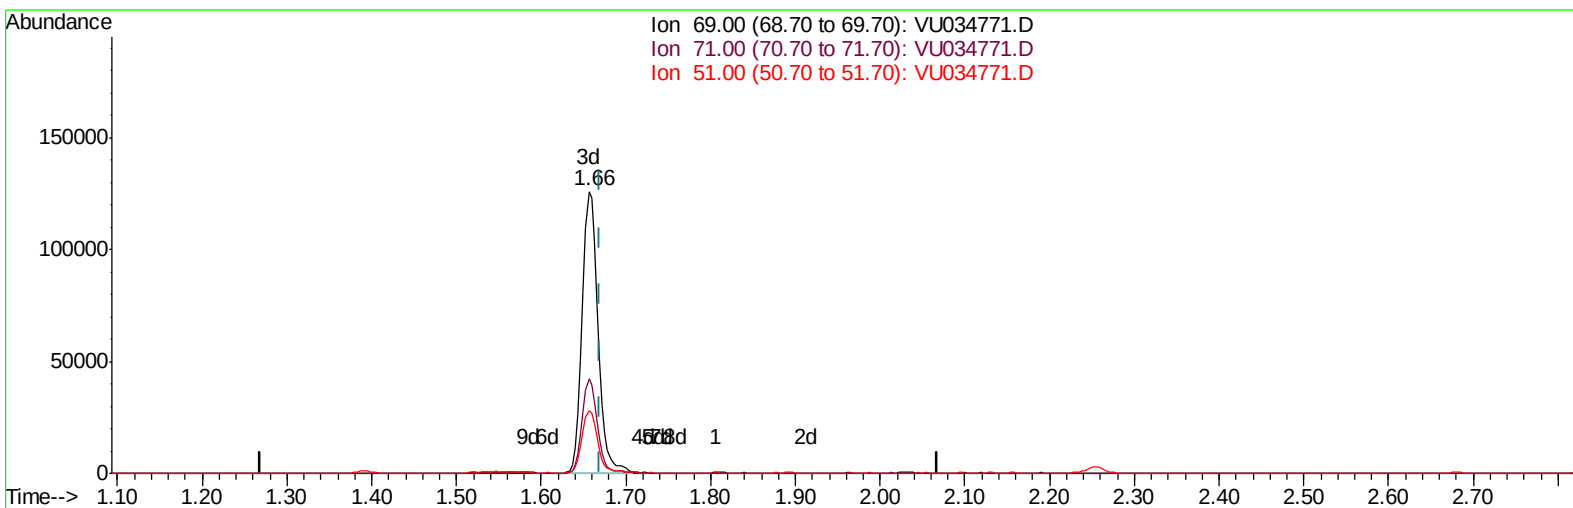

TIC: VU034771.D

(7) Chloroethane-d5 (S)

1.656min (-0.013) 41.89ug/L m

response 163956

Ion	Exp%	Act%
69.00	100	100
71.00	31.80	0.08#
51.00	32.70	0.05#
0.00	0.00	0.00