
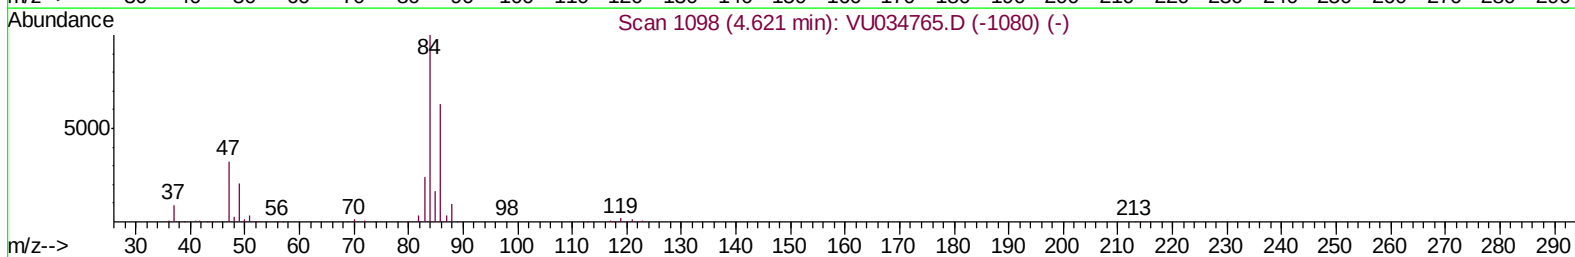
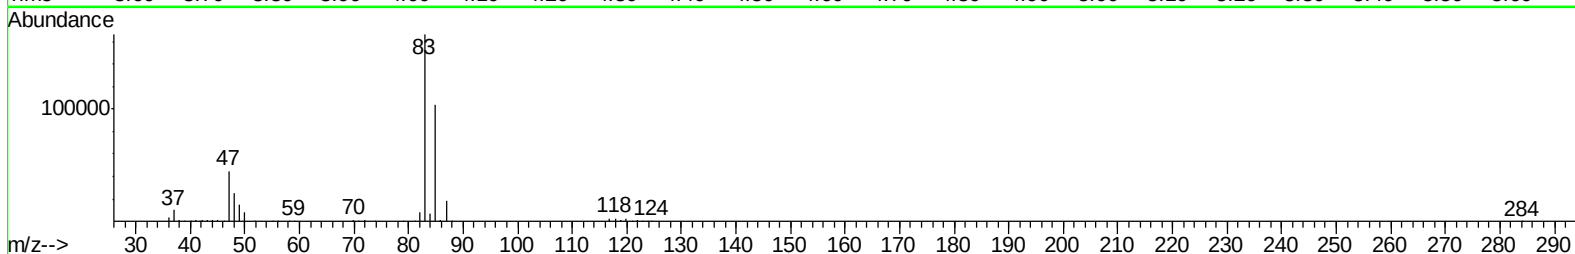


Data File : VU034778.D
Acq On : 24 Sep 2019 17:59
Operator : JC/SP
Sample : K4932-04RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Sep 25 05:27:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 25 02:59:31 2019
Response via : Initial Calibration

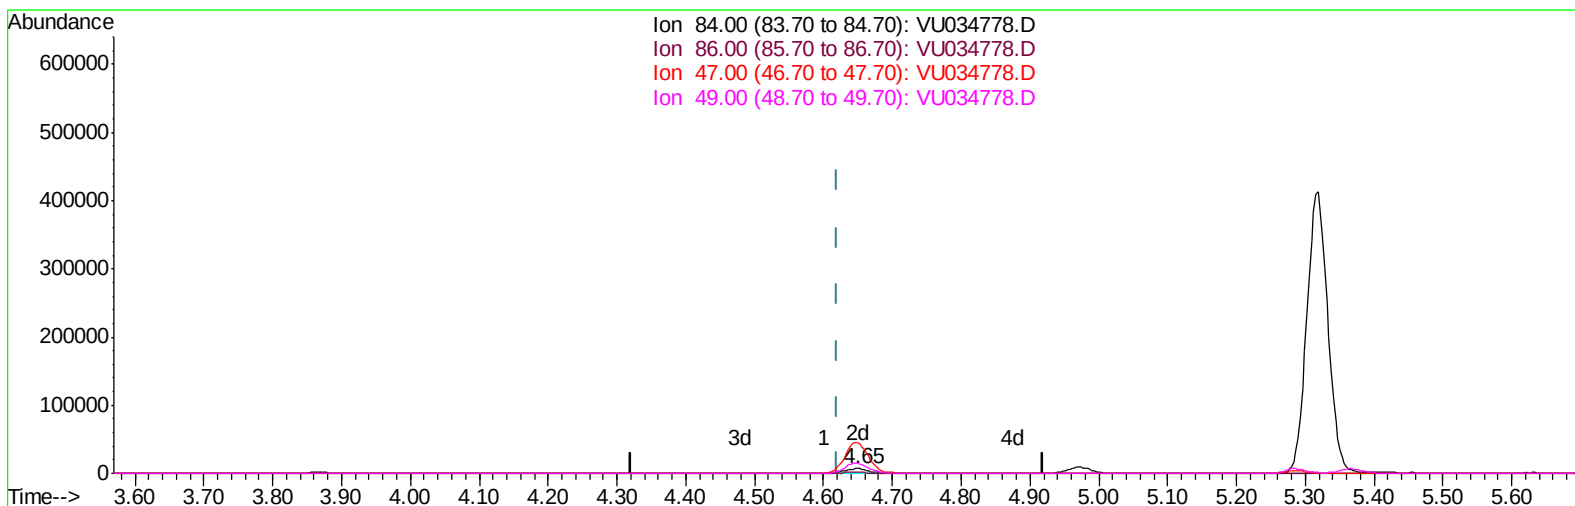

TIC: VU034778.D

(24) Chloroform-d (S)

4.650min (+0.029) 1.82ug/L m

response 16712

Ion	Exp%	Act%
84.00	100	100
86.00	61.70	3.78#
47.00	58.40	0.33#
49.00	34.10	0.00#