
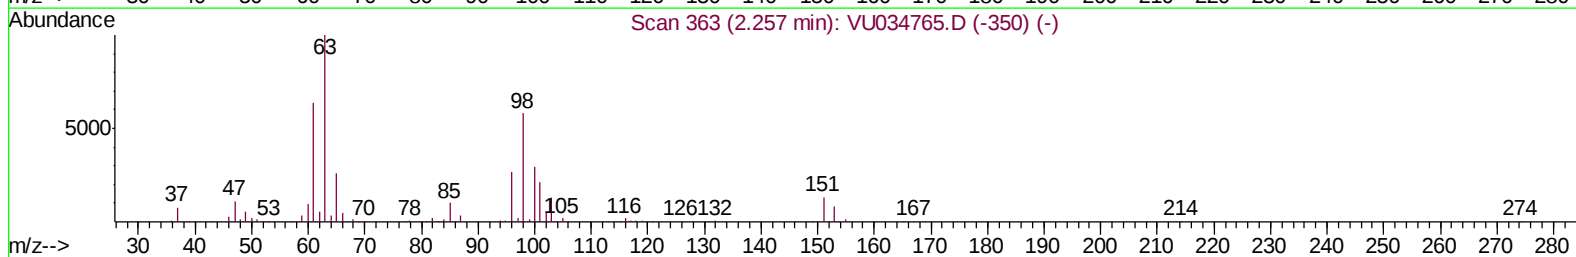
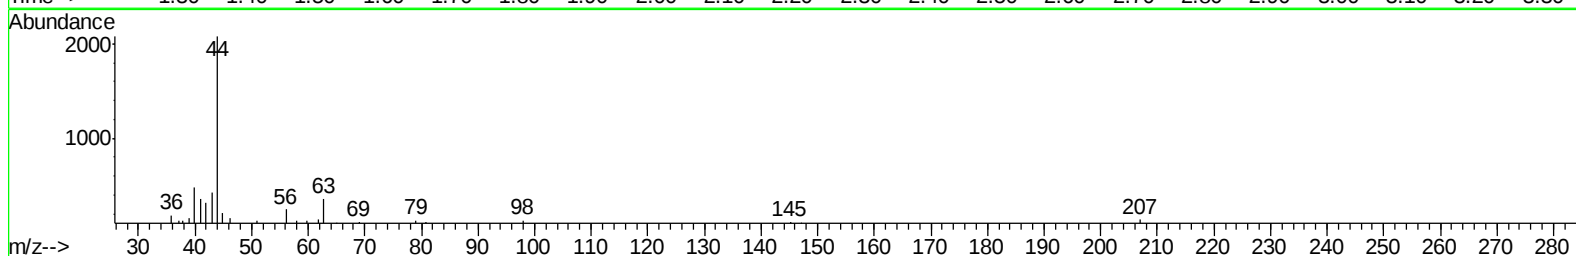


Data File : VU034785.D
Acq On : 24 Sep 2019 20:43
Operator : JC/SP
Sample : K4948-02DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Sep 25 03:05:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 25 02:59:31 2019
Response via : Initial Calibration

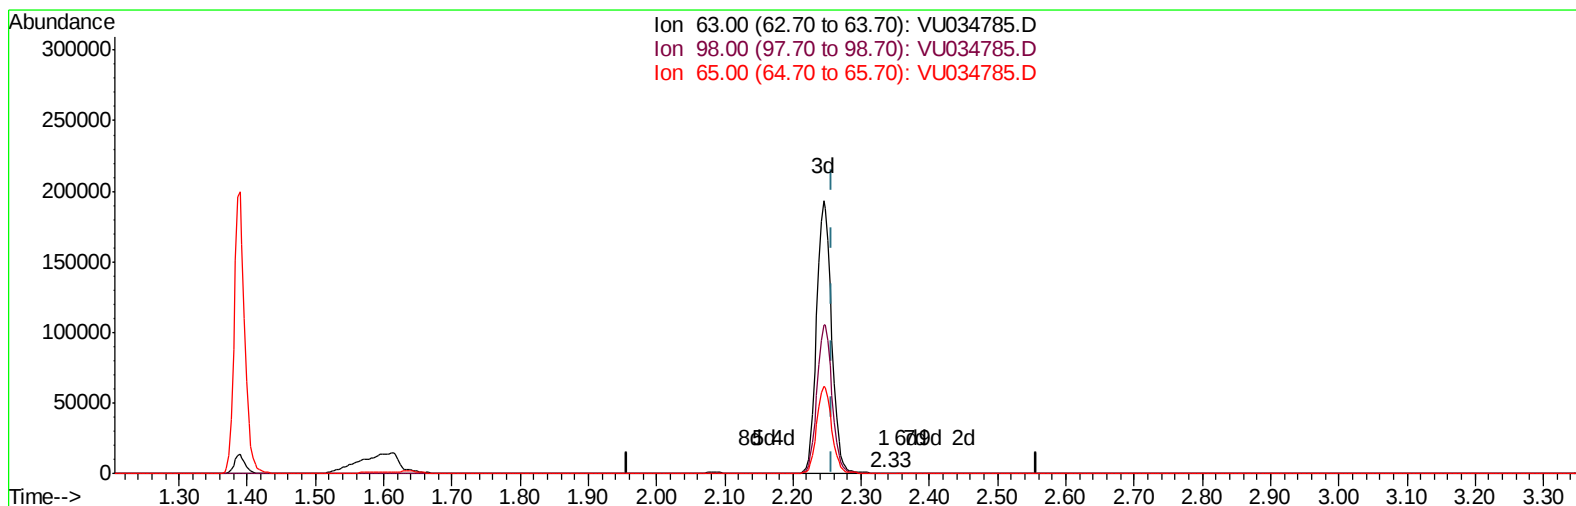

TIC: VU034785.D

(11) 1,1-Dichloroethene-d2 (S)

2.334min (+0.077) 0.02ug/L

response 168

Ion	Exp%	Act%
63.00	100	100
98.00	57.60	48.81
65.00	24.00	24.40
0.00	0.00	0.00