
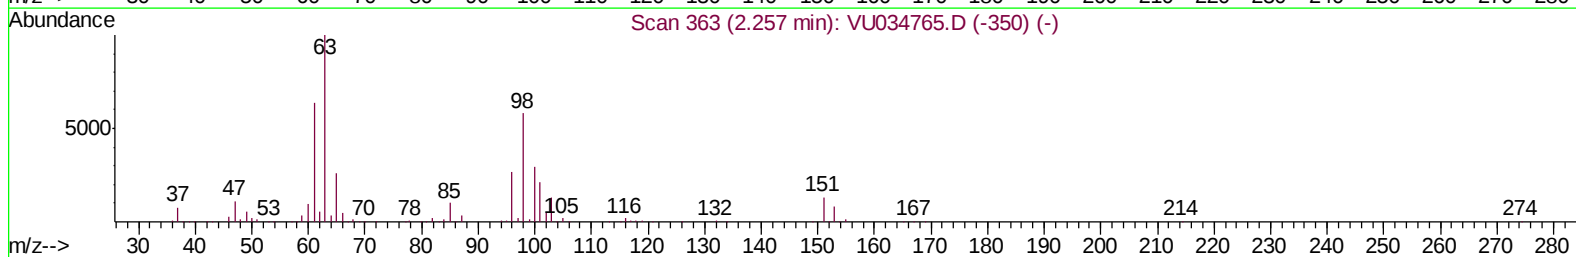
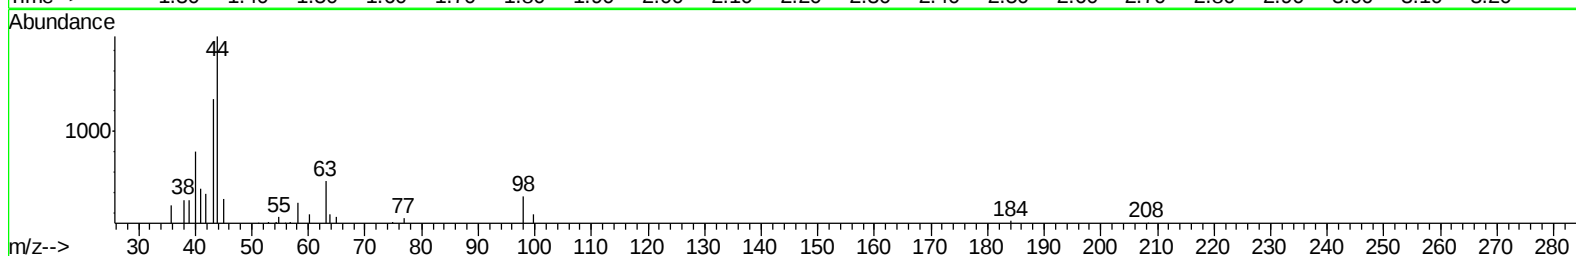


Data File : VU034790.D  
Acq On : 24 Sep 2019 22:41  
Operator : JC/SP  
Sample : K4984-06ME 10X  
Misc : 4.99g/5.0ml/100uL/5.0mL/MSVOA\_U/MEOH  
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Sep 25 03:06:32 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM091919WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Sep 25 02:59:31 2019  
Response via : Initial Calibration

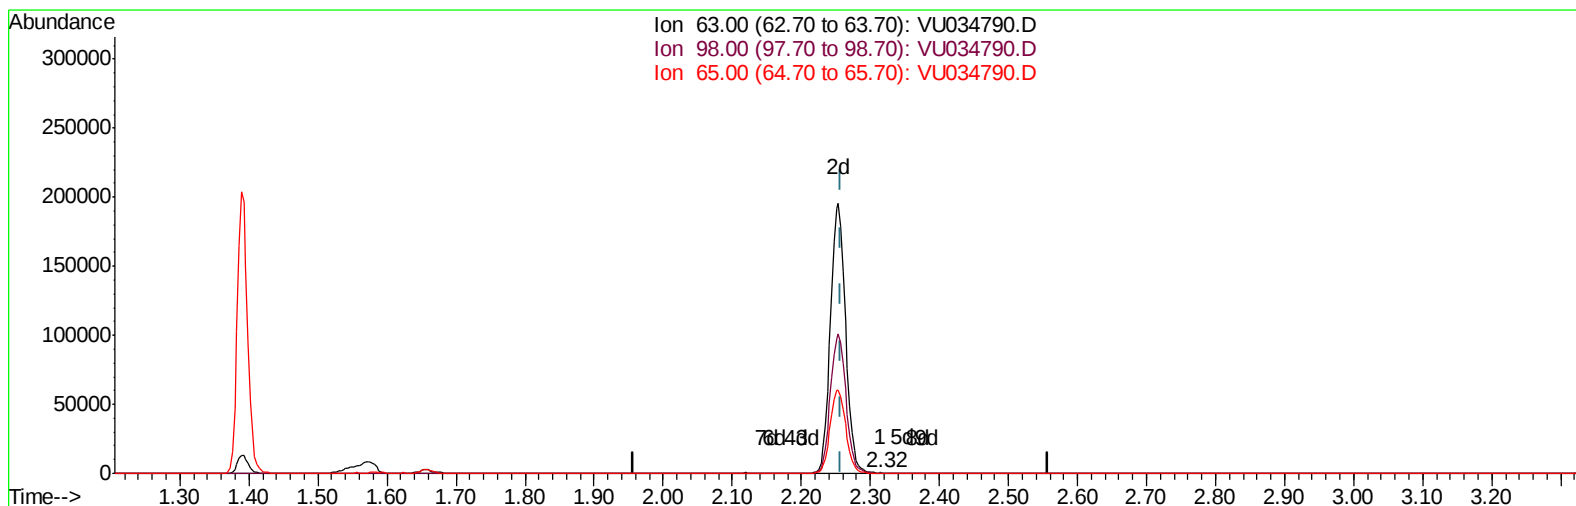

TIC: VU034790.D

(11) 1,1-Dichloroethene-d2 (S)

2.315min (+0.058) 0.04ug/L

response 397

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 63.00 | 100   | 100   |
| 98.00 | 57.60 | 65.74 |
| 65.00 | 24.00 | 28.72 |
| 0.00  | 0.00  | 0.00  |