


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092419\
Data File : VU034764.D
Acq On : 24 Sep 2019 11:41
Operator : JC/SP
Sample : BFB37
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB37

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Title : VOC Analysis
Last Update : Thu Sep 26 06:56:48 2019

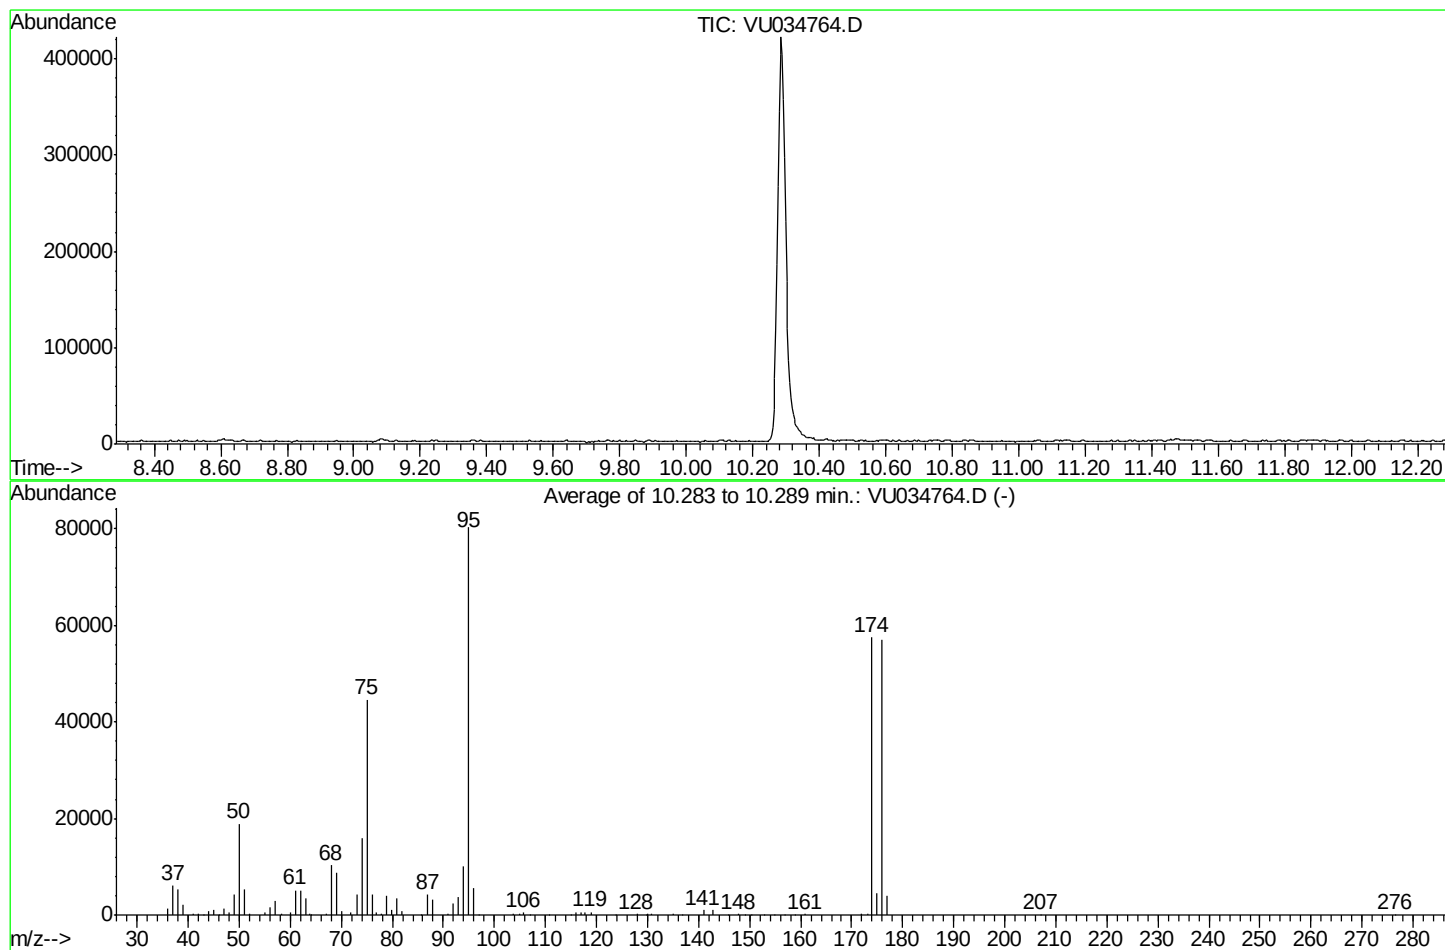

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.5	18866	PASS
75	95	30	80	55.6	44682	PASS
95	95	100	100	100.0	80325	PASS
96	95	5	9	6.9	5530	PASS
173	174	0.00	2	0.4	257	PASS
174	95	50	120	71.6	57490	PASS
175	174	5	9	8.1	4631	PASS
176	174	95	101	99.1	56992	PASS
177	176	5	9	7.0	4014	PASS

m/z	Abundance
36.00	1243.0
37.00	6490.0
38.00	5431.0
39.00	2296.0
39.90	464.0
41.00	208.0
42.00	133.0
42.90	190.0
44.00	1997.0
44.90	1049.0
45.80	122.0
46.90	1528.0
48.10	580.0
49.00	4139.0
50.00	18352.0
51.00	5522.0
52.00	166.0
55.00	395.0
56.10	1358.0
57.00	2902.0
58.30	197.0
60.00	925.0
61.00	5243.0
62.00	5178.0
63.00	3792.0
63.90	292.0
67.10	355.0
68.00	10051.0
69.00	8879.0
70.00	706.0
72.00	540.0
73.00	4148.0
74.00	15822.0
75.00	43632.0
76.00	4037.0
77.00	461.0
77.80	138.0
78.90	3685.0
79.90	999.0
80.90	3644.0
81.90	899.0
85.70	114.0
87.00	4107.0
88.00	3049.0
90.80	382.0
92.00	2342.0
93.00	3751.0
94.00	10089.0
95.00	79728.0
96.00	5633.0
103.80	315.0
104.90	150.0
105.80	376.0
110.80	210.0
114.90	120.0
115.90	383.0
116.90	394.0
117.80	458.0
118.90	541.0
123.80	125.0
127.90	253.0
129.80	396.0
130.90	215.0
134.90	178.0
136.80	128.0
141.00	860.0
142.90	905.0
145.80	119.0
147.90	127.0
150.20	124.0
152.90	143.0
156.70	113.0
158.80	127.0
160.90	223.0
172.00	206.0
173.20	771.0
174.00	55016.0
175.00	4420.0
176.00	54824.0
177.00	3927.0
276.50	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.00	1344.0
37.00	6195.0
38.00	5654.0
39.00	2224.0
39.90	470.0
41.00	235.0
42.00	159.0
43.00	252.0
44.00	2055.0
44.90	1172.0
45.90	135.0
46.90	1528.0
48.10	524.0
49.00	4279.0
50.00	19520.0
51.00	5483.0
51.90	215.0
55.10	453.0
56.00	1600.0
57.00	3065.0
58.30	191.0
60.00	857.0
61.00	5293.0
62.00	5073.0
63.00	3455.0
63.90	271.0
67.10	399.0
68.00	10727.0
69.00	9095.0
70.00	944.0
71.90	514.0
73.00	4191.0
74.00	16640.0
75.00	46304.0
76.00	4227.0
76.90	476.0
77.80	288.0
78.90	3992.0
79.90	964.0
80.90	3542.0
82.00	853.0
87.00	4326.0
88.00	3091.0
90.80	392.0
92.00	2502.0
93.00	3869.0
94.00	10197.0
95.00	82856.0
96.00	5718.0
97.00	125.0
103.70	345.0
104.90	157.0
105.80	489.0
106.90	138.0
110.80	204.0
115.00	136.0
115.90	446.0
116.90	462.0
117.70	555.0
118.90	637.0
127.90	251.0
130.00	322.0
130.90	234.0
134.90	157.0
141.00	1014.0
142.90	991.0
145.90	117.0
147.90	222.0
155.00	111.0
156.70	152.0
158.80	115.0
160.90	175.0
171.90	191.0
174.00	59304.0
175.00	4774.0
176.00	58720.0
177.00	4241.0
207.10	107.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.00	1374.0
37.00	5358.0
38.00	5235.0
39.00	2054.0
39.90	557.0
41.00	243.0
42.00	147.0
43.10	400.0
43.90	1898.0
45.00	1135.0
46.00	173.0
46.90	1170.0
47.90	445.0
48.90	3960.0
50.00	18728.0
51.00	5048.0
51.90	280.0
55.10	458.0
56.00	1680.0
57.00	2870.0
58.30	125.0
60.00	732.0
61.00	4847.0
62.00	4742.0
63.00	2882.0
64.10	289.0
67.10	394.0
68.00	10156.0
69.00	8537.0
70.00	1006.0
71.90	510.0
73.00	4078.0
74.00	15509.0
75.00	44112.0
76.10	4108.0
76.90	443.0
77.80	440.0
78.90	3951.0
79.90	1012.0
80.90	3386.0
82.00	828.0
86.90	3928.0
87.90	3293.0
90.80	374.0
92.00	2390.0
93.00	3561.0
94.00	9797.0
95.00	78392.0
96.00	5239.0
96.90	243.0
103.80	354.0
104.70	163.0
105.80	497.0
106.90	151.0
110.80	168.0
115.10	143.0
115.90	475.0
116.90	424.0
117.70	457.0
118.90	628.0
127.90	257.0
130.00	295.0
130.80	219.0
135.00	141.0
140.90	1075.0
142.90	948.0
145.90	103.0
147.90	262.0
149.00	114.0
154.90	169.0
156.80	134.0
161.00	136.0
171.90	167.0
174.00	58152.0
175.00	4700.0
176.00	57432.0
177.00	3874.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

Scan 2847 (10.244 min): VU034764.D
BFB37

m/z	Abundance
35.90	116.0
39.10	100.0
40.00	517.0
42.40	132.0
42.90	217.0
44.00	1209.0
44.90	157.0
59.80	102.0
60.20	103.0
85.00	112.0
110.90	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37