

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040266.D
 Acq On : 24 Sep 2020 12:20
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	92	rBV	238500	262865	14.56%	1.862%
2	1.919	171	180	195	rVB	182149	238429	13.21%	1.689%
3	2.578	371	385	400	rBV	403906	672496	37.26%	4.764%
4	2.806	448	456	466	rVB2	3997	7341	0.41%	0.052%
5	2.851	466	470	474	rBV2	268	288	0.02%	0.002%
6	3.063	526	536	544	rVB5	2772	4836	0.27%	0.034%
7	3.147	559	562	564	rBV	546	336	0.02%	0.002%
8	3.160	564	566	569	rVV3	476	377	0.02%	0.003%
9	3.202	569	579	593	rVV3	4135	9405	0.52%	0.067%
10	3.372	623	632	636	rBV5	1660	2531	0.14%	0.018%
11	3.642	713	716	719	rVV3	417	298	0.02%	0.002%
12	3.825	771	773	779	rVB2	437	301	0.02%	0.002%
13	3.899	791	796	800	rVB2	450	324	0.02%	0.002%
14	3.989	818	824	828	rBV2	318	405	0.02%	0.003%
15	4.186	882	885	892	rVB2	406	285	0.02%	0.002%
16	4.362	933	940	942	rVB2	282	295	0.02%	0.002%
17	4.642	1009	1027	1050	rBV	198276	488650	27.07%	3.462%
18	4.912	1107	1111	1113	rBV2	408	320	0.02%	0.002%
19	5.083	1146	1164	1185	rBV	322401	717850	39.77%	5.086%
20	5.269	1220	1222	1225	rVB2	771	392	0.02%	0.003%
21	5.292	1225	1229	1231	rBV3	1019	919	0.05%	0.007%
22	5.388	1255	1259	1262	rBV5	1448	1352	0.07%	0.010%
23	5.481	1285	1288	1293	rBV3	364	287	0.02%	0.002%
24	5.539	1299	1306	1314	rVB5	883	1190	0.07%	0.008%
25	5.742	1345	1369	1393	rBV2	669930	1804999	100.00%	12.788%
26	5.909	1419	1421	1425	rBV3	401	323	0.02%	0.002%
27	5.967	1435	1439	1442	rBV3	667	421	0.02%	0.003%
28	6.050	1461	1465	1467	rBV2	823	674	0.04%	0.005%
29	6.099	1477	1480	1482	rBV	393	275	0.02%	0.002%
30	6.189	1505	1508	1510	rVB2	461	296	0.02%	0.002%
31	6.263	1514	1531	1550	rBV	581591	1088450	60.30%	7.711%
32	6.423	1577	1581	1586	rVB5	997	1020	0.06%	0.007%
33	6.462	1588	1593	1595	rBV	373	377	0.02%	0.003%
34	6.542	1609	1618	1629	rVB7	7096	13860	0.77%	0.098%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040266.D
 Acq On : 24 Sep 2020 12:20
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

35	6.703	1649	1668	1686	rBV	432124	835144	46.27%	5.917%
36	6.848	1710	1713	1716	rVB3	1015	606	0.03%	0.004%
37	6.899	1726	1729	1731	rBV3	518	280	0.02%	0.002%
38	6.935	1738	1740	1745	rBV3	585	412	0.02%	0.003%
39	7.076	1777	1784	1787	rBV2	479	467	0.03%	0.003%
40	7.185	1812	1818	1822	rBV4	581	671	0.04%	0.005%
41	7.382	1876	1879	1883	rVB	412	294	0.02%	0.002%
42	7.574	1919	1939	1960	rBV	242850	429506	23.80%	3.043%
43	7.800	1999	2009	2020	rBV5	4191	7859	0.44%	0.056%
44	7.906	2028	2042	2060	rBV	804001	1378968	76.40%	9.769%
45	8.021	2076	2078	2083	rVB3	623	401	0.02%	0.003%
46	8.137	2109	2114	2117	rBV3	398	380	0.02%	0.003%
47	8.185	2117	2129	2148	rBV2	178950	302436	16.76%	2.143%
48	8.369	2183	2186	2192	rVB2	392	375	0.02%	0.003%
49	8.404	2193	2197	2202	rVB5	925	1027	0.06%	0.007%
50	8.555	2239	2244	2249	rVB5	1400	1534	0.08%	0.011%
51	8.639	2256	2270	2307	rBV	541326	946125	52.42%	6.703%
52	8.925	2351	2359	2368	rVB4	1919	3276	0.18%	0.023%
53	8.999	2380	2382	2385	rVV	504	289	0.02%	0.002%
54	9.160	2426	2432	2436	rBV2	429	377	0.02%	0.003%
55	9.214	2447	2449	2454	rVB	344	293	0.02%	0.002%
56	9.253	2458	2461	2467	rVB2	722	591	0.03%	0.004%
57	9.327	2481	2484	2487	rBV	599	388	0.02%	0.003%
58	9.420	2499	2513	2531	rBV	831859	1367442	75.76%	9.688%
59	9.568	2554	2559	2560	rBV	2154	1508	0.08%	0.011%
60	9.700	2591	2600	2606	rVB5	1965	2747	0.15%	0.019%
61	9.825	2634	2639	2643	rBV3	464	369	0.02%	0.003%
62	10.015	2694	2698	2702	rBV3	435	397	0.02%	0.003%
63	10.105	2712	2726	2729	rBV5	3097	4321	0.24%	0.031%
64	10.182	2746	2750	2754	rBV2	298	282	0.02%	0.002%
65	10.298	2780	2786	2793	rVV4	615	932	0.05%	0.007%
66	10.484	2835	2844	2853	rBV4	1975	2813	0.16%	0.020%
67	10.590	2873	2877	2879	rBV2	359	283	0.02%	0.002%
68	10.632	2887	2890	2893	rBV2	406	312	0.02%	0.002%
69	10.754	2915	2928	2945	rBV	529872	862470	47.78%	6.110%
70	10.819	2945	2948	2951	rVB2	1021	607	0.03%	0.004%
71	10.906	2971	2975	2977	rBV3	346	294	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040266.D
 Acq On : 24 Sep 2020 12:20
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK201

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

72	11.089	3023	3032	3038	rBV3	1891	2507	0.14%	0.018%
73	11.253	3076	3083	3084	rBV	557	529	0.03%	0.004%
74	11.468	3147	3150	3158	rVB3	2413	2436	0.13%	0.017%
75	11.549	3170	3175	3176	rBV	458	367	0.02%	0.003%
76	11.606	3190	3193	3196	rBV	395	281	0.02%	0.002%
77	11.632	3199	3201	3205	rVB2	500	349	0.02%	0.002%
78	11.745	3227	3236	3243	rVB6	4533	6442	0.36%	0.046%
79	11.806	3243	3255	3275	rBV	778198	1267811	70.24%	8.982%
80	11.902	3280	3285	3287	rBV3	580	467	0.03%	0.003%
81	12.188	3360	3374	3390	rBV	772035	1261763	69.90%	8.939%
82	12.269	3395	3399	3404	rBV5	652	501	0.03%	0.004%
83	12.404	3438	3441	3447	rVB3	479	470	0.03%	0.003%
84	12.433	3447	3450	3454	rBV2	554	473	0.03%	0.003%
85	12.507	3470	3473	3478	rBV	562	515	0.03%	0.004%
86	12.658	3518	3520	3525	rVB2	639	407	0.02%	0.003%
87	12.796	3561	3563	3567	rBV2	485	324	0.02%	0.002%
88	12.989	3618	3623	3629	rVB2	1890	1987	0.11%	0.014%
89	13.086	3648	3653	3655	rBV3	634	665	0.04%	0.005%
90	13.211	3684	3692	3703	rVB4	7370	10746	0.60%	0.076%
91	13.500	3778	3782	3785	rBV2	617	517	0.03%	0.004%
92	13.594	3806	3811	3816	rBV3	1096	1226	0.07%	0.009%
93	13.831	3877	3885	3894	rVB5	11675	17691	0.98%	0.125%
94	13.893	3900	3904	3906	rBV2	623	564	0.03%	0.004%
95	13.999	3932	3937	3941	rBV3	955	842	0.05%	0.006%
96	14.076	3950	3961	3971	rBV	19861	33692	1.87%	0.239%
97	14.317	4028	4036	4047	rVB4	13374	20933	1.16%	0.148%
98	14.523	4097	4100	4102	rBV	644	432	0.02%	0.003%
99	15.712	4467	4470	4473	rBV3	1111	653	0.04%	0.005%
100	16.175	4612	4614	4616	rBV2	1281	650	0.04%	0.005%


Sum of corrected areas: 14115183

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092420\
Data File : VU040266.D
Acq On : 24 Sep 2020 12:20
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

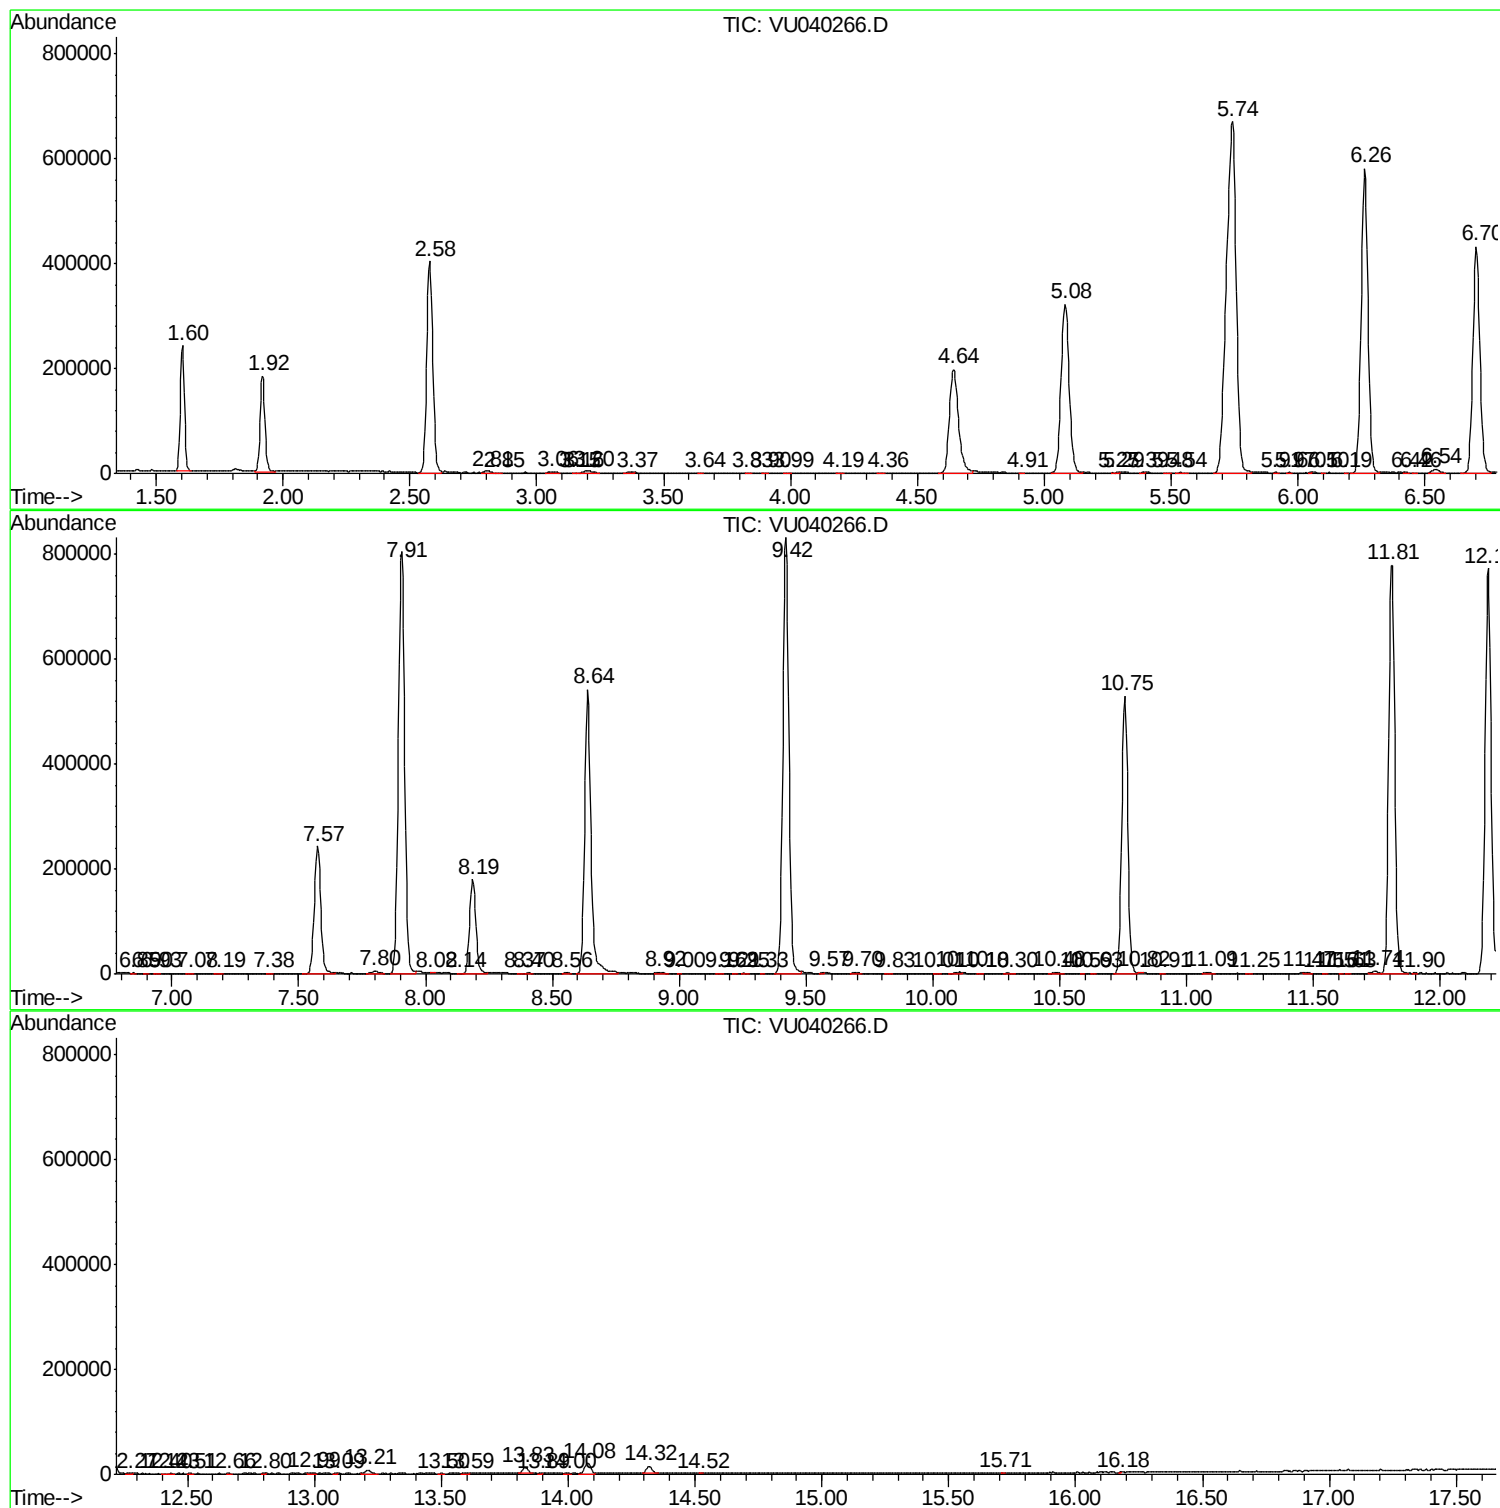

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092420\
Data File : VU040266.D
Acq On : 24 Sep 2020 12:20
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092420\
Data File : VU040266.D
Acq On : 24 Sep 2020 12:20
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK201

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc