

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040267.D
 Acq On : 24 Sep 2020 12:42
 Operator : SY/MD
 Sample : VU0924WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	97	rVB	229835	250756	14.53%	1.854%
2	1.919	172	180	193	rVB	170916	221122	12.81%	1.635%
3	2.578	373	385	403	rBV	381291	638848	37.01%	4.723%
4	2.806	447	456	464	rVV	3108	4500	0.26%	0.033%
5	2.864	470	474	479	rVB2	527	459	0.03%	0.003%
6	2.890	479	482	485	rBV3	572	300	0.02%	0.002%
7	2.928	490	494	498	rBV3	891	995	0.06%	0.007%
8	3.060	527	535	536	rBV3	2191	2495	0.14%	0.018%
9	3.205	568	580	592	rVV2	5095	10993	0.64%	0.081%
10	3.372	627	632	642	rVB5	1155	1612	0.09%	0.012%
11	3.430	645	650	656	rBV2	446	510	0.03%	0.004%
12	3.475	659	664	668	rBV	311	293	0.02%	0.002%
13	3.571	692	694	701	rVB2	369	290	0.02%	0.002%
14	4.031	830	837	840	rBV3	413	416	0.02%	0.003%
15	4.096	855	857	863	rVB2	409	374	0.02%	0.003%
16	4.330	923	930	933	rBV2	591	603	0.03%	0.004%
17	4.369	938	942	949	rVV2	345	449	0.03%	0.003%
18	4.645	1011	1028	1059	rBV	193396	497596	28.83%	3.679%
19	4.816	1079	1081	1085	rVB3	716	453	0.03%	0.003%
20	5.083	1146	1164	1185	rBV	313589	691482	40.06%	5.112%
21	5.227	1204	1209	1213	rBV3	473	502	0.03%	0.004%
22	5.301	1229	1232	1238	rBV3	1160	1044	0.06%	0.008%
23	5.375	1252	1255	1258	rBV3	439	365	0.02%	0.003%
24	5.436	1271	1274	1277	rVB3	636	471	0.03%	0.003%
25	5.629	1331	1334	1339	rBV2	477	414	0.02%	0.003%
26	5.742	1347	1369	1392	rBV2	634902	1726008	100.00%	12.761%
27	5.951	1431	1434	1436	rVB3	738	312	0.02%	0.002%
28	6.050	1459	1465	1469	rVB4	791	1061	0.06%	0.008%
29	6.115	1481	1485	1488	rBV2	586	408	0.02%	0.003%
30	6.263	1515	1531	1553	rBV	546717	1022451	59.24%	7.559%
31	6.366	1560	1563	1570	rVB5	747	857	0.05%	0.006%
32	6.539	1608	1617	1631	rBV8	7021	13506	0.78%	0.100%
33	6.703	1651	1668	1686	rBV	411723	790607	45.81%	5.845%
34	6.806	1698	1700	1702	rBV3	632	433	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040267.D
 Acq On : 24 Sep 2020 12:42
 Operator : SY/MD
 Sample : VU0924WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

35	6.915	1730	1734	1739	rVB3	484	379	0.02%	0.003%
36	7.192	1818	1820	1825	rVB3	598	475	0.03%	0.004%
37	7.311	1852	1857	1860	rBV	404	337	0.02%	0.002%
38	7.481	1905	1910	1914	rBV3	409	376	0.02%	0.003%
39	7.575	1925	1939	1959	rBV	230729	409551	23.73%	3.028%
40	7.803	2001	2010	2018	rBV4	2766	4429	0.26%	0.033%
41	7.835	2018	2020	2027	rVB3	518	388	0.02%	0.003%
42	7.906	2027	2042	2057	rBV	766973	1308649	75.82%	9.675%
43	8.054	2086	2088	2091	rBV3	582	379	0.02%	0.003%
44	8.185	2116	2129	2150	rBV	171757	293030	16.98%	2.166%
45	8.333	2173	2175	2180	rVB	552	340	0.02%	0.003%
46	8.362	2180	2184	2188	rBV4	477	578	0.03%	0.004%
47	8.472	2211	2218	2220	rBV3	665	680	0.04%	0.005%
48	8.484	2220	2222	2225	rVB	574	332	0.02%	0.002%
49	8.504	2226	2228	2235	rVB3	706	464	0.03%	0.003%
50	8.558	2235	2245	2249	rBV5	1245	1857	0.11%	0.014%
51	8.639	2257	2270	2303	rBV	542918	964388	55.87%	7.130%
52	8.915	2350	2356	2362	rBV5	1237	1906	0.11%	0.014%
53	8.973	2372	2374	2380	rVB2	733	445	0.03%	0.003%
54	8.999	2380	2382	2386	rBV2	358	325	0.02%	0.002%
55	9.037	2390	2394	2400	rVB2	322	330	0.02%	0.002%
56	9.079	2404	2407	2411	rVV	379	296	0.02%	0.002%
57	9.420	2499	2513	2552	rBV	783324	1293538	74.94%	9.564%
58	9.574	2556	2561	2568	rVB3	1613	1737	0.10%	0.013%
59	9.697	2595	2599	2607	rVB4	1306	1581	0.09%	0.012%
60	9.883	2653	2657	2658	rBV	468	293	0.02%	0.002%
61	10.099	2718	2724	2727	rBV4	1847	2149	0.12%	0.016%
62	10.166	2741	2745	2748	rVB2	413	313	0.02%	0.002%
63	10.227	2758	2764	2766	rBV2	539	437	0.03%	0.003%
64	10.484	2839	2844	2849	rVB2	1092	1163	0.07%	0.009%
65	10.533	2855	2859	2863	rVB2	510	300	0.02%	0.002%
66	10.639	2887	2892	2894	rVV2	542	358	0.02%	0.003%
67	10.754	2913	2928	2945	rBV	527178	853024	49.42%	6.307%
68	10.825	2945	2950	2955	rVB3	865	806	0.05%	0.006%
69	11.041	3014	3017	3023	rVB2	377	319	0.02%	0.002%
70	11.079	3023	3029	3030	rBV	947	603	0.03%	0.004%
71	11.179	3055	3060	3063	rBV3	381	375	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092420\
 Data File : VU040267.D
 Acq On : 24 Sep 2020 12:42
 Operator : SY/MD
 Sample : VU0924WBL02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis

72	11.465	3142	3149	3154	rBV4	1548	2023	0.12%	0.015%
73	11.574	3180	3183	3189	rBV2	338	373	0.02%	0.003%
74	11.745	3227	3236	3241	rVV5	2240	3612	0.21%	0.027%
75	11.806	3242	3255	3274	rVV	759947	1217655	70.55%	9.003%
76	11.877	3274	3277	3282	rVB3	573	456	0.03%	0.003%
77	12.188	3360	3374	3390	rBV	757913	1226575	71.06%	9.069%
78	12.343	3419	3422	3424	rBV2	564	350	0.02%	0.003%
79	12.478	3461	3464	3468	rBV3	438	383	0.02%	0.003%
80	12.648	3514	3517	3520	rBV2	515	395	0.02%	0.003%
81	12.716	3533	3538	3540	rBV2	386	348	0.02%	0.003%
82	12.809	3565	3567	3573	rVB2	682	404	0.02%	0.003%
83	12.883	3587	3590	3594	rBV3	412	294	0.02%	0.002%
84	12.951	3608	3611	3613	rBV	589	345	0.02%	0.003%
85	12.963	3613	3615	3619	rVV	576	332	0.02%	0.002%
86	12.999	3619	3626	3629	rVB5	1134	1377	0.08%	0.010%
87	13.018	3629	3632	3634	rBV2	475	328	0.02%	0.002%
88	13.169	3677	3679	3682	rBV	501	326	0.02%	0.002%
89	13.208	3684	3691	3700	rVB5	3541	5145	0.30%	0.038%
90	13.259	3704	3707	3708	rBV	637	322	0.02%	0.002%
91	13.664	3831	3833	3840	rVB2	752	821	0.05%	0.006%
92	13.703	3840	3845	3849	rBV3	637	576	0.03%	0.004%
93	13.748	3849	3859	3863	rVB3	824	1228	0.07%	0.009%
94	13.783	3863	3870	3875	rBV3	1041	1306	0.08%	0.010%
95	13.832	3876	3885	3893	rBV6	5550	8810	0.51%	0.065%
96	14.076	3954	3961	3972	rVB2	8306	12192	0.71%	0.090%
97	14.317	4029	4036	4045	rVB7	5182	7897	0.46%	0.058%
98	14.484	4086	4088	4091	rVB	728	329	0.02%	0.002%
99	15.304	4340	4343	4347	rBV2	1106	1063	0.06%	0.008%
100	15.712	4468	4470	4471	rBV2	944	442	0.03%	0.003%


Sum of corrected areas: 13525622

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU092420\
Data File : VU040267.D
Acq On : 24 Sep 2020 12:42
Operator : SY/MD
Sample : VU0924WBL02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

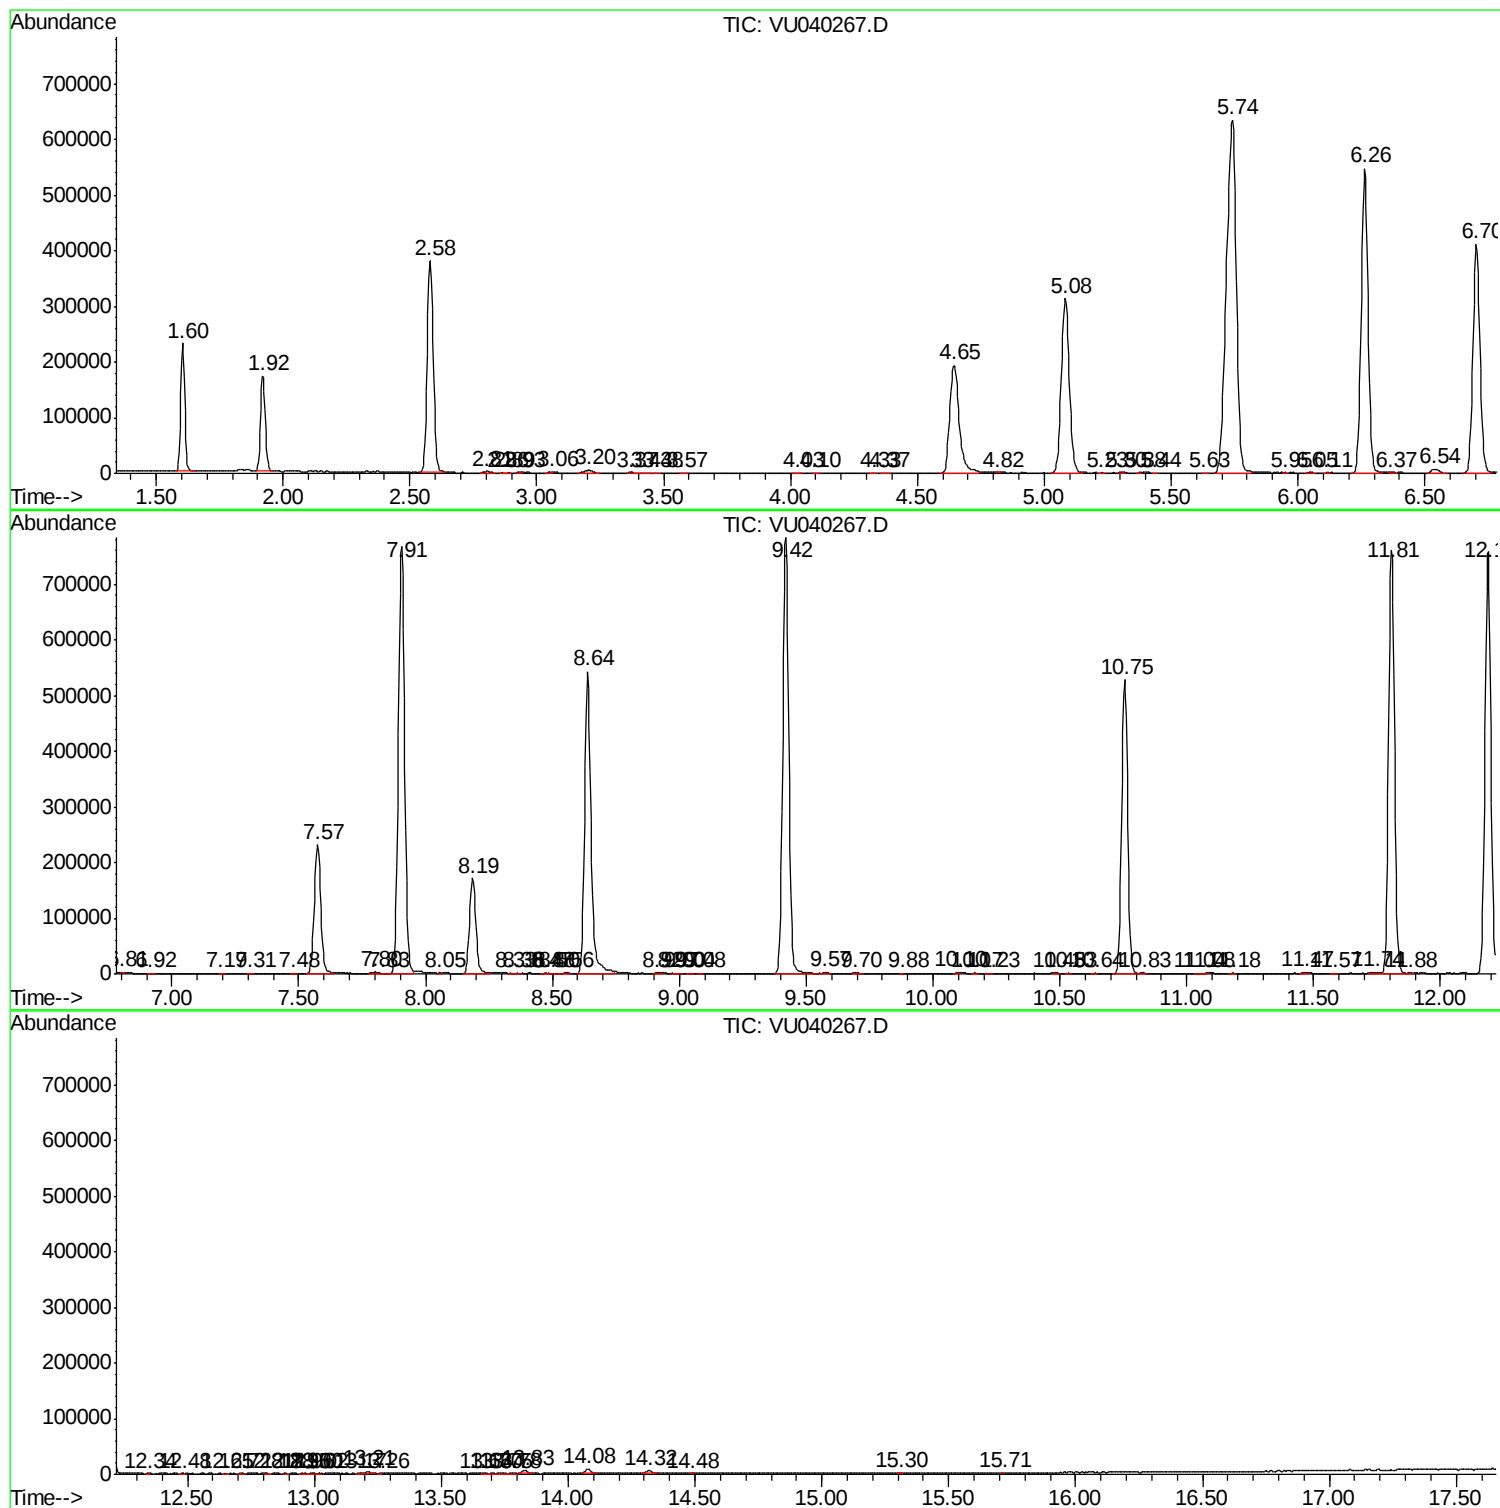

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092420\
Data File : VU040267.D
Acq On : 24 Sep 2020 12:42
Operator : SY/MD
Sample : VU0924WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU092420\
Data File : VU040267.D
Acq On : 24 Sep 2020 12:42
Operator : SY/MD
Sample : VU0924WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc