


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092420\
 Data File : VU040259.D
 Acq On : 24 Sep 2020 08:59
 Operator : SY/MD
 Sample : BFB31
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB201

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM092420WMA.M
 Title : VOC Analysis
 Last Update : Fri Sep 25 09:34:00 2020

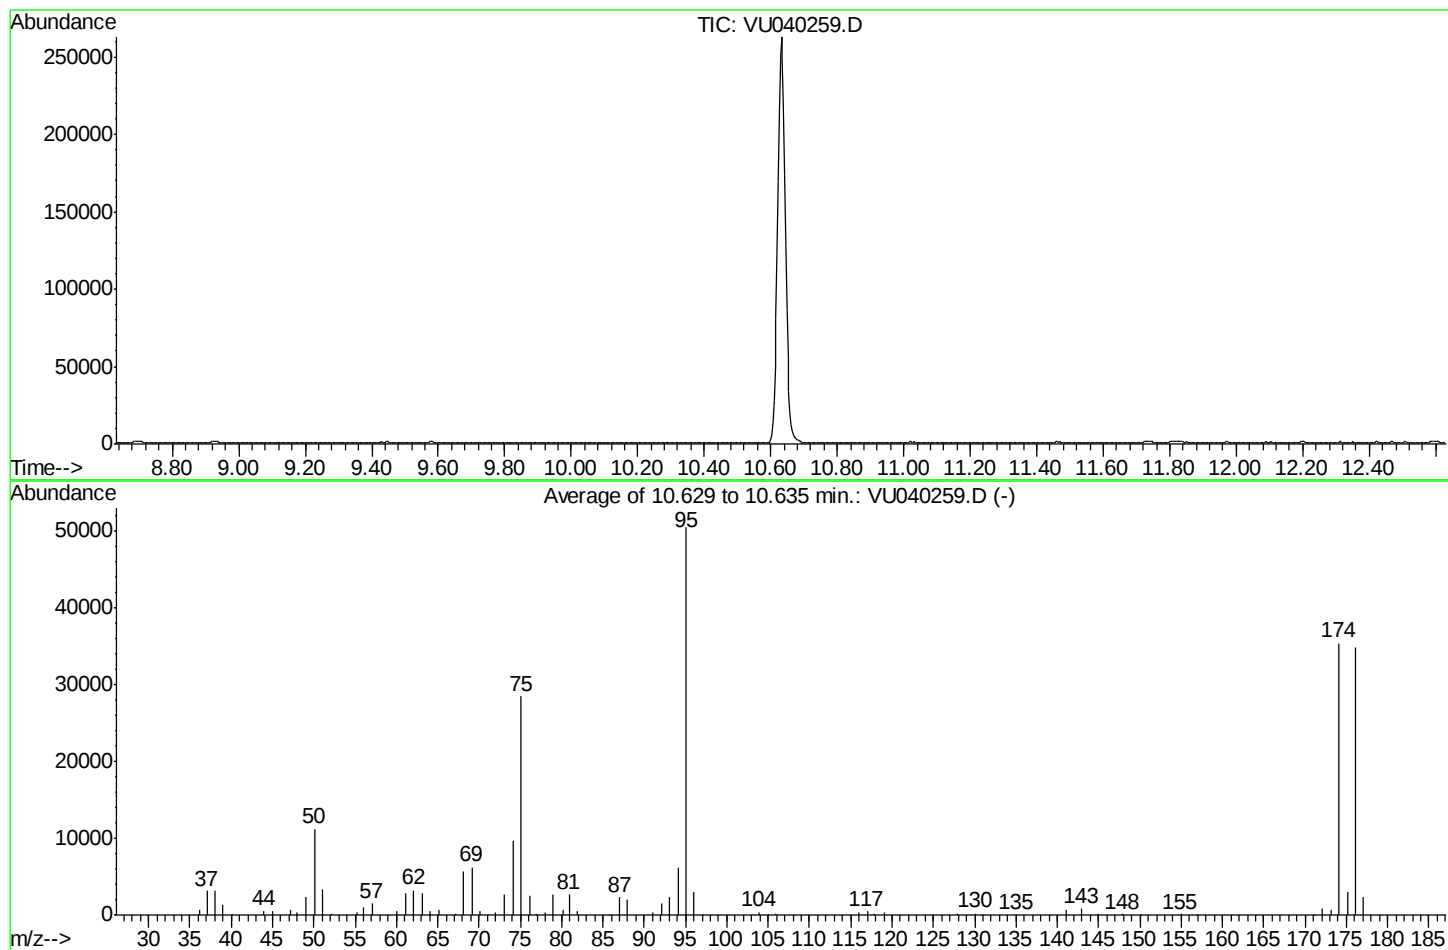

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	11214	PASS
75	95	30	80	56.4	28498	PASS
95	95	100	100	100.0	50538	PASS
96	95	5	9	5.9	2979	PASS
173	174	0.00	2	1.8	630	PASS
174	95	50	120	70.1	35437	PASS
175	174	5	9	8.3	2945	PASS
176	174	95	101	98.3	34842	PASS
177	176	5	9	6.6	2295	PASS

m/z	Abundance
36.10	704.0
37.10	3022.0
38.10	3342.0
39.00	1374.0
40.10	448.0
43.90	1014.0
45.10	534.0
47.10	631.0
48.00	337.0
49.10	2549.0
50.10	10878.0
51.10	3493.0
52.20	203.0
55.20	284.0
56.00	1019.0
57.00	1428.0
60.00	511.0
61.00	2942.0
62.10	3183.0
63.10	2822.0
64.10	598.0
65.10	638.0
67.20	248.0
68.10	5608.0
69.10	5837.0
70.10	485.0
72.00	304.0
73.10	2598.0
74.10	9721.0
75.10	28184.0
76.10	2739.0
77.00	253.0
78.00	214.0
78.90	2714.0
80.10	760.0
80.90	2711.0
81.90	558.0
85.70	108.0
87.00	2294.0
88.00	1907.0
91.00	308.0
92.00	1587.0
93.10	2191.0
94.10	6476.0
95.10	49248.0
96.00	2855.0
97.10	101.0
103.90	325.0
104.90	120.0
105.90	183.0
115.90	286.0
117.00	408.0
117.90	193.0
119.00	412.0
127.90	152.0
130.10	174.0
130.90	120.0
141.00	612.0
143.00	828.0
145.00	142.0
147.90	118.0
155.00	133.0
171.10	108.0
172.10	740.0
173.10	642.0
174.10	34272.0
175.10	2845.0
176.10	33960.0
177.10	2328.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

m/z	Abundance
36.10	690.0
37.10	3288.0
38.10	3215.0
39.00	1344.0
40.10	406.0
44.00	1076.0
45.10	445.0
47.10	718.0
47.90	356.0
49.10	2473.0
50.10	11567.0
51.10	3452.0
52.10	134.0
55.20	326.0
56.00	1135.0
57.10	1426.0
60.00	528.0
61.10	2988.0
62.10	3384.0
63.10	2925.0
64.10	539.0
65.10	591.0
67.10	198.0
68.10	5786.0
69.10	6400.0
70.10	537.0
72.00	286.0
73.10	2669.0
74.10	9995.0
75.10	29368.0
76.10	2647.0
77.00	195.0
78.00	309.0
78.90	2820.0
80.10	730.0
80.90	2702.0
81.90	569.0
85.70	125.0
87.00	2351.0
88.00	2175.0
91.00	328.0
92.00	1465.0
93.10	2405.0
94.10	6487.0
95.10	52256.0
96.00	3060.0
103.90	377.0
105.90	187.0
115.90	288.0
117.00	500.0
117.90	167.0
119.00	378.0
127.90	183.0
130.10	208.0
130.90	135.0
135.10	119.0
141.00	645.0
143.00	793.0
145.00	177.0
147.90	136.0
154.90	148.0
172.10	905.0
173.10	631.0
174.10	36688.0
175.10	3025.0
176.10	35944.0
177.10	2387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

m/z	Abundance
36.10	563.0
37.10	3176.0
38.10	2799.0
39.00	1234.0
40.10	405.0
44.00	1038.0
45.00	407.0
47.10	694.0
48.00	359.0
49.10	2209.0
50.10	11199.0
51.10	3186.0
55.20	224.0
56.00	1107.0
57.00	1433.0
60.00	556.0
61.10	2812.0
62.00	3187.0
63.10	2702.0
64.10	429.0
65.10	603.0
67.00	144.0
68.10	5424.0
69.10	6403.0
70.10	520.0
72.00	254.0
73.10	2654.0
74.10	9312.0
75.10	27944.0
76.10	2351.0
76.90	197.0
78.00	311.0
78.90	2600.0
80.10	686.0
80.90	2546.0
82.00	559.0
87.00	2258.0
88.00	2115.0
91.00	326.0
92.10	1284.0
93.10	2193.0
94.10	5754.0
95.10	50112.0
96.10	3024.0
103.90	362.0
105.90	195.0
115.90	261.0
117.00	503.0
117.90	172.0
119.00	404.0
128.00	191.0
130.10	204.0
141.00	586.0
143.00	699.0
144.90	197.0
147.90	123.0
150.00	116.0
156.90	108.0
171.20	112.0
172.10	864.0
173.10	617.0
174.10	35352.0
175.10	2965.0
176.10	34624.0
177.10	2170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

Scan 2877 (10.590 min): VU040259.D
BFB31

m/z	Abundance
40.00	369.0
44.00	519.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201