

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044801.D
 Acq On : 24 Sep 2021 10:41
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rVB	168310	191985	14.93%	2.032%
2	1.909	169	177	199	rVB	153105	206020	16.02%	2.180%
3	2.568	370	382	410	rVV	261383	443807	34.51%	4.697%
4	2.694	419	421	425	rVB4	242	154	0.01%	0.002%
5	2.713	425	427	432	rVB3	308	190	0.01%	0.002%
6	2.745	434	437	440	rVB	340	241	0.02%	0.003%
7	2.761	440	442	446	rBV2	183	155	0.01%	0.002%
8	2.793	446	452	462	rBV2	1062	1490	0.12%	0.016%
9	2.896	481	484	486	rBV2	121	100	0.01%	0.001%
10	2.938	494	497	498	rBV	353	165	0.01%	0.002%
11	3.047	523	531	533	rBV3	1638	1685	0.13%	0.018%
12	3.182	569	573	574	rBV2	365	257	0.02%	0.003%
13	3.227	584	587	591	rVB3	351	264	0.02%	0.003%
14	3.256	592	596	598	rBV	136	111	0.01%	0.001%
15	3.308	607	612	618	rBV2	199	275	0.02%	0.003%
16	3.343	620	623	626	rVV2	167	141	0.01%	0.001%
17	3.359	626	628	633	rVB2	142	97	0.01%	0.001%
18	3.385	633	636	639	rBV2	151	100	0.01%	0.001%
19	3.562	688	691	694	rBV	226	189	0.01%	0.002%
20	3.703	732	735	737	rBV2	209	160	0.01%	0.002%
21	3.723	738	741	744	rVB2	166	136	0.01%	0.001%
22	3.938	805	808	815	rVV2	98	98	0.01%	0.001%
23	4.025	833	835	840	rVB2	191	167	0.01%	0.002%
24	4.051	840	843	845	rBV	145	119	0.01%	0.001%
25	4.079	850	852	855	rVV2	161	106	0.01%	0.001%
26	4.102	856	859	862	rVV2	121	95	0.01%	0.001%
27	4.134	867	869	873	rBV2	120	97	0.01%	0.001%
28	4.179	879	883	885	rBV	125	111	0.01%	0.001%
29	4.337	929	932	937	rVB2	144	138	0.01%	0.001%
30	4.420	955	958	960	rBV	146	99	0.01%	0.001%
31	4.636	1010	1025	1056	rBV2	145597	403619	31.39%	4.272%
32	4.886	1099	1103	1111	rBV2	277	396	0.03%	0.004%
33	4.986	1131	1134	1137	rVB	154	131	0.01%	0.001%
34	5.070	1143	1160	1185	rBV	227276	497687	38.70%	5.267%
35	5.292	1226	1229	1230	rBV	229	141	0.01%	0.001%
36	5.382	1253	1257	1259	rBV	261	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044801.D
 Acq On : 24 Sep 2021 10:41
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.729	1343	1365	1394	rBV2	471074	1285861	100.00%	13.609%
38	6.025	1452	1457	1459	rBV2	284	313	0.02%	0.003%
39	6.128	1484	1489	1492	rBV2	270	253	0.02%	0.003%
40	6.147	1492	1495	1499	rVB2	260	234	0.02%	0.002%
41	6.253	1514	1528	1555	rBV	319562	606030	47.13%	6.414%
42	6.349	1555	1558	1559	rBV2	211	107	0.01%	0.001%
43	6.536	1606	1616	1626	rVB8	3601	6824	0.53%	0.072%
44	6.697	1648	1666	1693	rBV	305158	596054	46.35%	6.309%
45	6.796	1693	1697	1698	rBV2	353	223	0.02%	0.002%
46	7.057	1770	1778	1789	rVB4	527	996	0.08%	0.011%
47	7.108	1789	1794	1797	rBV2	129	136	0.01%	0.001%
48	7.189	1811	1819	1827	rVB3	1435	2130	0.17%	0.023%
49	7.391	1877	1882	1884	rBV2	115	108	0.01%	0.001%
50	7.439	1894	1897	1899	rBV2	206	175	0.01%	0.002%
51	7.571	1922	1938	1954	rBV	158507	279953	21.77%	2.963%
52	7.690	1966	1975	1980	rBV3	960	1485	0.12%	0.016%
53	7.713	1980	1982	1986	rVB3	423	241	0.02%	0.003%
54	7.758	1993	1996	2002	rVB2	157	143	0.01%	0.002%
55	7.806	2002	2011	2018	rBV3	816	1199	0.09%	0.013%
56	7.902	2026	2041	2056	rBV	553484	941833	73.25%	9.968%
57	7.970	2057	2062	2074	rVB	8103	14081	1.10%	0.149%
58	8.182	2116	2128	2149	rBV	112768	186809	14.53%	1.977%
59	8.462	2212	2215	2217	rBV	162	127	0.01%	0.001%
60	8.642	2257	2271	2302	rBV	486421	854295	66.44%	9.042%
61	9.192	2438	2442	2443	rBV	257	206	0.02%	0.002%
62	9.263	2460	2464	2467	rBV2	119	109	0.01%	0.001%
63	9.420	2500	2513	2553	rVB	454998	750840	58.39%	7.947%
64	9.574	2555	2561	2568	rVV	481	638	0.05%	0.007%
65	9.697	2592	2599	2606	rVB3	959	1358	0.11%	0.014%
66	9.822	2634	2638	2644	rBV	155	167	0.01%	0.002%
67	9.925	2667	2670	2675	rVB	137	100	0.01%	0.001%
68	10.053	2708	2710	2712	rBV	170	102	0.01%	0.001%
69	10.082	2714	2719	2721	rBV	202	183	0.01%	0.002%
70	10.108	2721	2727	2728	rBV2	438	346	0.03%	0.004%
71	10.349	2799	2802	2805	rBV2	163	105	0.01%	0.001%
72	10.459	2830	2836	2841	rBV2	228	362	0.03%	0.004%
73	10.484	2841	2844	2850	rVV3	312	319	0.02%	0.003%
74	10.629	2882	2889	2893	rBV	216	286	0.02%	0.003%
75	10.677	2896	2904	2914	rBV3	2074	3054	0.24%	0.032%
76	10.761	2917	2930	2949	rBV	419140	674956	52.49%	7.144%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044801.D
 Acq On : 24 Sep 2021 10:41
 Operator : SY/MD
 Sample : VU0924WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK007

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.870	2959	2964	2965	rBV3	304	231	0.02%	0.002%
78	10.883	2965	2968	2971	rBV3	338	259	0.02%	0.003%
79	11.057	3019	3022	3026	rBV2	148	124	0.01%	0.001%
80	11.086	3028	3031	3033	rBV2	392	270	0.02%	0.003%
81	11.121	3038	3042	3048	rBV2	323	384	0.03%	0.004%
82	11.153	3048	3052	3055	rBV3	305	210	0.02%	0.002%
83	11.436	3137	3140	3141	rBV2	177	107	0.01%	0.001%
84	11.462	3141	3148	3149	rBV4	1478	1476	0.11%	0.016%
85	11.574	3181	3183	3186	rBV	193	152	0.01%	0.002%
86	11.697	3215	3221	3222	rBV2	744	710	0.06%	0.008%
87	11.745	3232	3236	3243	rVB2	734	900	0.07%	0.010%
88	11.815	3245	3258	3285	rVB	421104	653503	50.82%	6.917%
89	11.912	3285	3288	3291	rBV	230	185	0.01%	0.002%
90	11.938	3291	3296	3297	rBV3	685	540	0.04%	0.006%
91	12.195	3363	3376	3394	rBV	493013	805630	62.65%	8.527%
92	13.057	3639	3644	3648	rBV2	279	359	0.03%	0.004%
93	13.227	3692	3697	3703	rVB3	1026	1184	0.09%	0.013%
94	13.311	3720	3723	3725	rBV	237	182	0.01%	0.002%
95	13.844	3882	3889	3899	rVB5	2166	3078	0.24%	0.033%
96	14.092	3956	3966	3976	rBV2	6598	10193	0.79%	0.108%
97	14.333	4034	4041	4053	rBV3	2873	3947	0.31%	0.042%
98	15.111	4279	4283	4286	rBV2	438	450	0.03%	0.005%
99	15.188	4305	4307	4310	rBV2	350	245	0.02%	0.003%
100	16.156	4606	4608	4613	rBV3	491	423	0.03%	0.004%


Sum of corrected areas: 9448385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044801.D
Acq On : 24 Sep 2021 10:41
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

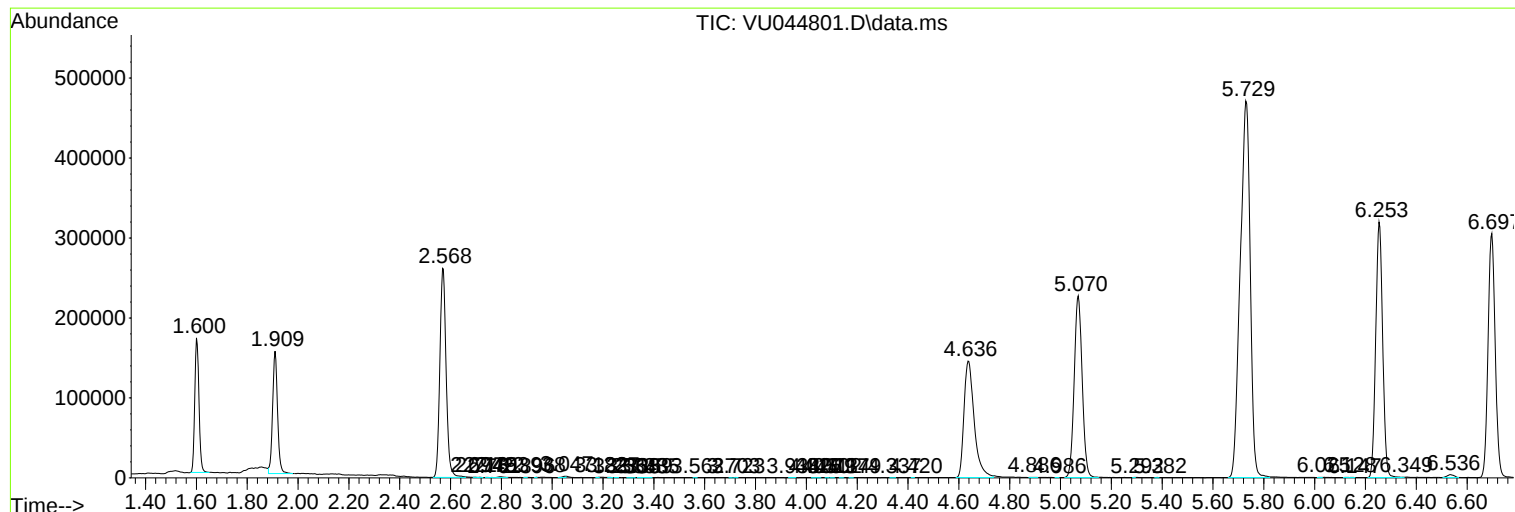

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044801.D
Acq On : 24 Sep 2021 10:41
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044801.D
Acq On : 24 Sep 2021 10:41
Operator : SY/MD
Sample : VU0924WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
