

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044804.D
 Acq On : 24 Sep 2021 12:05
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	166750	191158	15.29%	2.052%
2	1.913	170	178	194	rVB	138559	187706	15.01%	2.015%
3	2.572	370	383	399	rBV	255184	427681	34.20%	4.592%
4	2.794	442	452	453	rBV3	2156	2643	0.21%	0.028%
5	2.961	500	504	509	rVV2	299	352	0.03%	0.004%
6	3.006	515	518	520	rBV2	196	166	0.01%	0.002%
7	3.051	525	532	543	rVB3	548	1122	0.09%	0.012%
8	3.144	558	561	564	rVB	198	145	0.01%	0.002%
9	3.189	568	575	580	rVV3	487	658	0.05%	0.007%
10	3.212	580	582	588	rVB2	205	189	0.02%	0.002%
11	3.344	614	623	624	rBV2	300	313	0.03%	0.003%
12	3.360	624	628	636	rVB3	591	773	0.06%	0.008%
13	3.414	643	645	646	rBV3	285	122	0.01%	0.001%
14	3.450	653	656	659	rBV2	182	130	0.01%	0.001%
15	3.524	676	679	682	rBV2	145	146	0.01%	0.002%
16	3.633	707	713	716	rBV2	222	272	0.02%	0.003%
17	3.694	729	732	737	rVV	223	224	0.02%	0.002%
18	3.723	738	741	748	rVB2	227	214	0.02%	0.002%
19	3.781	751	759	763	rBV2	302	429	0.03%	0.005%
20	3.887	785	792	794	rBV2	162	191	0.02%	0.002%
21	4.016	828	832	836	rBV2	142	150	0.01%	0.002%
22	4.074	847	850	853	rVB2	208	147	0.01%	0.002%
23	4.109	858	861	864	rBV	168	143	0.01%	0.002%
24	4.218	893	895	898	rVB2	225	135	0.01%	0.001%
25	4.241	898	902	905	rBV2	208	213	0.02%	0.002%
26	4.562	998	1002	1004	rBV2	166	175	0.01%	0.002%
27	4.636	1008	1025	1064	rBV	139507	449908	35.98%	4.830%
28	4.826	1082	1084	1090	rVB	256	140	0.01%	0.002%
29	5.070	1142	1160	1185	rVV	216240	487484	38.99%	5.234%
30	5.299	1226	1231	1235	rVB2	574	525	0.04%	0.006%
31	5.366	1249	1252	1255	rBV2	215	175	0.01%	0.002%
32	5.398	1259	1262	1265	rBV2	129	117	0.01%	0.001%
33	5.414	1265	1267	1272	rVB2	207	176	0.01%	0.002%
34	5.447	1273	1277	1280	rBV2	269	258	0.02%	0.003%
35	5.463	1280	1282	1288	rVB2	166	126	0.01%	0.001%
36	5.633	1332	1335	1340	rVB2	191	198	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044804.D
 Acq On : 24 Sep 2021 12:05
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.729	1342	1365	1392	rBV2	460513	1250348	100.00%	13.424%
38	6.254	1513	1528	1545	rBV	326819	621421	49.70%	6.672%
39	6.337	1552	1554	1557	rVB2	455	230	0.02%	0.002%
40	6.360	1559	1561	1567	rVV3	416	396	0.03%	0.004%
41	6.389	1568	1570	1575	rVB	530	307	0.02%	0.003%
42	6.437	1582	1585	1590	rVB3	398	354	0.03%	0.004%
43	6.479	1590	1598	1602	rBV2	291	461	0.04%	0.005%
44	6.537	1607	1616	1623	rBV7	2889	4987	0.40%	0.054%
45	6.591	1632	1633	1636	rVB	318	123	0.01%	0.001%
46	6.610	1636	1639	1644	rVB	287	318	0.03%	0.003%
47	6.697	1648	1666	1687	rBV	294996	577226	46.17%	6.197%
48	6.810	1697	1701	1705	rVB4	818	673	0.05%	0.007%
49	6.852	1712	1714	1719	rVB2	260	199	0.02%	0.002%
50	6.884	1719	1724	1727	rBV2	258	237	0.02%	0.003%
51	7.048	1770	1775	1778	rBV2	395	428	0.03%	0.005%
52	7.186	1811	1818	1826	rBV3	1353	2183	0.17%	0.023%
53	7.241	1831	1835	1838	rBV	253	221	0.02%	0.002%
54	7.279	1843	1847	1851	rBV2	186	211	0.02%	0.002%
55	7.337	1862	1865	1869	rBV	255	233	0.02%	0.003%
56	7.373	1869	1876	1878	rBV2	209	295	0.02%	0.003%
57	7.569	1924	1937	1954	rBV	153136	269139	21.53%	2.890%
58	7.688	1970	1974	1978	rBV4	859	695	0.06%	0.007%
59	7.903	2026	2041	2056	rBV	531117	916720	73.32%	9.842%
60	7.974	2057	2063	2075	rVB3	8493	13918	1.11%	0.149%
61	8.183	2116	2128	2150	rBV	106011	180640	14.45%	1.939%
62	8.318	2166	2170	2171	rBV2	196	117	0.01%	0.001%
63	8.475	2212	2219	2221	rBV3	760	815	0.07%	0.009%
64	8.639	2256	2270	2315	rBV	464043	825241	66.00%	8.860%
65	8.884	2342	2346	2349	rBV3	215	190	0.02%	0.002%
66	8.958	2367	2369	2371	rBV	209	140	0.01%	0.002%
67	9.032	2387	2392	2395	rBV	203	196	0.02%	0.002%
68	9.106	2409	2415	2418	rVB	256	263	0.02%	0.003%
69	9.134	2418	2424	2427	rBV2	175	209	0.02%	0.002%
70	9.356	2488	2493	2495	rBV	152	162	0.01%	0.002%
71	9.421	2500	2513	2553	rVV	471113	775320	62.01%	8.324%
72	9.572	2555	2560	2567	rVB3	456	517	0.04%	0.006%
73	9.700	2592	2600	2608	rVB2	838	1090	0.09%	0.012%
74	10.025	2697	2701	2703	rBV	154	118	0.01%	0.001%
75	10.302	2784	2787	2791	rBV2	148	136	0.01%	0.001%
76	10.475	2837	2841	2848	rBV2	208	287	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044804.D
 Acq On : 24 Sep 2021 12:05
 Operator : SY/MD
 Sample : M3873-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.597	2876	2879	2883	rBV2	189	166	0.01%	0.002%
78	10.678	2896	2904	2912	rVB3	2234	2855	0.23%	0.031%
79	10.761	2917	2930	2951	rVB	407331	651047	52.07%	6.990%
80	10.858	2957	2960	2962	rBV	250	167	0.01%	0.002%
81	11.003	3001	3005	3011	rVB3	256	232	0.02%	0.002%
82	11.093	3030	3033	3038	rVB2	251	164	0.01%	0.002%
83	11.118	3038	3041	3045	rVB2	379	303	0.02%	0.003%
84	11.298	3095	3097	3103	rBV2	262	307	0.02%	0.003%
85	11.459	3140	3147	3149	rBV3	1210	1337	0.11%	0.014%
86	11.700	3218	3222	3227	rVB3	781	860	0.07%	0.009%
87	11.816	3246	3258	3276	rBV	423209	669570	53.55%	7.189%
88	11.929	3290	3293	3294	rBV2	435	267	0.02%	0.003%
89	11.977	3304	3308	3318	rVB4	1377	1682	0.13%	0.018%
90	12.073	3334	3338	3344	rVB2	921	885	0.07%	0.010%
91	12.195	3362	3376	3393	rBV	483634	779834	62.37%	8.373%
92	12.459	3454	3458	3460	rBV2	244	210	0.02%	0.002%
93	12.636	3510	3513	3516	rVB	243	130	0.01%	0.001%
94	12.694	3528	3531	3534	rBV	157	135	0.01%	0.001%
95	12.819	3567	3570	3573	rBV	235	162	0.01%	0.002%
96	12.864	3578	3584	3587	rBV2	265	332	0.03%	0.004%
97	13.086	3651	3653	3659	rBV	206	215	0.02%	0.002%
98	14.096	3964	3967	3976	rVB3	1043	1243	0.10%	0.013%
99	14.250	4009	4015	4018	rBV2	332	403	0.03%	0.004%
100	15.002	4246	4249	4251	rBV3	336	202	0.02%	0.002%




Sum of corrected areas: 9314176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044804.D
Acq On : 24 Sep 2021 12:05
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

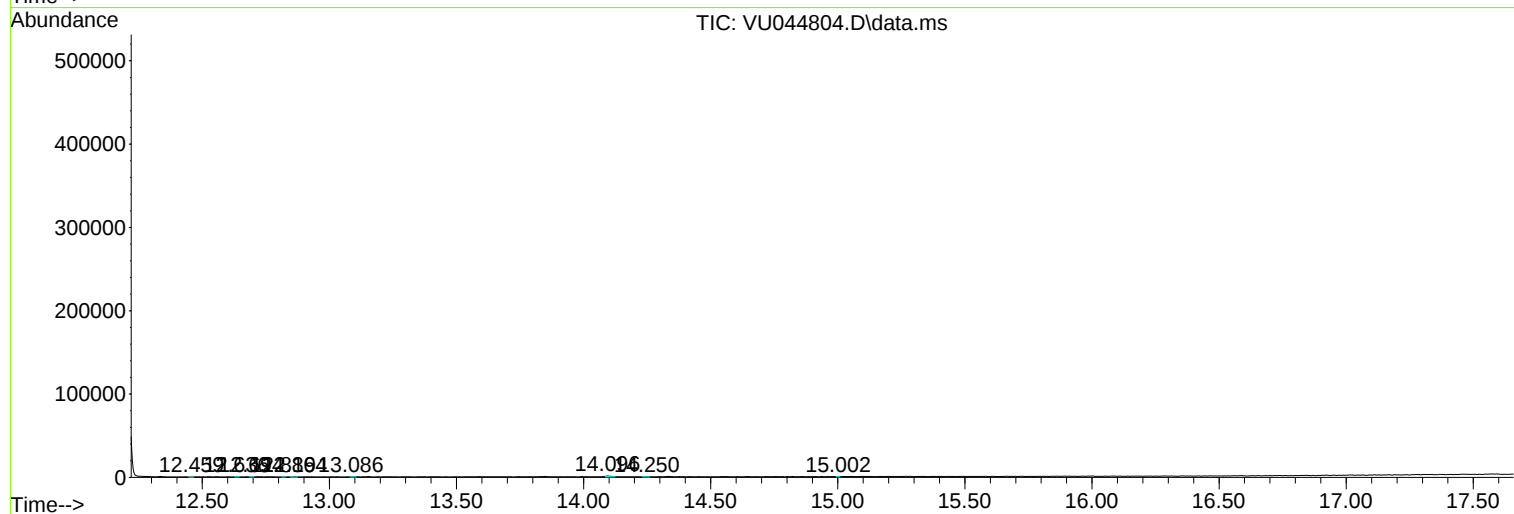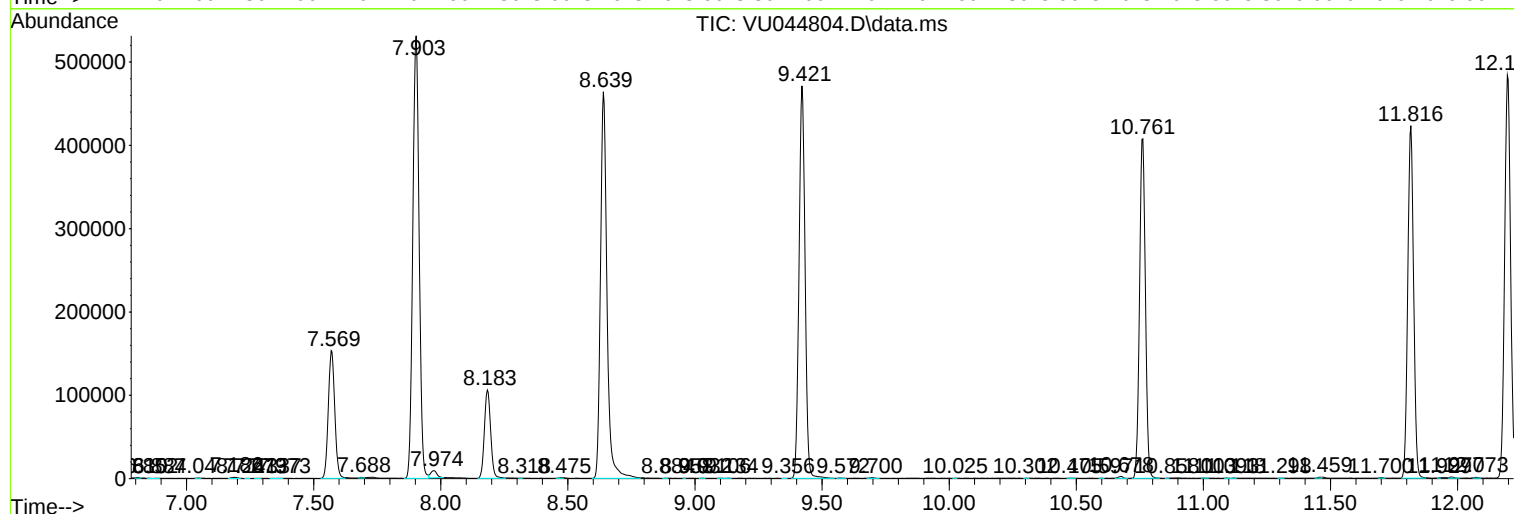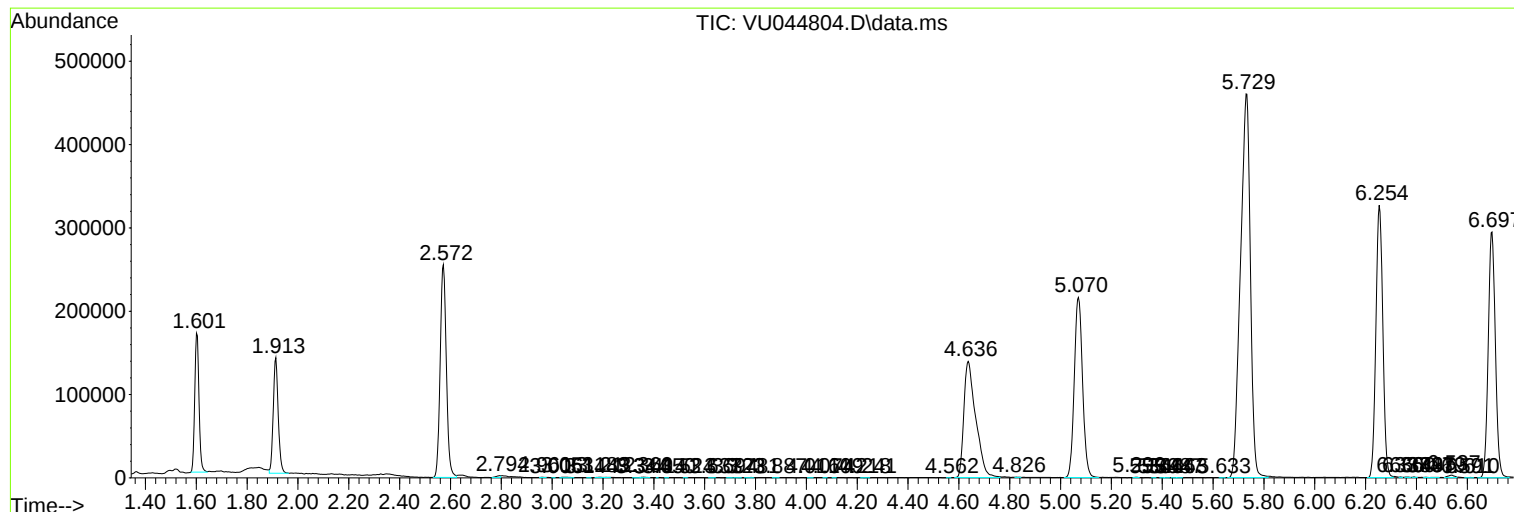

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044804.D
Acq On : 24 Sep 2021 12:05
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044804.D
Acq On : 24 Sep 2021 12:05
Operator : SY/MD
Sample : M3873-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
