

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044807.D
 Acq On : 24 Sep 2021 13:15
 Operator : SY/MD
 Sample : M3873-05DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	38	42	48	rBV2	5913	5279	0.43%	0.051%
2	1.600	74	81	93	rBV	162388	184900	15.02%	1.798%
3	1.912	170	178	191	rVB	141630	188701	15.32%	1.835%
4	2.571	370	383	407	rBV	245016	415407	33.74%	4.040%
5	2.771	441	445	447	rBV2	218	216	0.02%	0.002%
6	2.793	450	452	462	rVB3	484	640	0.05%	0.006%
7	2.954	494	502	503	rBV	418	442	0.04%	0.004%
8	2.986	510	512	519	rVB2	296	242	0.02%	0.002%
9	3.050	523	532	541	rVB3	3656	6220	0.51%	0.060%
10	3.095	544	546	548	rBV	139	93	0.01%	0.001%
11	3.137	556	559	564	rBV	290	317	0.03%	0.003%
12	3.173	564	570	571	rBV2	377	289	0.02%	0.003%
13	3.304	606	611	614	rBV2	255	234	0.02%	0.002%
14	3.359	618	628	638	rVB2	4316	8341	0.68%	0.081%
15	3.427	645	649	652	rVB2	158	126	0.01%	0.001%
16	3.449	652	656	659	rBV	160	155	0.01%	0.002%
17	3.494	667	670	675	rVB2	164	147	0.01%	0.001%
18	3.517	675	677	680	rBV2	123	103	0.01%	0.001%
19	3.571	689	694	697	rVB2	172	165	0.01%	0.002%
20	3.626	707	711	714	rVB2	209	175	0.01%	0.002%
21	3.649	714	718	720	rBV2	199	146	0.01%	0.001%
22	3.790	758	762	763	rBV2	187	136	0.01%	0.001%
23	3.832	771	775	777	rBV	230	146	0.01%	0.001%
24	3.848	777	780	784	rBV2	146	166	0.01%	0.002%
25	3.909	794	799	802	rBV	223	244	0.02%	0.002%
26	3.957	810	814	817	rVB2	179	122	0.01%	0.001%
27	3.973	817	819	823	rVB	196	123	0.01%	0.001%
28	4.009	827	830	833	rBV	177	150	0.01%	0.001%
29	4.108	859	861	863	rBV2	166	117	0.01%	0.001%
30	4.137	867	870	874	rVB2	168	108	0.01%	0.001%
31	4.558	998	1001	1005	rVB2	219	168	0.01%	0.002%
32	4.578	1005	1007	1010	rBV2	144	102	0.01%	0.001%
33	4.642	1010	1027	1030	rBV2	146233	304433	24.72%	2.961%
34	4.922	1111	1114	1118	rBV2	167	146	0.01%	0.001%
35	5.070	1143	1160	1182	rBV	217942	483365	39.25%	4.701%
36	5.221	1204	1207	1208	rBV3	233	102	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044807.D
 Acq On : 24 Sep 2021 13:15
 Operator : SY/MD
 Sample : M3873-05DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.285	1223	1227	1228	rBV2	179	123	0.01%	0.001%
38	5.349	1241	1247	1254	rVB2	362	430	0.03%	0.004%
39	5.385	1254	1258	1260	rBV2	170	143	0.01%	0.001%
40	5.423	1267	1270	1274	rVB	168	128	0.01%	0.001%
41	5.459	1274	1281	1283	rBV	156	162	0.01%	0.002%
42	5.501	1286	1294	1298	rVB2	154	233	0.02%	0.002%
43	5.732	1343	1366	1399	rBV2	450982	1231372	100.00%	11.975%
44	5.880	1410	1412	1415	rVV2	325	181	0.01%	0.002%
45	6.166	1497	1501	1502	rBV2	212	138	0.01%	0.001%
46	6.189	1505	1508	1513	rVB2	348	285	0.02%	0.003%
47	6.253	1513	1528	1550	rBV	346425	651421	52.90%	6.335%
48	6.546	1605	1619	1639	rBV	580564	1095213	88.94%	10.651%
49	6.697	1652	1666	1687	rVB	295321	573199	46.55%	5.574%
50	6.890	1724	1726	1728	rVB2	263	106	0.01%	0.001%
51	6.928	1735	1738	1740	rBV2	192	119	0.01%	0.001%
52	7.041	1769	1773	1774	rBV	287	194	0.02%	0.002%
53	7.054	1774	1777	1785	rVB	555	642	0.05%	0.006%
54	7.086	1785	1787	1794	rVB2	161	171	0.01%	0.002%
55	7.121	1794	1798	1800	rBV2	153	129	0.01%	0.001%
56	7.189	1808	1819	1829	rVB4	1673	2702	0.22%	0.026%
57	7.497	1909	1915	1918	rBV	121	142	0.01%	0.001%
58	7.571	1925	1938	1956	rBV	150642	268029	21.77%	2.607%
59	7.690	1968	1975	1976	rBV3	815	895	0.07%	0.009%
60	7.902	2026	2041	2056	rBV	528069	900101	73.10%	8.753%
61	8.182	2116	2128	2144	rBV	105756	178767	14.52%	1.738%
62	8.279	2154	2158	2159	rVB3	243	143	0.01%	0.001%
63	8.291	2159	2162	2166	rBV	257	251	0.02%	0.002%
64	8.449	2207	2211	2213	rBV2	251	215	0.02%	0.002%
65	8.533	2233	2237	2243	rBV2	182	224	0.02%	0.002%
66	8.581	2249	2252	2254	rBV	166	136	0.01%	0.001%
67	8.642	2257	2271	2321	rVV	455314	829963	67.40%	8.071%
68	8.983	2372	2377	2379	rBV2	123	130	0.01%	0.001%
69	9.211	2441	2448	2451	rBV2	265	321	0.03%	0.003%
70	9.420	2500	2513	2530	rBV	488420	807895	65.61%	7.857%
71	9.571	2557	2560	2568	rVB3	385	521	0.04%	0.005%
72	10.050	2706	2709	2710	rBV	170	113	0.01%	0.001%
73	10.098	2719	2724	2728	rBV2	291	315	0.03%	0.003%
74	10.227	2761	2764	2769	rBV	230	222	0.02%	0.002%
75	10.674	2896	2903	2916	rVB2	2071	2988	0.24%	0.029%
76	10.761	2916	2930	2952	rBV	408622	647516	52.58%	6.297%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044807.D
 Acq On : 24 Sep 2021 13:15
 Operator : SY/MD
 Sample : M3873-05DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.857	2957	2960	2961	rBV	228	123	0.01%	0.001%
78	10.873	2961	2965	2969	rBV3	447	444	0.04%	0.004%
79	10.896	2969	2972	2975	rBV	239	141	0.01%	0.001%
80	10.934	2981	2984	2987	rBV	193	135	0.01%	0.001%
81	11.041	3015	3017	3024	rVB2	335	235	0.02%	0.002%
82	11.073	3024	3027	3030	rBV	158	112	0.01%	0.001%
83	11.462	3139	3148	3149	rBV3	1281	1348	0.11%	0.013%
84	11.581	3183	3185	3191	rVB2	284	250	0.02%	0.002%
85	11.700	3216	3222	3230	rVB5	841	1146	0.09%	0.011%
86	11.735	3230	3233	3236	rBV	116	101	0.01%	0.001%
87	11.815	3245	3258	3277	rBV	448361	702841	57.08%	6.835%
88	11.934	3292	3295	3297	rBV2	475	286	0.02%	0.003%
89	11.976	3304	3308	3314	rVB3	1270	1395	0.11%	0.014%
90	12.028	3321	3324	3328	rBV	195	111	0.01%	0.001%
91	12.069	3335	3337	3340	rBV2	218	104	0.01%	0.001%
92	12.108	3347	3349	3352	rVB2	218	100	0.01%	0.001%
93	12.198	3364	3377	3399	rBV	479200	774611	62.91%	7.533%
94	12.555	3486	3488	3489	rBV	222	110	0.01%	0.001%
95	12.680	3524	3527	3532	rBV	236	174	0.01%	0.002%
96	13.452	3764	3767	3770	rBV2	282	222	0.02%	0.002%
97	14.397	4056	4061	4067	rBV2	238	372	0.03%	0.004%
98	14.864	4203	4206	4209	rBV2	290	219	0.02%	0.002%
99	15.021	4253	4255	4258	rBV2	244	141	0.01%	0.001%
100	15.526	4409	4412	4414	rBV2	380	274	0.02%	0.003%




Sum of corrected areas: 10282939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044807.D
Acq On : 24 Sep 2021 13:15
Operator : SY/MD
Sample : M3873-05DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

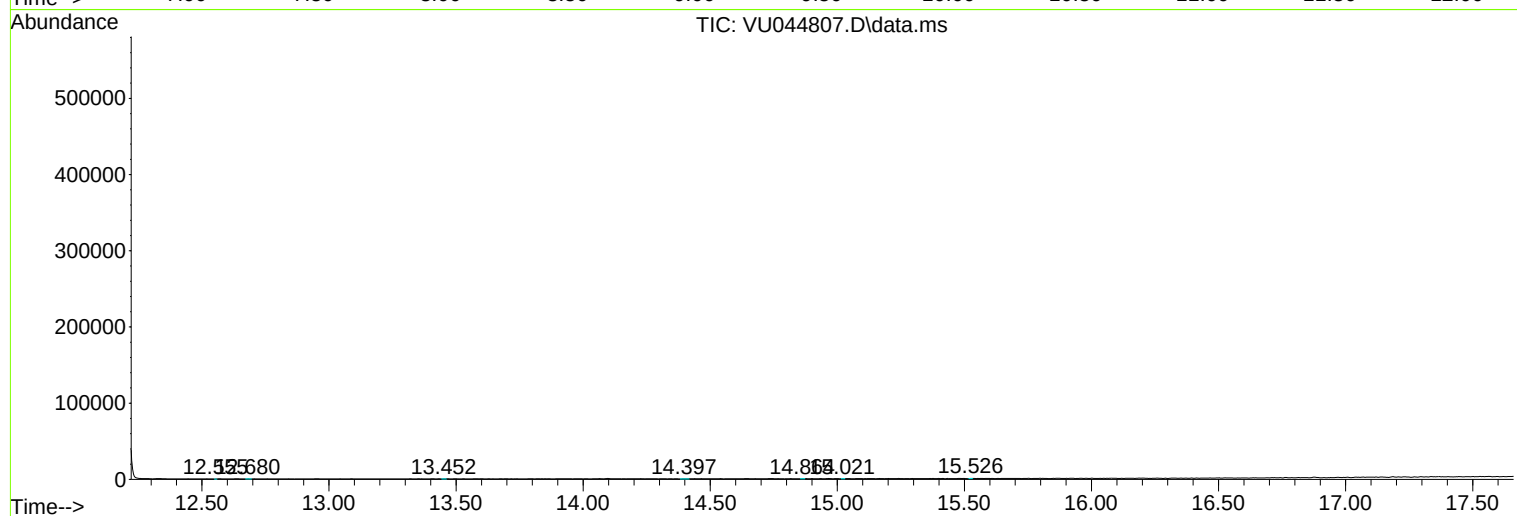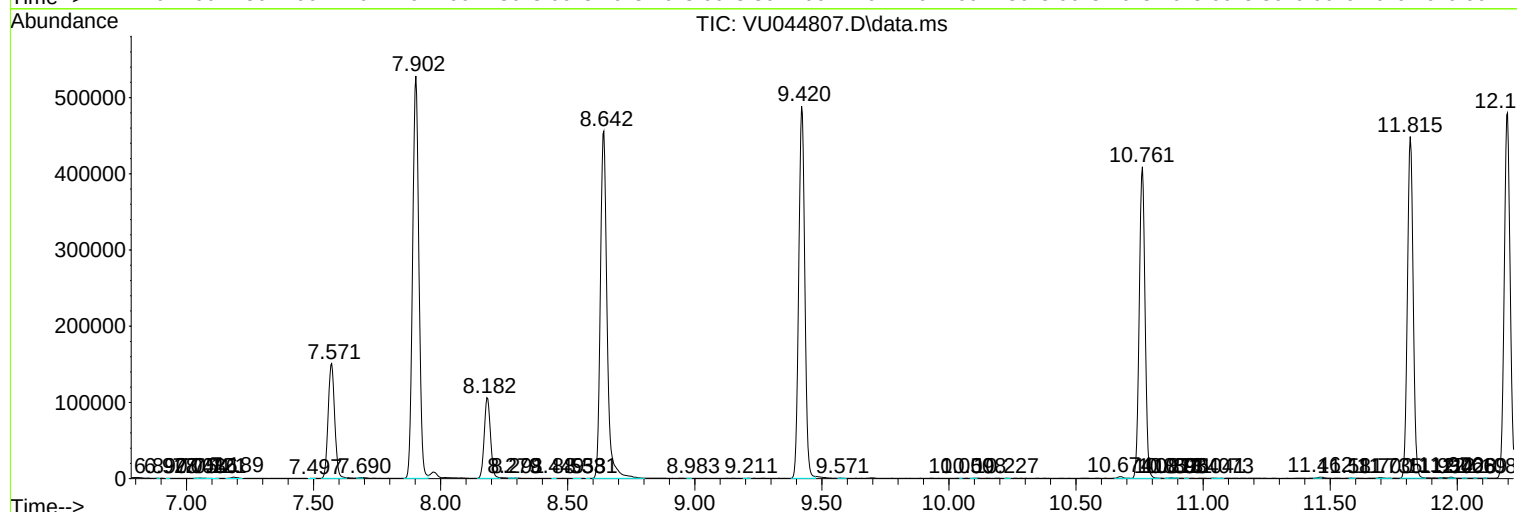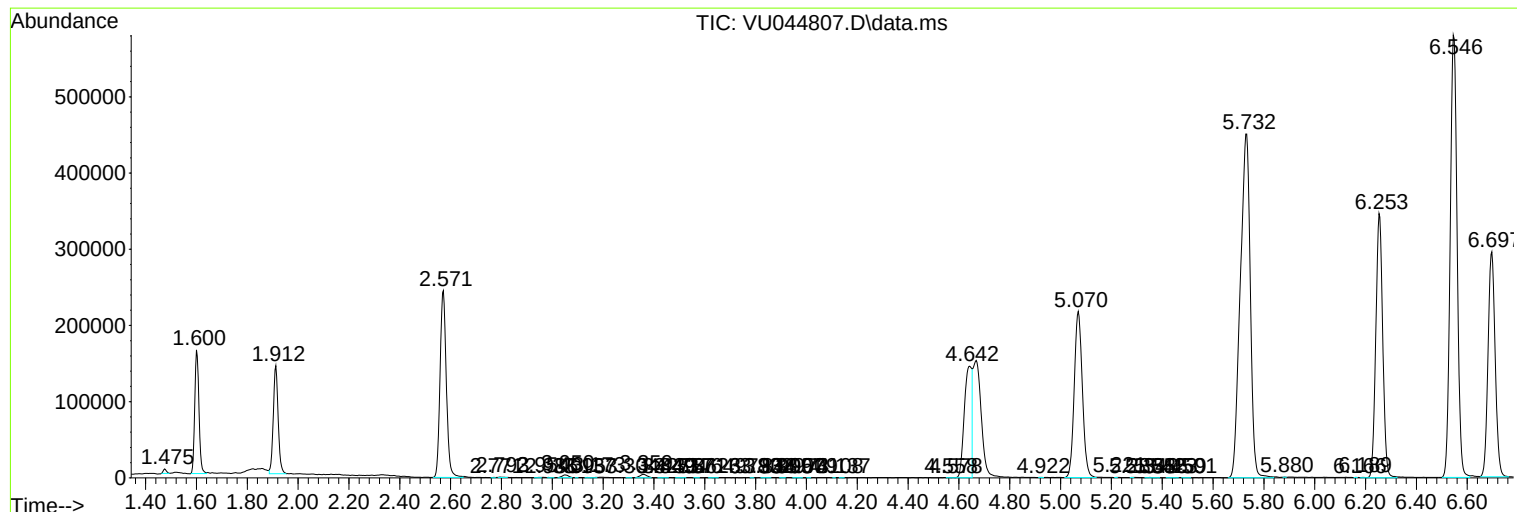

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044807.D
Acq On : 24 Sep 2021 13:15
Operator : SY/MD
Sample : M3873-05DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044807.D
Acq On : 24 Sep 2021 13:15
Operator : SY/MD
Sample : M3873-05DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
