

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044812.D
 Acq On : 24 Sep 2021 15:10
 Operator : SY/MD
 Sample : M3873-16DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	157720	178766	14.36%	1.820%
2	1.909	169	177	195	rVB	125802	171584	13.78%	1.746%
3	2.568	370	382	403	rBV	235597	394942	31.73%	4.020%
4	2.700	420	423	424	rBV	233	138	0.01%	0.001%
5	2.777	444	447	449	rBV	328	244	0.02%	0.002%
6	2.909	487	488	492	rBV	179	104	0.01%	0.001%
7	2.957	499	503	504	rBV2	280	195	0.02%	0.002%
8	3.051	522	532	545	rVB2	4126	7293	0.59%	0.074%
9	3.202	568	579	588	rVB4	641	1382	0.11%	0.014%
10	3.244	588	592	599	rBV	261	270	0.02%	0.003%
11	3.321	613	616	617	rBV	222	153	0.01%	0.002%
12	3.359	617	628	639	rVB3	4788	8844	0.71%	0.090%
13	3.404	639	642	646	rBV2	185	165	0.01%	0.002%
14	3.459	656	659	661	rBV2	183	131	0.01%	0.001%
15	3.520	675	678	681	rVB	163	144	0.01%	0.001%
16	3.539	681	684	686	rBV2	118	89	0.01%	0.001%
17	3.716	735	739	742	rBV2	119	111	0.01%	0.001%
18	3.771	752	756	759	rBV2	178	154	0.01%	0.002%
19	3.832	772	775	778	rBV2	159	129	0.01%	0.001%
20	3.874	785	788	791	rBV2	101	69	0.01%	0.001%
21	4.054	840	844	848	rBV2	108	102	0.01%	0.001%
22	4.070	848	849	853	rBV2	132	81	0.01%	0.001%
23	4.224	893	897	899	rBV2	275	252	0.02%	0.003%
24	4.671	1007	1036	1064	rBV2	404624	1244824	100.00%	12.670%
25	4.883	1098	1102	1104	rBV2	398	273	0.02%	0.003%
26	5.002	1136	1139	1140	rBV	168	83	0.01%	0.001%
27	5.070	1143	1160	1183	rVV	204904	462463	37.15%	4.707%
28	5.215	1203	1205	1207	rVB	306	108	0.01%	0.001%
29	5.231	1207	1210	1216	rVB2	217	154	0.01%	0.002%
30	5.253	1216	1217	1221	rVB2	185	122	0.01%	0.001%
31	5.276	1221	1224	1225	rBV	116	67	0.01%	0.001%
32	5.729	1344	1365	1388	rBV2	433232	1175573	94.44%	11.966%
33	6.018	1452	1455	1459	rBV2	202	160	0.01%	0.002%
34	6.041	1460	1462	1468	rVB2	311	192	0.02%	0.002%
35	6.121	1481	1487	1488	rBV	341	309	0.02%	0.003%
36	6.166	1498	1501	1504	rBV2	202	131	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044812.D
 Acq On : 24 Sep 2021 15:10
 Operator : SY/MD
 Sample : M3873-16DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.253	1512	1528	1545	rBV	328868	614843	49.39%	6.258%
38	6.546	1604	1619	1633	rBV2	63729	121051	9.72%	1.232%
39	6.697	1650	1666	1689	rBV	283889	549792	44.17%	5.596%
40	6.854	1712	1715	1718	rVB	376	247	0.02%	0.003%
41	7.044	1768	1774	1783	rVV3	451	733	0.06%	0.007%
42	7.076	1783	1784	1790	rVB	181	101	0.01%	0.001%
43	7.124	1796	1799	1801	rBV	88	65	0.01%	0.001%
44	7.186	1811	1818	1827	rBV2	1642	2593	0.21%	0.026%
45	7.256	1837	1840	1848	rBV2	198	194	0.02%	0.002%
46	7.382	1875	1879	1881	rBV2	99	83	0.01%	0.001%
47	7.475	1905	1908	1913	rVB2	210	165	0.01%	0.002%
48	7.507	1915	1918	1920	rBV	137	84	0.01%	0.001%
49	7.571	1925	1938	1956	rBV	146059	253896	20.40%	2.584%
50	7.684	1968	1973	1975	rBV2	996	902	0.07%	0.009%
51	7.742	1988	1991	1993	rBV2	176	78	0.01%	0.001%
52	7.796	2006	2008	2010	rBV	155	74	0.01%	0.001%
53	7.903	2026	2041	2056	rBV	501453	851976	68.44%	8.672%
54	7.973	2059	2063	2072	rVB	7397	10046	0.81%	0.102%
55	8.182	2117	2128	2149	rBV	102558	171673	13.79%	1.747%
56	8.285	2158	2160	2161	rBV2	243	86	0.01%	0.001%
57	8.314	2167	2169	2171	rBV2	204	98	0.01%	0.001%
58	8.337	2174	2176	2178	rBV	159	68	0.01%	0.001%
59	8.404	2193	2197	2199	rBV2	178	151	0.01%	0.002%
60	8.568	2245	2248	2252	rVB	108	75	0.01%	0.001%
61	8.594	2252	2256	2257	rBV2	138	94	0.01%	0.001%
62	8.639	2257	2270	2302	rBV	456492	799322	64.21%	8.136%
63	8.848	2333	2335	2338	rVB2	195	104	0.01%	0.001%
64	8.925	2357	2359	2362	rBV2	126	84	0.01%	0.001%
65	9.044	2392	2396	2403	rVB2	293	340	0.03%	0.003%
66	9.073	2403	2405	2407	rBV	154	93	0.01%	0.001%
67	9.099	2411	2413	2416	rBV	146	118	0.01%	0.001%
68	9.234	2448	2455	2456	rBV	186	228	0.02%	0.002%
69	9.420	2500	2513	2548	rBV	459775	762469	61.25%	7.761%
70	9.578	2557	2562	2565	rVB2	386	361	0.03%	0.004%
71	9.645	2580	2583	2586	rBV	211	183	0.01%	0.002%
72	9.703	2595	2601	2607	rVB3	644	882	0.07%	0.009%
73	9.803	2627	2632	2635	rBV2	284	330	0.03%	0.003%
74	9.941	2672	2675	2684	rVB2	165	197	0.02%	0.002%
75	10.102	2723	2725	2729	rVB	263	176	0.01%	0.002%
76	10.349	2799	2802	2804	rBV	113	80	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044812.D
 Acq On : 24 Sep 2021 15:10
 Operator : SY/MD
 Sample : M3873-16DL 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.443	2828	2831	2833	rBV	183	115	0.01%	0.001%
78	10.674	2895	2903	2910	rBV3	1773	2316	0.19%	0.024%
79	10.761	2916	2930	2949	rBV	384447	621013	49.89%	6.321%
80	10.867	2961	2963	2970	rVB4	277	277	0.02%	0.003%
81	10.992	2998	3002	3004	rBV2	215	194	0.02%	0.002%
82	11.214	3068	3071	3072	rBV2	177	92	0.01%	0.001%
83	11.269	3086	3088	3095	rVB	239	185	0.01%	0.002%
84	11.410	3129	3132	3134	rBV2	198	161	0.01%	0.002%
85	11.462	3140	3148	3160	rVB4	1376	2238	0.18%	0.023%
86	11.552	3174	3176	3178	rBV	190	105	0.01%	0.001%
87	11.700	3217	3222	3230	rBV4	810	971	0.08%	0.010%
88	11.816	3246	3258	3277	rBV	414996	657820	52.84%	6.696%
89	11.902	3282	3285	3287	rBV3	322	245	0.02%	0.002%
90	11.935	3291	3295	3297	rBV2	399	349	0.03%	0.004%
91	12.195	3363	3376	3396	rBV	456307	742507	59.65%	7.558%
92	12.330	3415	3418	3419	rBV2	218	138	0.01%	0.001%
93	12.484	3463	3466	3468	rBV	203	138	0.01%	0.001%
94	12.590	3496	3499	3505	rBV2	278	300	0.02%	0.003%
95	12.639	3511	3514	3517	rBV	183	154	0.01%	0.002%
96	12.851	3578	3580	3584	rBV	184	78	0.01%	0.001%
97	13.224	3693	3696	3697	rBV2	175	112	0.01%	0.001%
98	13.266	3707	3709	3712	rBV2	176	157	0.01%	0.002%
99	13.825	3880	3883	3886	rBV	265	174	0.01%	0.002%
100	14.098	3963	3968	3974	rVB3	565	840	0.07%	0.009%


Sum of corrected areas: 9824615

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044812.D
Acq On : 24 Sep 2021 15:10
Operator : SY/MD
Sample : M3873-16DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

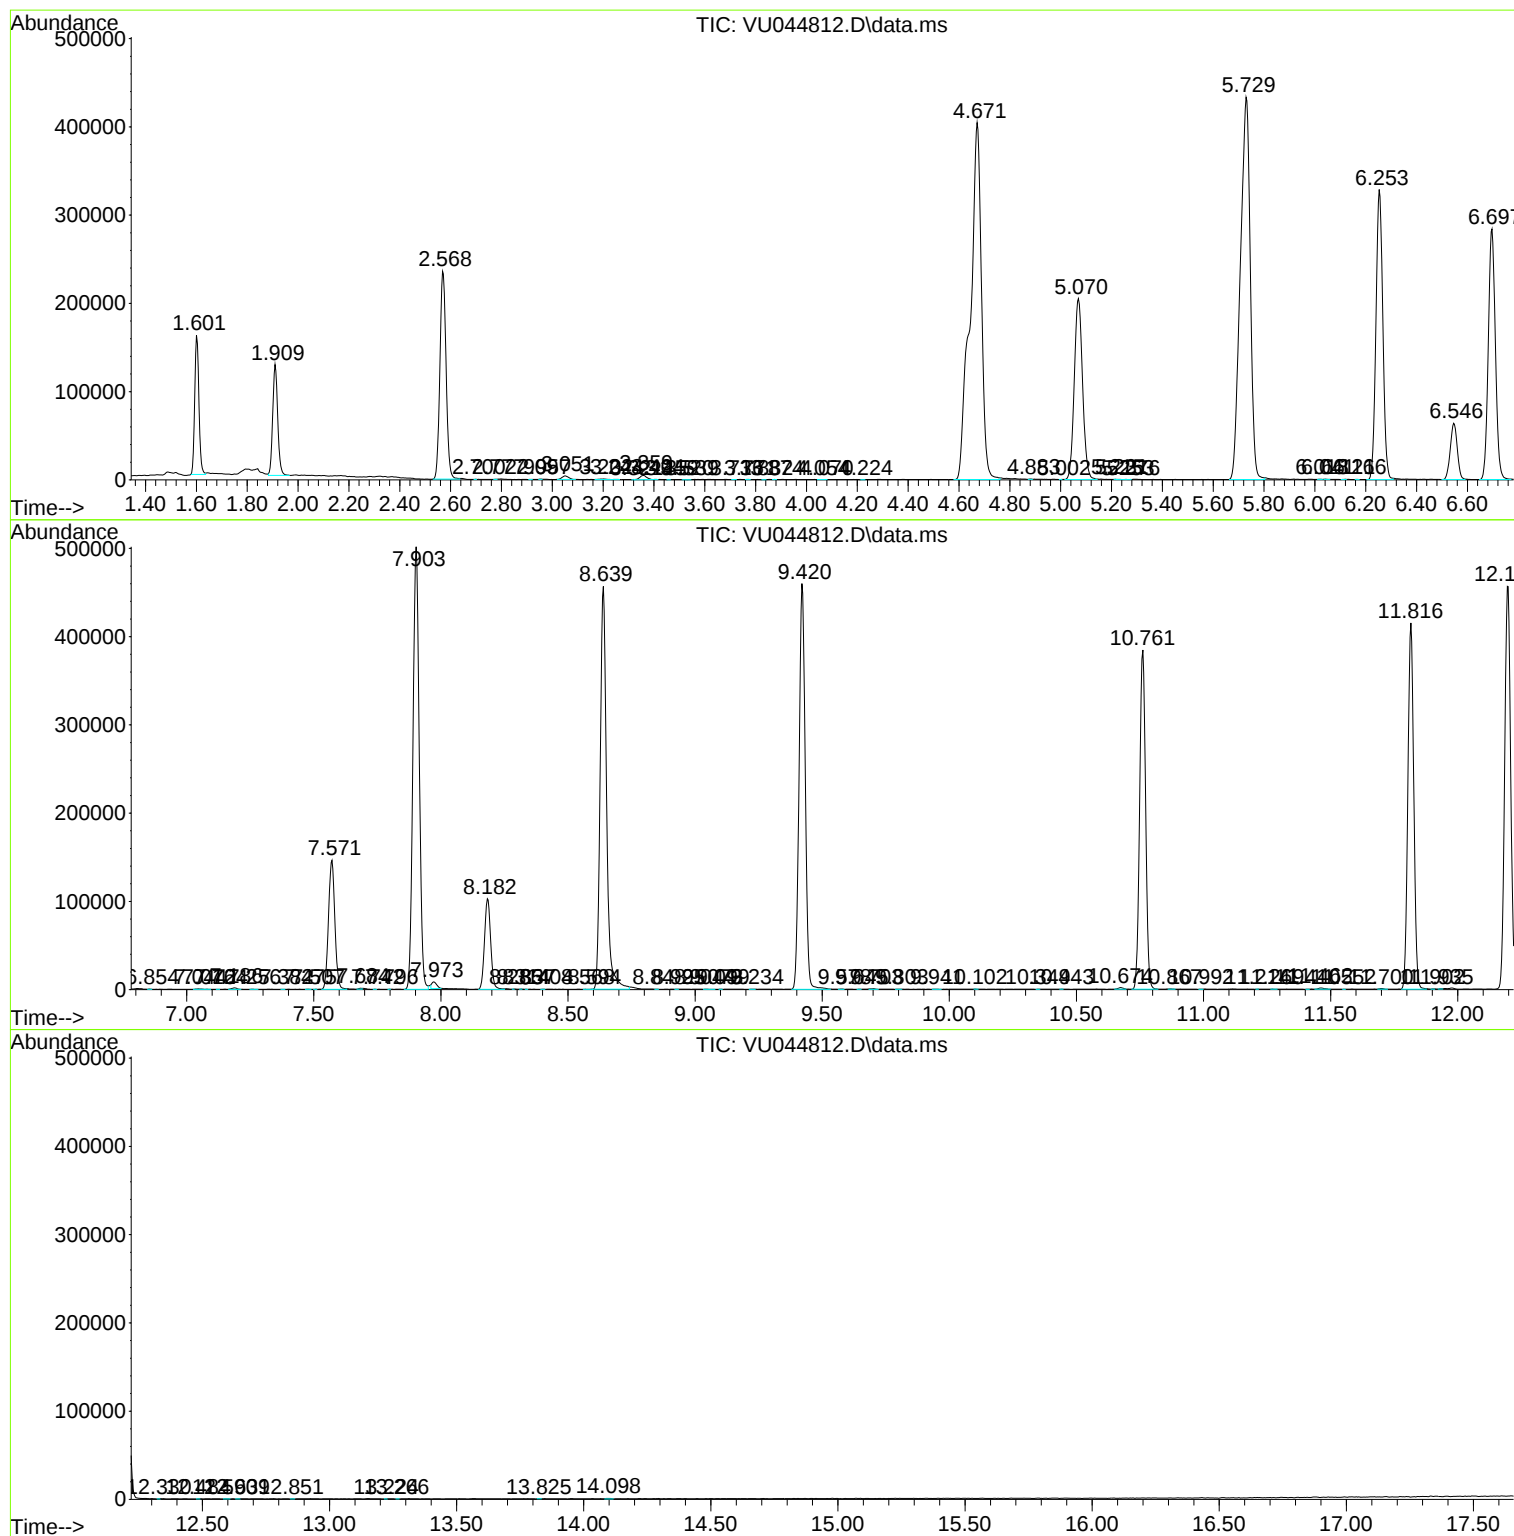

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044812.D
Acq On : 24 Sep 2021 15:10
Operator : SY/MD
Sample : M3873-16DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044812.D
Acq On : 24 Sep 2021 15:10
Operator : SY/MD
Sample : M3873-16DL 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
