

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044813.D
 Acq On : 24 Sep 2021 15:47
 Operator : SY/MD
 Sample : M3873-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rBV2	373157	449009	1.09%	0.801%
2	1.912	170	178	193	rVB	129777	175826	0.43%	0.314%
3	2.571	371	383	399	rBV2	257700	468083	1.14%	0.835%
4	2.716	426	428	429	rBV2	285	134	0.00%	0.000%
5	2.793	438	452	461	rBV4	3404	9143	0.02%	0.016%
6	3.051	526	532	541	rVB4	856	1529	0.00%	0.003%
7	3.096	541	546	550	rBV2	243	292	0.00%	0.001%
8	3.134	554	558	560	rBV	269	261	0.00%	0.000%
9	3.186	570	574	577	rBV	390	366	0.00%	0.001%
10	3.359	614	628	651	rBV	229890	448632	1.09%	0.800%
11	3.459	657	659	664	rVB2	408	206	0.00%	0.000%
12	3.552	685	688	692	rBV2	207	147	0.00%	0.000%
13	3.588	692	699	709	rVB3	1007	1995	0.00%	0.004%
14	3.790	759	762	765	rBV2	174	157	0.00%	0.000%
15	3.877	777	789	803	rVB3	4483	9867	0.02%	0.018%
16	4.205	884	891	895	rBV2	245	340	0.00%	0.001%
17	4.292	913	918	923	rVB2	169	166	0.00%	0.000%
18	4.317	923	926	929	rBV2	163	169	0.00%	0.000%
19	4.510	982	986	992	rVB	231	260	0.00%	0.000%
20	4.562	997	1002	1005	rBV2	299	338	0.00%	0.001%
21	4.674	1010	1037	1080	rBV	18486760	41065869	100.00%	73.266%
22	5.070	1149	1160	1187	rVB	213049	475740	1.16%	0.849%
23	5.523	1298	1301	1302	rBV	242	161	0.00%	0.000%
24	5.597	1320	1324	1328	rBV2	205	171	0.00%	0.000%
25	5.620	1328	1331	1334	rBV2	195	165	0.00%	0.000%
26	5.645	1334	1339	1343	rBV2	223	195	0.00%	0.000%
27	5.732	1343	1366	1392	rBV2	437124	1193878	2.91%	2.130%
28	5.867	1405	1408	1410	rBV2	297	218	0.00%	0.000%
29	5.941	1427	1431	1435	rBV3	333	412	0.00%	0.001%
30	6.025	1453	1457	1459	rBV	278	231	0.00%	0.000%
31	6.108	1480	1483	1485	rBV3	244	172	0.00%	0.000%
32	6.144	1491	1494	1495	rBV2	435	267	0.00%	0.000%
33	6.160	1495	1499	1503	rVV5	559	703	0.00%	0.001%
34	6.253	1514	1528	1551	rBV	345204	652990	1.59%	1.165%
35	6.427	1578	1582	1584	rBV	266	174	0.00%	0.000%
36	6.549	1603	1620	1652	rBV	2879997	5346713	13.02%	9.539%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044813.D
 Acq On : 24 Sep 2021 15:47
 Operator : SY/MD
 Sample : M3873-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.697	1654	1666	1693	rVB	288470	574332	1.40%	1.025%
38	7.054	1769	1777	1786	rBV4	743	1458	0.00%	0.003%
39	7.182	1807	1817	1818	rBV3	1649	1507	0.00%	0.003%
40	7.275	1842	1846	1851	rBV2	199	249	0.00%	0.000%
41	7.356	1868	1871	1873	rBV2	216	176	0.00%	0.000%
42	7.452	1896	1901	1904	rBV2	314	310	0.00%	0.001%
43	7.504	1913	1917	1921	rBV2	215	212	0.00%	0.000%
44	7.571	1924	1938	1956	rBV	158414	270719	0.66%	0.483%
45	7.722	1967	1985	1994	rVB8	3771	8544	0.02%	0.015%
46	7.793	2004	2007	2010	rBV	264	158	0.00%	0.000%
47	7.819	2010	2015	2019	rVB2	245	231	0.00%	0.000%
48	7.851	2022	2025	2027	rVB2	220	157	0.00%	0.000%
49	7.902	2027	2041	2057	rBV	514871	889952	2.17%	1.588%
50	7.973	2057	2063	2075	rVB3	7855	13458	0.03%	0.024%
51	8.137	2110	2114	2116	rBV2	226	163	0.00%	0.000%
52	8.185	2116	2129	2144	rBV	108903	180091	0.44%	0.321%
53	8.314	2167	2169	2171	rVV2	374	176	0.00%	0.000%
54	8.340	2175	2177	2182	rVB3	261	177	0.00%	0.000%
55	8.372	2184	2187	2191	rVB3	238	204	0.00%	0.000%
56	8.446	2207	2210	2211	rBV2	256	162	0.00%	0.000%
57	8.478	2211	2220	2225	rBV3	1167	1898	0.00%	0.003%
58	8.587	2250	2254	2256	rBV3	261	206	0.00%	0.000%
59	8.639	2257	2270	2314	rVV	437943	788553	1.92%	1.407%
60	8.870	2338	2342	2346	rBV4	641	688	0.00%	0.001%
61	9.099	2409	2413	2415	rBV	213	156	0.00%	0.000%
62	9.195	2440	2443	2449	rBV3	266	290	0.00%	0.001%
63	9.311	2476	2479	2482	rBV	186	129	0.00%	0.000%
64	9.327	2482	2484	2488	rVB2	225	141	0.00%	0.000%
65	9.423	2501	2514	2547	rBV	483503	813523	1.98%	1.451%
66	9.568	2555	2559	2560	rBV	210	165	0.00%	0.000%
67	9.581	2560	2563	2567	rVB	514	379	0.00%	0.001%
68	9.690	2589	2597	2606	rVB5	1125	1577	0.00%	0.003%
69	9.809	2631	2634	2638	rVV2	184	150	0.00%	0.000%
70	9.848	2642	2646	2654	rVB2	297	248	0.00%	0.000%
71	9.960	2678	2681	2683	rBV	200	175	0.00%	0.000%
72	10.102	2721	2725	2726	rBV2	375	201	0.00%	0.000%
73	10.195	2751	2754	2757	rBV	196	150	0.00%	0.000%
74	10.349	2798	2802	2809	rVB2	225	193	0.00%	0.000%
75	10.378	2809	2811	2817	rBV2	188	145	0.00%	0.000%
76	10.481	2840	2843	2847	rBV3	340	287	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044813.D
 Acq On : 24 Sep 2021 15:47
 Operator : SY/MD
 Sample : M3873-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.677	2893	2904	2912	rBV4	2466	3312	0.01%	0.006%
78	10.761	2917	2930	2954	rVB	405960	642412	1.56%	1.146%
79	10.870	2960	2964	2968	rBV4	431	437	0.00%	0.001%
80	10.896	2970	2972	2976	rVV	633	544	0.00%	0.001%
81	11.127	3041	3044	3050	rVB2	243	256	0.00%	0.000%
82	11.182	3058	3061	3063	rBV	197	135	0.00%	0.000%
83	11.320	3101	3104	3113	rBV	246	389	0.00%	0.001%
84	11.465	3141	3149	3155	rBV7	1414	2277	0.01%	0.004%
85	11.629	3195	3200	3206	rVB3	441	403	0.00%	0.001%
86	11.700	3218	3222	3227	rVB4	836	825	0.00%	0.001%
87	11.815	3246	3258	3277	rBV	469858	739470	1.80%	1.319%
88	11.947	3295	3299	3301	rBV4	516	514	0.00%	0.001%
89	11.973	3304	3307	3321	rVB5	1285	1974	0.00%	0.004%
90	12.198	3364	3377	3397	rVV	499236	798619	1.94%	1.425%
91	12.333	3415	3419	3422	rBV	536	433	0.00%	0.001%
92	12.378	3430	3433	3436	rBV2	163	136	0.00%	0.000%
93	12.455	3454	3457	3459	rBV2	214	174	0.00%	0.000%
94	12.520	3475	3477	3482	rVB2	287	209	0.00%	0.000%
95	12.603	3501	3503	3508	rVB	205	154	0.00%	0.000%
96	12.639	3510	3514	3515	rBV	370	242	0.00%	0.000%
97	12.780	3551	3558	3562	rBV2	296	410	0.00%	0.001%
98	13.780	3866	3869	3876	rBV	295	245	0.00%	0.000%
99	14.594	4120	4122	4126	rBV2	252	153	0.00%	0.000%
100	14.979	4240	4242	4249	rVB	402	281	0.00%	0.001%




Sum of corrected areas: 56050673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044813.D
Acq On : 24 Sep 2021 15:47
Operator : SY/MD
Sample : M3873-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

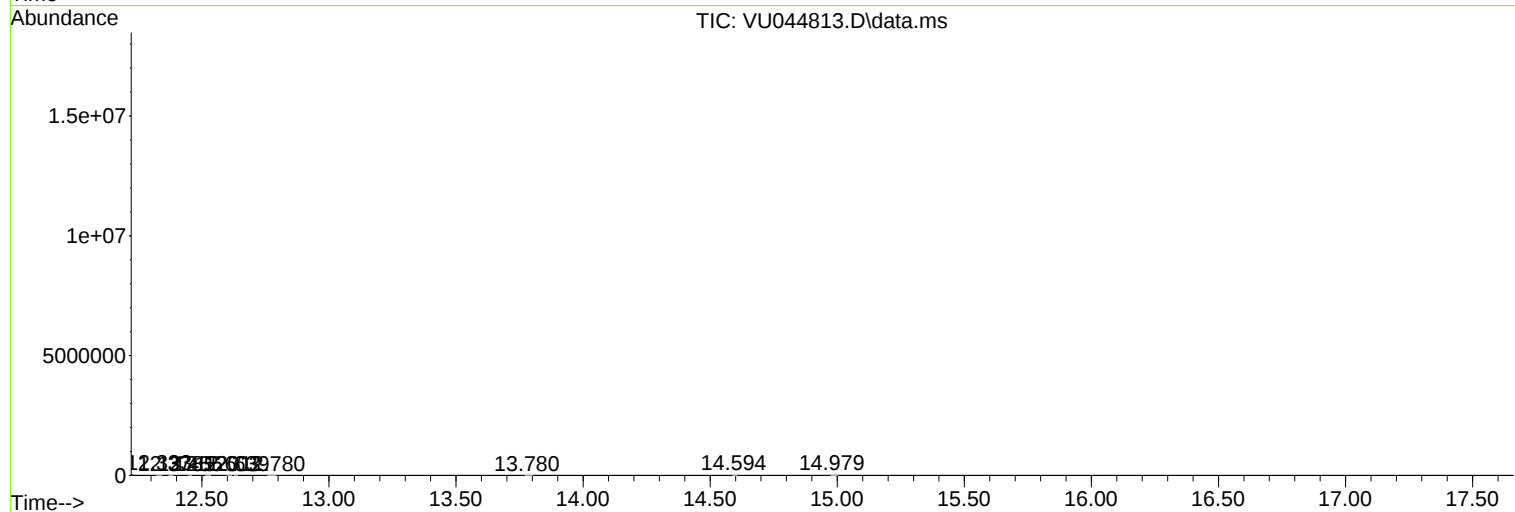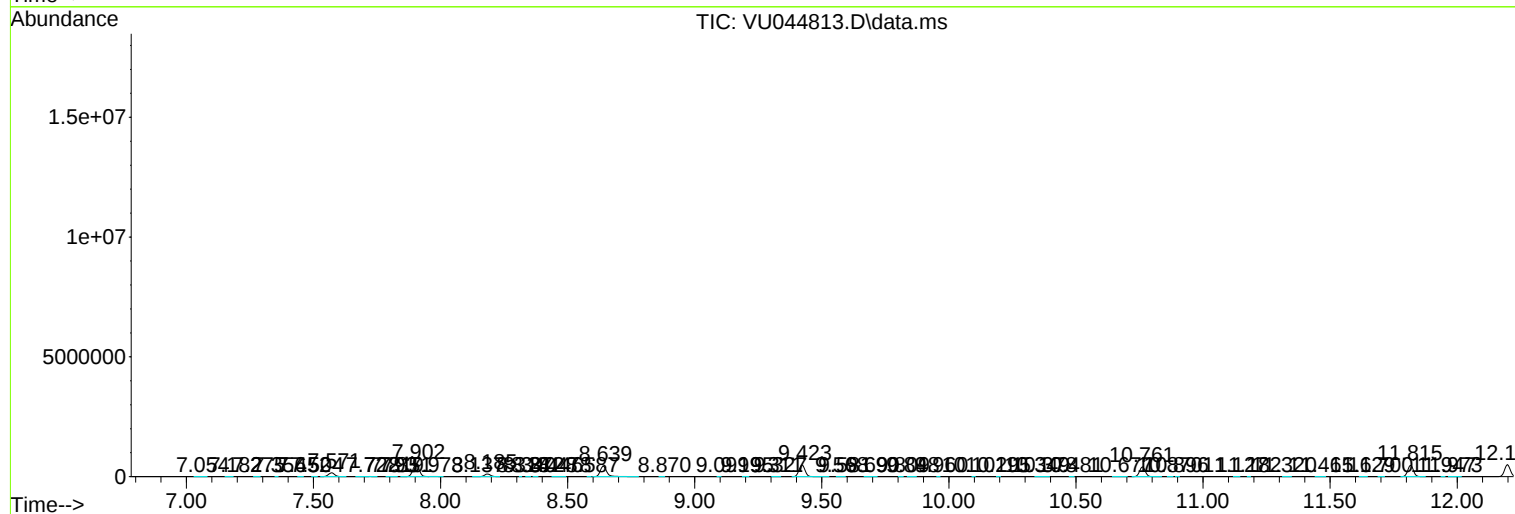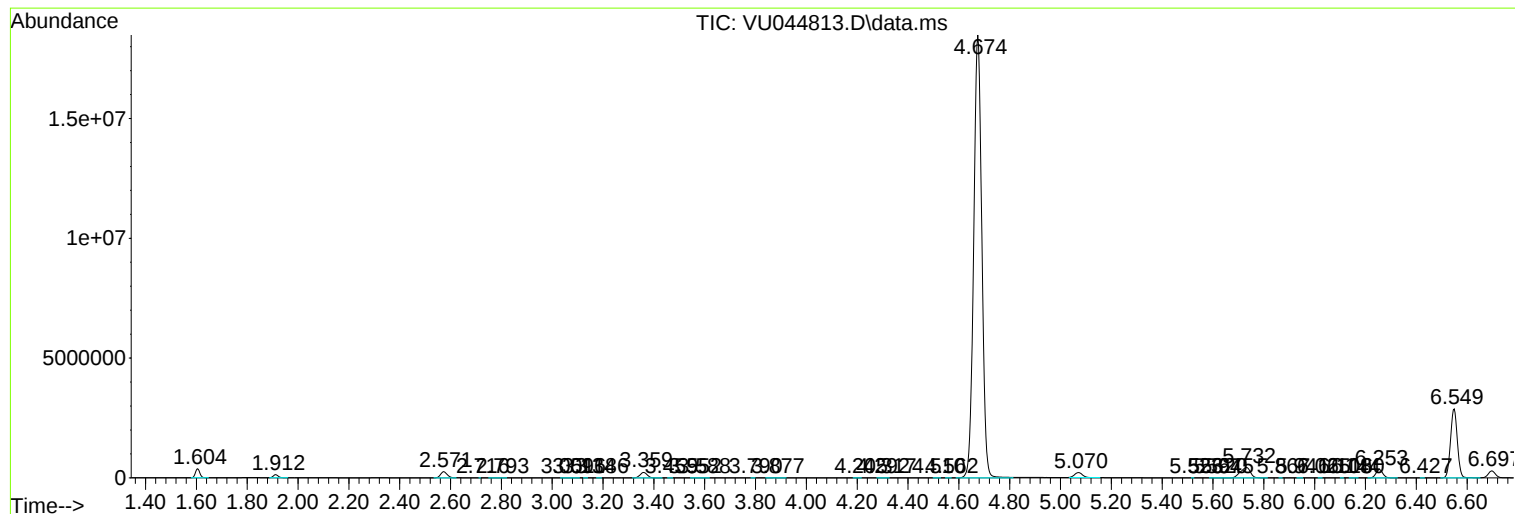

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044813.D
Acq On : 24 Sep 2021 15:47
Operator : SY/MD
Sample : M3873-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044813.D
Acq On : 24 Sep 2021 15:47
Operator : SY/MD
Sample : M3873-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------