

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044815.D
 Acq On : 24 Sep 2021 16:57
 Operator : SY/MD
 Sample : M3873-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	152011	173477	5.94%	1.394%
2	1.909	170	177	195	rVB	132960	180653	6.19%	1.452%
3	2.572	369	383	400	rBV	234009	395878	13.56%	3.181%
4	2.803	440	455	460	rBV	8650	21420	0.73%	0.172%
5	3.044	525	530	531	rBV2	632	530	0.02%	0.004%
6	3.192	565	576	585	rBV3	2276	4934	0.17%	0.040%
7	3.298	606	609	615	rBV2	186	262	0.01%	0.002%
8	3.359	615	628	644	rVB2	46531	91018	3.12%	0.731%
9	3.436	649	652	657	rVV2	183	150	0.01%	0.001%
10	3.475	660	664	668	rVB2	168	145	0.00%	0.001%
11	3.501	668	672	675	rBV	139	127	0.00%	0.001%
12	3.572	690	694	698	rBV2	113	109	0.00%	0.001%
13	3.713	732	738	741	rBV2	151	150	0.01%	0.001%
14	3.726	741	742	747	rBV2	116	93	0.00%	0.001%
15	3.752	748	750	754	rVB2	169	139	0.00%	0.001%
16	3.797	761	764	768	rBV2	154	121	0.00%	0.001%
17	3.896	792	795	797	rBV2	148	90	0.00%	0.001%
18	3.973	816	819	821	rBV	191	164	0.01%	0.001%
19	4.025	832	835	838	rBV	175	180	0.01%	0.001%
20	4.083	849	853	857	rBV2	228	215	0.01%	0.002%
21	4.115	857	863	866	rBV2	227	222	0.01%	0.002%
22	4.134	867	869	872	rVV	223	176	0.01%	0.001%
23	4.179	880	883	888	rBV2	214	206	0.01%	0.002%
24	4.221	892	896	903	rVV2	216	285	0.01%	0.002%
25	4.272	908	912	917	rVV2	163	215	0.01%	0.002%
26	4.334	929	931	940	rVV2	91	107	0.00%	0.001%
27	4.430	959	961	964	rVB	220	106	0.00%	0.001%
28	4.462	964	971	972	rBV	245	315	0.01%	0.003%
29	4.671	1008	1036	1083	rBV2	1163912	2918737	100.00%	23.453%
30	5.070	1142	1160	1182	rBV	210469	465765	15.96%	3.743%
31	5.208	1200	1203	1204	rBV2	272	161	0.01%	0.001%
32	5.221	1204	1207	1212	rVV6	549	445	0.02%	0.004%
33	5.256	1215	1218	1221	rVB2	215	132	0.00%	0.001%
34	5.292	1226	1229	1230	rBV2	311	179	0.01%	0.001%
35	5.356	1247	1249	1252	rVB2	124	88	0.00%	0.001%
36	5.411	1261	1266	1269	rBV	103	103	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044815.D
 Acq On : 24 Sep 2021 16:57
 Operator : SY/MD
 Sample : M3873-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.497	1291	1293	1297	rVB	134	109	0.00%	0.001%
38	5.571	1313	1316	1319	rBV2	180	148	0.01%	0.001%
39	5.597	1319	1324	1326	rBV2	192	174	0.01%	0.001%
40	5.732	1343	1366	1389	rBV2	433226	1186042	40.64%	9.530%
41	5.983	1441	1444	1446	rBV2	210	123	0.00%	0.001%
42	6.124	1484	1488	1493	rBV3	343	368	0.01%	0.003%
43	6.166	1495	1501	1503	rVB2	247	251	0.01%	0.002%
44	6.253	1513	1528	1553	rBV	332955	630710	21.61%	5.068%
45	6.366	1559	1563	1568	rBV2	447	402	0.01%	0.003%
46	6.417	1576	1579	1584	rBV3	221	246	0.01%	0.002%
47	6.472	1592	1596	1602	rBV3	233	292	0.01%	0.002%
48	6.546	1605	1619	1639	rBV	460727	868343	29.75%	6.977%
49	6.697	1651	1666	1695	rVB	283228	552769	18.94%	4.442%
50	6.809	1695	1701	1706	rBV4	773	907	0.03%	0.007%
51	6.864	1713	1718	1722	rVB2	202	210	0.01%	0.002%
52	6.970	1745	1751	1756	rVB2	178	228	0.01%	0.002%
53	6.999	1756	1760	1763	rBV2	220	234	0.01%	0.002%
54	7.047	1771	1775	1777	rBV2	475	416	0.01%	0.003%
55	7.128	1797	1800	1803	rBV3	262	179	0.01%	0.001%
56	7.189	1810	1819	1829	rVB4	1571	2504	0.09%	0.020%
57	7.269	1841	1844	1846	rBV	166	119	0.00%	0.001%
58	7.423	1890	1892	1894	rBV2	129	91	0.00%	0.001%
59	7.465	1902	1905	1908	rVB2	211	136	0.00%	0.001%
60	7.494	1912	1914	1917	rBV2	163	132	0.00%	0.001%
61	7.571	1925	1938	1960	rBV	146836	258807	8.87%	2.080%
62	7.677	1968	1971	1972	rBV2	400	238	0.01%	0.002%
63	7.732	1984	1988	1994	rVB3	394	403	0.01%	0.003%
64	7.761	1994	1997	1999	rBV2	188	104	0.00%	0.001%
65	7.800	2005	2009	2014	rBV2	140	145	0.00%	0.001%
66	7.903	2027	2041	2056	rBV	506811	863405	29.58%	6.938%
67	8.185	2116	2129	2155	rBV	101255	173789	5.95%	1.396%
68	8.388	2189	2192	2199	rBV3	225	206	0.01%	0.002%
69	8.478	2212	2220	2230	rVB2	874	1585	0.05%	0.013%
70	8.642	2258	2271	2307	rBV	433800	775078	26.56%	6.228%
71	9.076	2400	2406	2409	rBV2	196	228	0.01%	0.002%
72	9.369	2494	2497	2499	rBV	130	95	0.00%	0.001%
73	9.420	2500	2513	2538	rBV	477884	778353	26.67%	6.254%
74	9.610	2569	2572	2574	rBV2	186	100	0.00%	0.001%
75	9.693	2593	2598	2607	rVB3	765	1221	0.04%	0.010%
76	9.742	2607	2613	2616	rBV2	110	132	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044815.D
 Acq On : 24 Sep 2021 16:57
 Operator : SY/MD
 Sample : M3873-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7Y0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	9.806	2630	2633	2637	rBV2	158	147	0.01%	0.001%
78	9.902	2658	2663	2664	rBV2	285	279	0.01%	0.002%
79	10.105	2722	2726	2727	rBV	311	216	0.01%	0.002%
80	10.173	2744	2747	2751	rVB	239	160	0.01%	0.001%
81	10.401	2815	2818	2821	rBV2	145	110	0.00%	0.001%
82	10.501	2846	2849	2854	rBV2	167	201	0.01%	0.002%
83	10.584	2871	2875	2876	rBV	214	142	0.00%	0.001%
84	10.674	2896	2903	2913	rVB2	1726	2373	0.08%	0.019%
85	10.761	2917	2930	2954	rVV	395126	630703	21.61%	5.068%
86	10.890	2967	2970	2976	rBV3	388	328	0.01%	0.003%
87	11.021	3007	3011	3017	rVB2	177	192	0.01%	0.002%
88	11.102	3032	3036	3040	rBV3	235	185	0.01%	0.001%
89	11.462	3141	3148	3152	rBV3	1820	2240	0.08%	0.018%
90	11.568	3178	3181	3182	rBV	165	90	0.00%	0.001%
91	11.700	3217	3222	3228	rVB3	776	833	0.03%	0.007%
92	11.816	3246	3258	3277	rBV	439764	690081	23.64%	5.545%
93	11.976	3304	3308	3315	rVB3	1353	1632	0.06%	0.013%
94	12.198	3363	3377	3397	rBV	467859	757170	25.94%	6.084%
95	12.333	3415	3419	3429	rVB5	646	718	0.02%	0.006%
96	12.594	3496	3500	3504	rVB2	334	277	0.01%	0.002%
97	12.732	3539	3543	3546	rBV2	188	218	0.01%	0.002%
98	14.748	4167	4170	4172	rBV	300	169	0.01%	0.001%
99	15.147	4292	4294	4301	rBV2	318	279	0.01%	0.002%
100	15.233	4318	4321	4322	rBV2	353	218	0.01%	0.002%




Sum of corrected areas: 12445080

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044815.D
Acq On : 24 Sep 2021 16:57
Operator : SY/MD
Sample : M3873-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

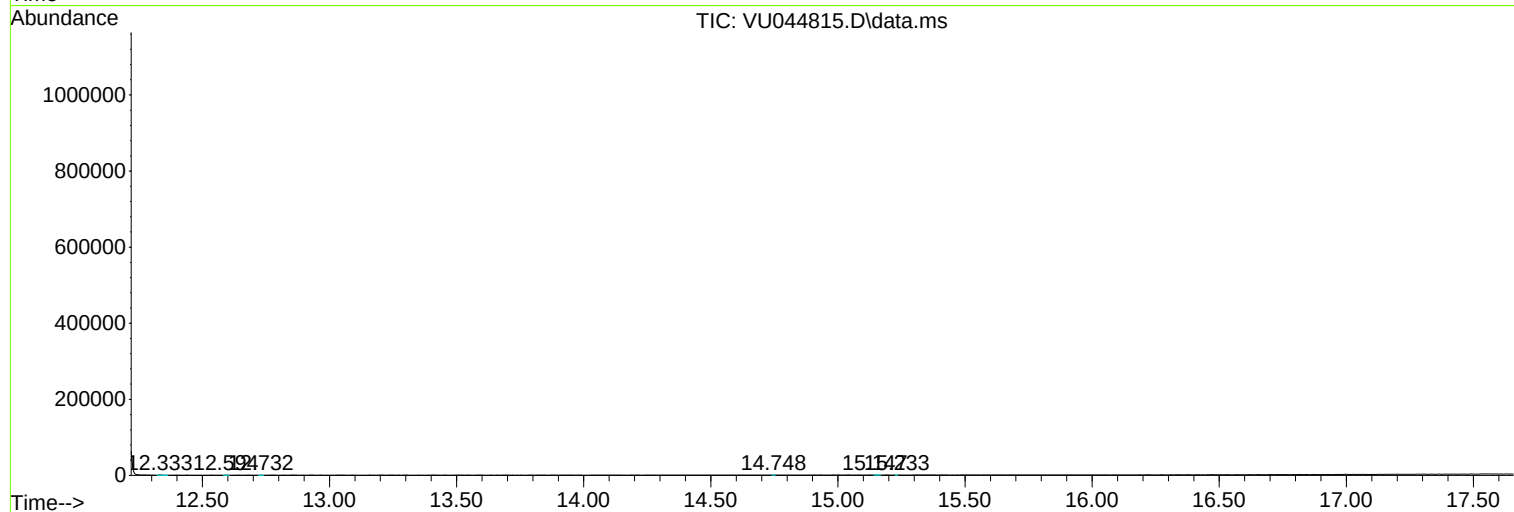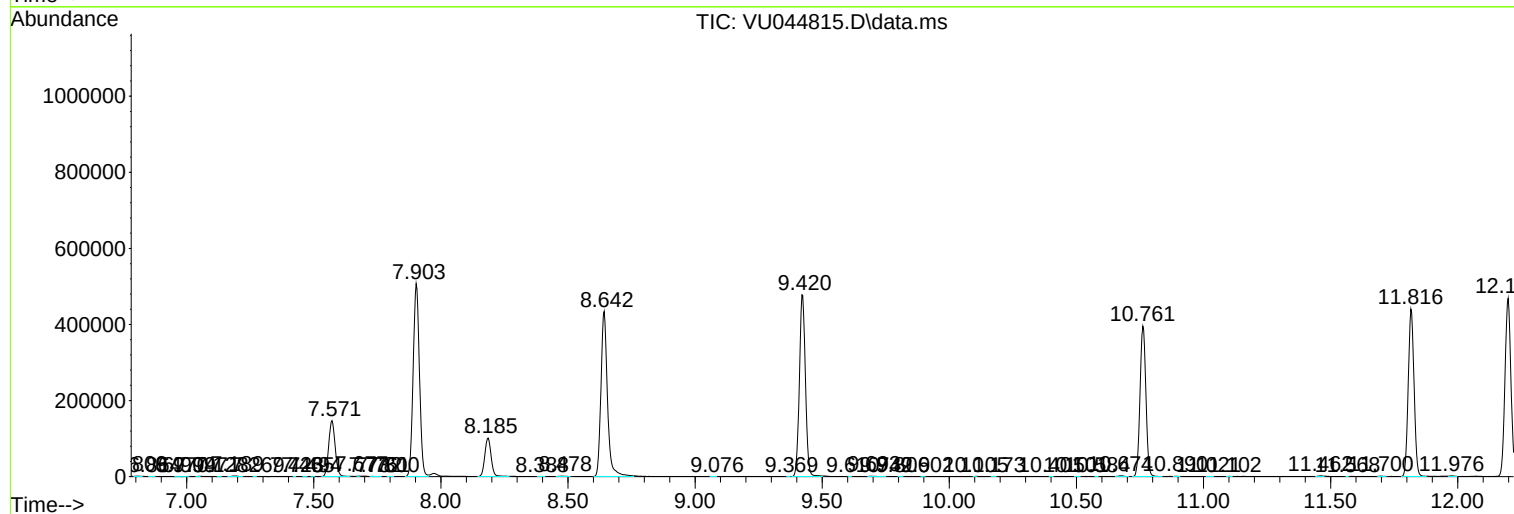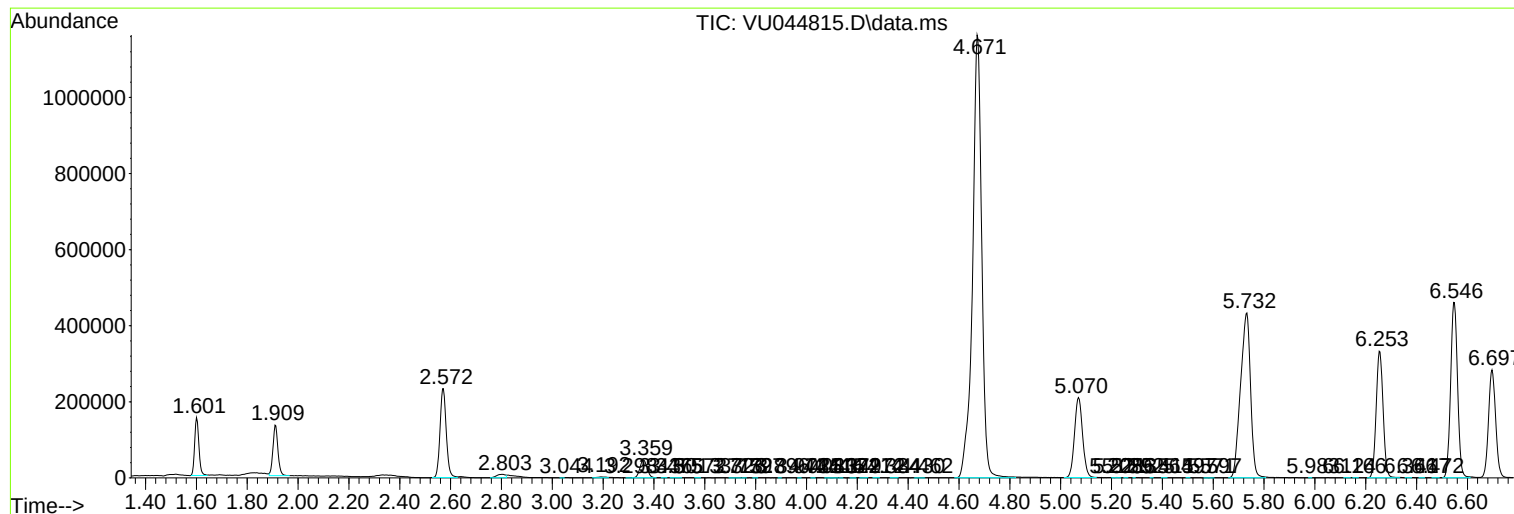

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044815.D
Acq On : 24 Sep 2021 16:57
Operator : SY/MD
Sample : M3873-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044815.D
Acq On : 24 Sep 2021 16:57
Operator : SY/MD
Sample : M3873-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
