

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044816.D
 Acq On : 24 Sep 2021 17:20
 Operator : SY/MD
 Sample : VIBLK002
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU044816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rBV	135105	152277	14.06%	1.837%
2	1.909	169	177	196	rVB	110941	151660	14.01%	1.829%
3	2.501	358	361	366	rVB2	250	192	0.02%	0.002%
4	2.568	370	382	403	rBV	207903	347108	32.06%	4.187%
5	2.784	441	449	452	rBV2	413	506	0.05%	0.006%
6	2.957	497	503	513	rBV3	288	554	0.05%	0.007%
7	3.051	523	532	543	rVB3	2877	4954	0.46%	0.060%
8	3.195	565	577	596	rBV	3050	7323	0.68%	0.088%
9	3.363	628	629	633	rVB	263	143	0.01%	0.002%
10	3.385	633	636	639	rBV	162	155	0.01%	0.002%
11	3.430	648	650	653	rBV2	136	117	0.01%	0.001%
12	3.584	695	698	702	rVB	213	115	0.01%	0.001%
13	3.610	702	706	709	rBV2	258	247	0.02%	0.003%
14	3.658	716	721	723	rBV2	210	196	0.02%	0.002%
15	3.838	772	777	779	rBV	181	136	0.01%	0.002%
16	3.912	797	800	803	rVB2	195	149	0.01%	0.002%
17	3.932	803	806	808	rBV	229	111	0.01%	0.001%
18	3.964	813	816	823	rVB2	192	212	0.02%	0.003%
19	4.009	826	830	834	rBV	218	225	0.02%	0.003%
20	4.076	847	851	856	rVB2	219	176	0.02%	0.002%
21	4.134	866	869	873	rBV2	178	199	0.02%	0.002%
22	4.189	884	886	892	rBV2	137	169	0.02%	0.002%
23	4.260	905	908	910	rBV	188	155	0.01%	0.002%
24	4.285	914	916	920	rBV	168	140	0.01%	0.002%
25	4.375	936	944	947	rBV2	222	347	0.03%	0.004%
26	4.398	947	951	954	rBV2	223	211	0.02%	0.003%
27	4.510	981	986	988	rBV	194	199	0.02%	0.002%
28	4.629	1007	1023	1053	rBV	151183	377516	34.87%	4.554%
29	5.070	1143	1160	1188	rBV	192938	429514	39.67%	5.181%
30	5.218	1202	1206	1208	rBV2	246	182	0.02%	0.002%
31	5.244	1211	1214	1216	rBV2	292	161	0.01%	0.002%
32	5.295	1222	1230	1233	rBV4	448	492	0.05%	0.006%
33	5.327	1233	1240	1243	rVV2	124	185	0.02%	0.002%
34	5.353	1243	1248	1253	rVB	260	298	0.03%	0.004%
35	5.388	1253	1259	1260	rBV	159	173	0.02%	0.002%
36	5.449	1274	1278	1282	rBV2	227	275	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044816.D
 Acq On : 24 Sep 2021 17:20
 Operator : SY/MD
 Sample : VIBLK002
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.507	1292	1296	1298	rBV	196	137	0.01%	0.002%
38	5.639	1331	1337	1343	rVB	207	368	0.03%	0.004%
39	5.729	1343	1365	1387	rBV2	392642	1082735	100.00%	13.060%
40	5.941	1429	1431	1435	rVB2	350	190	0.02%	0.002%
41	5.999	1446	1449	1455	rVB3	246	262	0.02%	0.003%
42	6.038	1455	1461	1462	rBV2	322	275	0.03%	0.003%
43	6.147	1493	1495	1499	rVB3	220	127	0.01%	0.002%
44	6.182	1504	1506	1511	rVB2	245	204	0.02%	0.002%
45	6.253	1512	1528	1549	rBV	309950	578150	53.40%	6.974%
46	6.414	1576	1578	1581	rBV2	173	132	0.01%	0.002%
47	6.539	1606	1617	1626	rVB6	3877	7714	0.71%	0.093%
48	6.584	1628	1631	1634	rVB2	208	117	0.01%	0.001%
49	6.697	1651	1666	1686	rBV	264627	511140	47.21%	6.165%
50	6.816	1697	1703	1709	rVB4	747	1107	0.10%	0.013%
51	6.842	1709	1711	1718	rBV2	272	192	0.02%	0.002%
52	6.893	1723	1727	1729	rBV	238	129	0.01%	0.002%
53	7.038	1769	1772	1773	rBV	344	228	0.02%	0.003%
54	7.051	1773	1776	1789	rVB3	657	936	0.09%	0.011%
55	7.102	1789	1792	1795	rBV2	251	235	0.02%	0.003%
56	7.182	1809	1817	1825	rVB2	1561	2073	0.19%	0.025%
57	7.285	1846	1849	1852	rVB2	204	125	0.01%	0.002%
58	7.314	1852	1858	1861	rVB2	227	257	0.02%	0.003%
59	7.340	1861	1866	1868	rBV2	196	176	0.02%	0.002%
60	7.459	1900	1903	1907	rBV2	248	237	0.02%	0.003%
61	7.571	1924	1938	1954	rBV	134439	234115	21.62%	2.824%
62	7.687	1969	1974	1982	rVB4	1050	1624	0.15%	0.020%
63	7.796	2004	2008	2012	rVB2	306	306	0.03%	0.004%
64	7.903	2026	2041	2056	rBV	455034	769003	71.02%	9.276%
65	8.182	2116	2128	2145	rBV	93928	157030	14.50%	1.894%
66	8.292	2160	2162	2168	rVB2	260	142	0.01%	0.002%
67	8.382	2187	2190	2192	rBV2	190	141	0.01%	0.002%
68	8.636	2256	2269	2313	rBV	431981	775031	71.58%	9.348%
69	8.848	2329	2335	2337	rBV2	268	258	0.02%	0.003%
70	9.272	2464	2467	2470	rBV2	277	252	0.02%	0.003%
71	9.420	2500	2513	2551	rBV	436041	724818	66.94%	8.743%
72	9.575	2557	2561	2562	rBV	187	152	0.01%	0.002%
73	9.700	2591	2600	2606	rBV4	490	744	0.07%	0.009%
74	9.758	2612	2618	2623	rBV2	169	232	0.02%	0.003%
75	9.787	2624	2627	2630	rBV2	175	138	0.01%	0.002%
76	9.964	2678	2682	2686	rBV2	199	183	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044816.D
 Acq On : 24 Sep 2021 17:20
 Operator : SY/MD
 Sample : VIBLK002
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.671	2897	2902	2910	rVB3	1598	2207	0.20%	0.027%
78	10.761	2917	2930	2951	rVB	377633	604575	55.84%	7.292%
79	10.867	2961	2963	2967	rVB2	276	175	0.02%	0.002%
80	10.902	2970	2974	2978	rVB2	258	211	0.02%	0.003%
81	11.095	3031	3034	3035	rBV	248	146	0.01%	0.002%
82	11.298	3094	3097	3099	rBV	159	135	0.01%	0.002%
83	11.465	3144	3149	3159	rVB4	1295	1965	0.18%	0.024%
84	11.565	3177	3180	3183	rBV2	160	152	0.01%	0.002%
85	11.581	3183	3185	3188	rVB2	249	165	0.02%	0.002%
86	11.697	3218	3221	3222	rBV	405	280	0.03%	0.003%
87	11.816	3246	3258	3280	rBV	405768	643498	59.43%	7.762%
88	11.918	3289	3290	3292	rBV	243	132	0.01%	0.002%
89	11.941	3295	3297	3303	rVV3	721	749	0.07%	0.009%
90	11.976	3305	3308	3319	rVB4	1287	1583	0.15%	0.019%
91	12.195	3363	3376	3397	rVV	431401	704630	65.08%	8.499%
92	12.333	3416	3419	3423	rVB2	263	185	0.02%	0.002%
93	12.423	3445	3447	3449	rBV	254	142	0.01%	0.002%
94	12.645	3514	3516	3520	rBV2	229	129	0.01%	0.002%
95	12.754	3545	3550	3553	rBV2	204	250	0.02%	0.003%
96	13.121	3658	3664	3666	rBV2	204	256	0.02%	0.003%
97	13.285	3713	3715	3718	rBV2	167	111	0.01%	0.001%
98	13.918	3909	3912	3919	rBV2	277	314	0.03%	0.004%
99	14.976	4239	4241	4245	rBV2	262	169	0.02%	0.002%
100	15.018	4252	4254	4257	rVB2	380	172	0.02%	0.002%


Sum of corrected areas: 8290518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044816.D
Acq On : 24 Sep 2021 17:20
Operator : SY/MD
Sample : VIBLK002
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

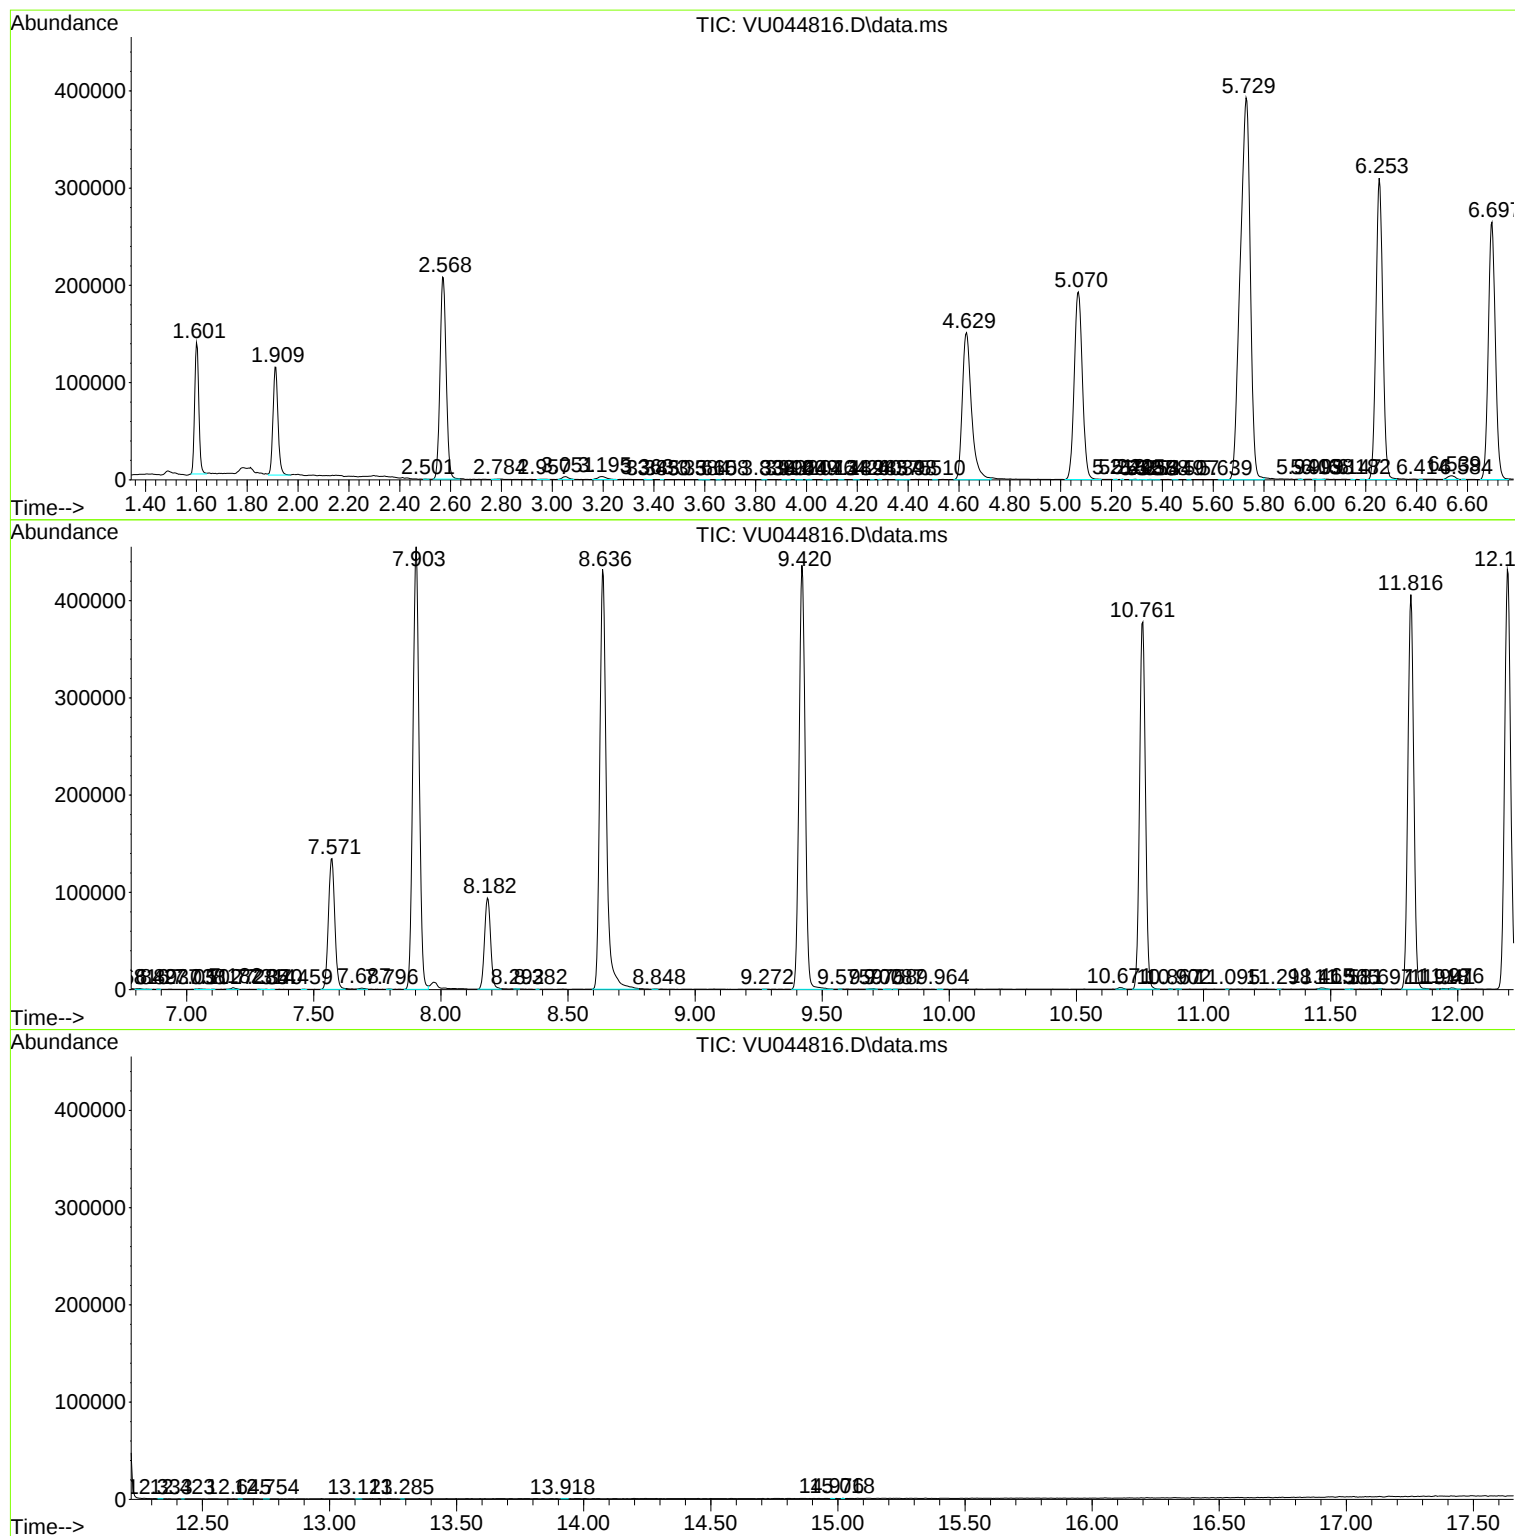

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044816.D
Acq On : 24 Sep 2021 17:20
Operator : SY/MD
Sample : VIBLK002
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044816.D
Acq On : 24 Sep 2021 17:20
Operator : SY/MD
Sample : VIBLK002
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
