

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044817.D
 Acq On : 24 Sep 2021 17:44
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU044817.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rBV	159160	181819	3.49%	1.130%
2	1.906	168	176	193	rVB	116534	164207	3.15%	1.020%
3	2.568	369	382	397	rBV	233050	390284	7.50%	2.425%
4	2.761	432	442	454	rBV3	4419	8936	0.17%	0.056%
5	2.909	484	488	490	rBV2	143	147	0.00%	0.001%
6	2.941	496	498	500	rBV	313	209	0.00%	0.001%
7	2.993	511	514	518	rBV	224	183	0.00%	0.001%
8	3.047	525	531	534	rBV5	721	883	0.02%	0.005%
9	3.096	545	546	552	rBV2	140	102	0.00%	0.001%
10	3.141	552	560	566	rBV4	976	1561	0.03%	0.010%
11	3.195	567	577	586	rVB2	1221	2530	0.05%	0.016%
12	3.266	595	599	601	rBV2	212	198	0.00%	0.001%
13	3.308	608	612	615	rBV2	188	175	0.00%	0.001%
14	3.356	615	627	644	rVB2	32367	63088	1.21%	0.392%
15	3.433	647	651	652	rBV	157	110	0.00%	0.001%
16	3.478	662	665	668	rVB2	174	118	0.00%	0.001%
17	3.498	668	671	674	rBV	168	179	0.00%	0.001%
18	3.543	682	685	689	rVB	205	159	0.00%	0.001%
19	3.716	736	739	742	rBV2	160	147	0.00%	0.001%
20	3.832	772	775	777	rBV	185	117	0.00%	0.001%
21	3.874	785	788	790	rBV	126	102	0.00%	0.001%
22	3.941	806	809	812	rBV	252	235	0.00%	0.001%
23	4.076	848	851	855	rVB	205	171	0.00%	0.001%
24	4.189	883	886	888	rBV2	183	112	0.00%	0.001%
25	4.263	905	909	911	rBV	187	187	0.00%	0.001%
26	4.379	942	945	947	rBV	133	115	0.00%	0.001%
27	4.446	961	966	970	rBV2	282	320	0.01%	0.002%
28	4.559	998	1001	1003	rBV2	146	107	0.00%	0.001%
29	4.671	1007	1036	1063	rBV2	921673	2379699	45.71%	14.787%
30	5.067	1143	1159	1183	rBV	206710	451884	8.68%	2.808%
31	5.218	1204	1206	1219	rVB5	600	766	0.01%	0.005%
32	5.292	1225	1229	1230	rBV	266	189	0.00%	0.001%
33	5.565	1312	1314	1317	rVB	238	155	0.00%	0.001%
34	5.729	1343	1365	1394	rBV2	419424	1156646	22.22%	7.187%
35	5.951	1430	1434	1438	rBV2	213	218	0.00%	0.001%
36	6.038	1457	1461	1466	rBV3	331	408	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044817.D
 Acq On : 24 Sep 2021 17:44
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.112	1482	1484	1490	rVB2	168	167	0.00%	0.001%
38	6.192	1507	1509	1513	rVB3	472	300	0.01%	0.002%
39	6.253	1513	1528	1548	rBV	341208	637747	12.25%	3.963%
40	6.356	1558	1560	1561	rBV	282	138	0.00%	0.001%
41	6.546	1602	1619	1652	rBV	2774769	5206086	100.00%	32.350%
42	6.697	1653	1666	1692	rVB	279343	552901	10.62%	3.436%
43	6.938	1734	1741	1745	rBV	439	613	0.01%	0.004%
44	7.034	1767	1771	1772	rBV2	502	372	0.01%	0.002%
45	7.134	1797	1802	1804	rBV2	211	230	0.00%	0.001%
46	7.179	1809	1816	1817	rBV2	1364	1104	0.02%	0.007%
47	7.259	1838	1841	1848	rBV	266	289	0.01%	0.002%
48	7.311	1855	1857	1861	rVB2	318	157	0.00%	0.001%
49	7.343	1865	1867	1871	rVB	206	101	0.00%	0.001%
50	7.375	1872	1877	1878	rBV3	179	138	0.00%	0.001%
51	7.449	1897	1900	1908	rBV2	230	297	0.01%	0.002%
52	7.568	1922	1937	1956	rBV	143682	251155	4.82%	1.561%
53	7.690	1968	1975	1981	rBV3	753	1183	0.02%	0.007%
54	7.796	2006	2008	2011	rBV	193	128	0.00%	0.001%
55	7.903	2026	2041	2056	rBV	492005	839511	16.13%	5.217%
56	7.970	2057	2062	2074	rVB2	7428	12349	0.24%	0.077%
57	8.182	2116	2128	2146	rBV2	100479	167628	3.22%	1.042%
58	8.327	2170	2173	2175	rBV	324	205	0.00%	0.001%
59	8.382	2187	2190	2193	rBV	208	187	0.00%	0.001%
60	8.430	2202	2205	2211	rBV	197	232	0.00%	0.001%
61	8.472	2212	2218	2229	rVB4	848	1503	0.03%	0.009%
62	8.536	2235	2238	2240	rBV	188	152	0.00%	0.001%
63	8.549	2240	2242	2244	rVB	250	114	0.00%	0.001%
64	8.636	2256	2269	2314	rBV	421379	749936	14.40%	4.660%
65	8.944	2362	2365	2371	rVB2	159	177	0.00%	0.001%
66	9.173	2434	2436	2441	rVB2	194	101	0.00%	0.001%
67	9.279	2466	2469	2471	rBV3	158	98	0.00%	0.001%
68	9.420	2500	2513	2530	rBV	493169	788382	15.14%	4.899%
69	9.552	2551	2554	2556	rBV2	177	114	0.00%	0.001%
70	9.629	2575	2578	2580	rBV	169	126	0.00%	0.001%
71	9.700	2593	2600	2606	rVB	635	855	0.02%	0.005%
72	9.880	2653	2656	2661	rBV	185	150	0.00%	0.001%
73	10.099	2721	2724	2725	rBV	232	118	0.00%	0.001%
74	10.623	2884	2887	2890	rBV	163	106	0.00%	0.001%
75	10.674	2895	2903	2910	rBV3	1773	2509	0.05%	0.016%
76	10.761	2917	2930	2951	rBV	390529	624256	11.99%	3.879%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
 Data File : VU044817.D
 Acq On : 24 Sep 2021 17:44
 Operator : SY/MD
 Sample : M3873-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.867	2960	2963	2967	rVB2	346	294	0.01%	0.002%
78	10.896	2968	2972	2980	rBV3	556	479	0.01%	0.003%
79	10.983	2996	2999	3004	rBV	155	163	0.00%	0.001%
80	11.115	3034	3040	3041	rBV	215	203	0.00%	0.001%
81	11.246	3076	3081	3084	rBV2	245	238	0.00%	0.001%
82	11.349	3110	3113	3118	rBV2	193	147	0.00%	0.001%
83	11.462	3142	3148	3159	rVB3	1386	2094	0.04%	0.013%
84	11.626	3195	3199	3203	rBV2	399	350	0.01%	0.002%
85	11.674	3211	3214	3217	rBV2	146	104	0.00%	0.001%
86	11.700	3217	3222	3225	rBV3	663	702	0.01%	0.004%
87	11.816	3245	3258	3279	rBV	440512	692264	13.30%	4.302%
88	11.976	3304	3308	3315	rVB2	1431	1593	0.03%	0.010%
89	12.066	3330	3336	3345	rBV4	1155	1455	0.03%	0.009%
90	12.198	3363	3377	3394	rBV	458432	742551	14.26%	4.614%
91	12.565	3489	3491	3498	rVB2	192	114	0.00%	0.001%
92	12.645	3512	3516	3519	rBV2	383	326	0.01%	0.002%
93	12.761	3550	3552	3553	rBV	265	107	0.00%	0.001%
94	12.880	3584	3589	3592	rBV	346	322	0.01%	0.002%
95	12.902	3593	3596	3599	rBV2	255	214	0.00%	0.001%
96	13.385	3744	3746	3751	rVB2	247	123	0.00%	0.001%
97	14.124	3974	3976	3980	rBV2	220	135	0.00%	0.001%
98	14.838	4195	4198	4201	rVB	298	171	0.00%	0.001%
99	14.970	4237	4239	4242	rBV	232	107	0.00%	0.001%
100	15.121	4283	4286	4288	rBV2	254	178	0.00%	0.001%




Sum of corrected areas: 16092815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044817.D
Acq On : 24 Sep 2021 17:44
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

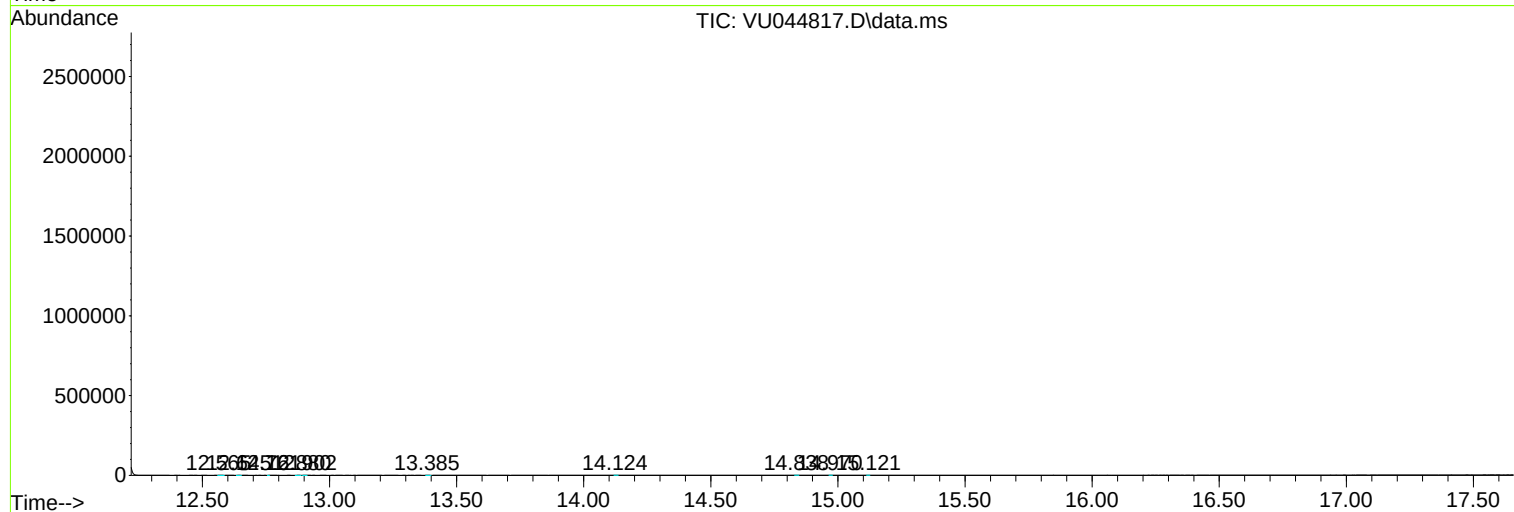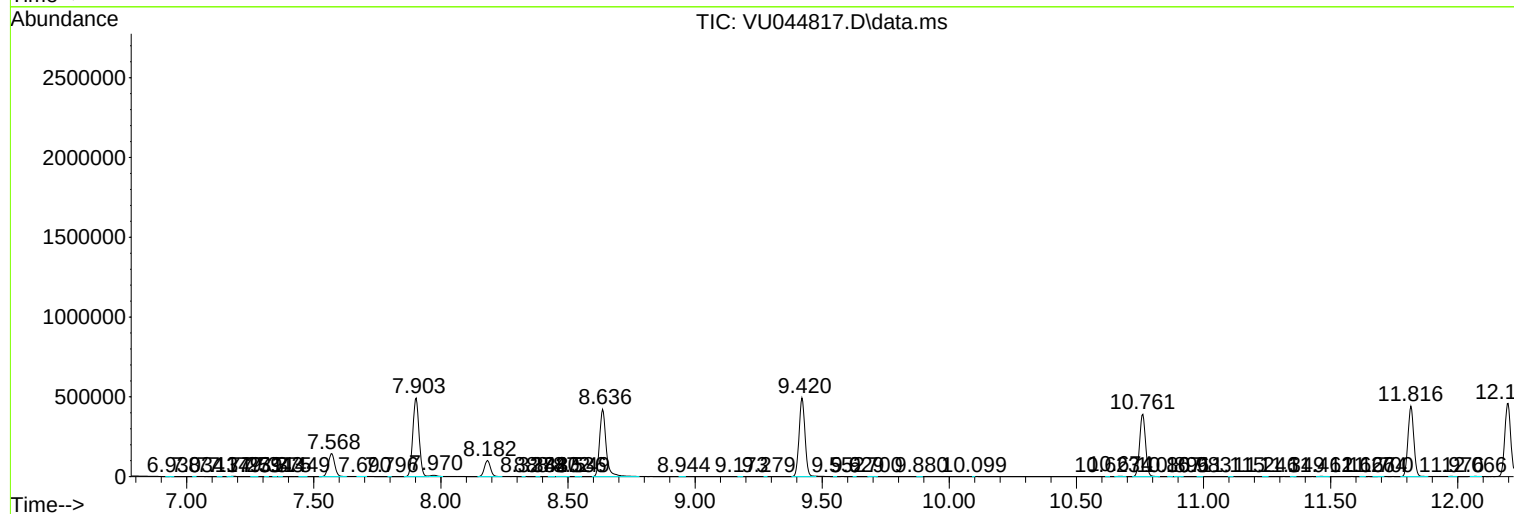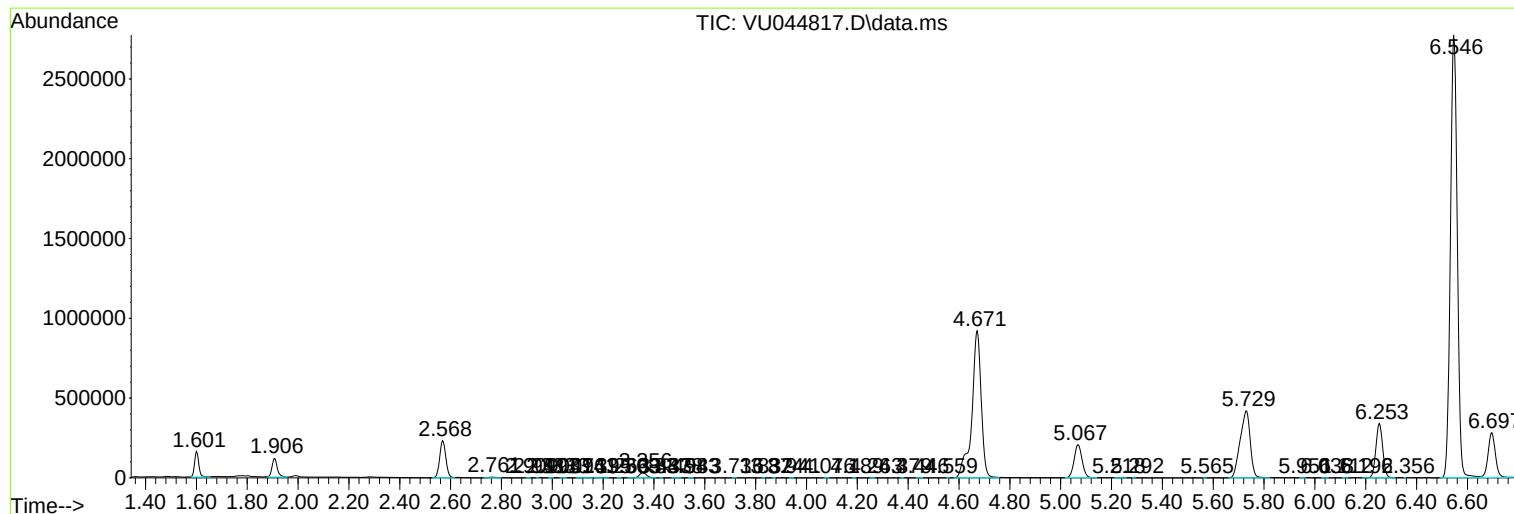

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044817.D
Acq On : 24 Sep 2021 17:44
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092421\
Data File : VU044817.D
Acq On : 24 Sep 2021 17:44
Operator : SY/MD
Sample : M3873-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
