


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092424\
Data File : VU060987.D
Acq On : 24 Sep 2024 10:12
Operator : MD/SY
Sample : BFB004
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB004

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 25 04:46:41 2024

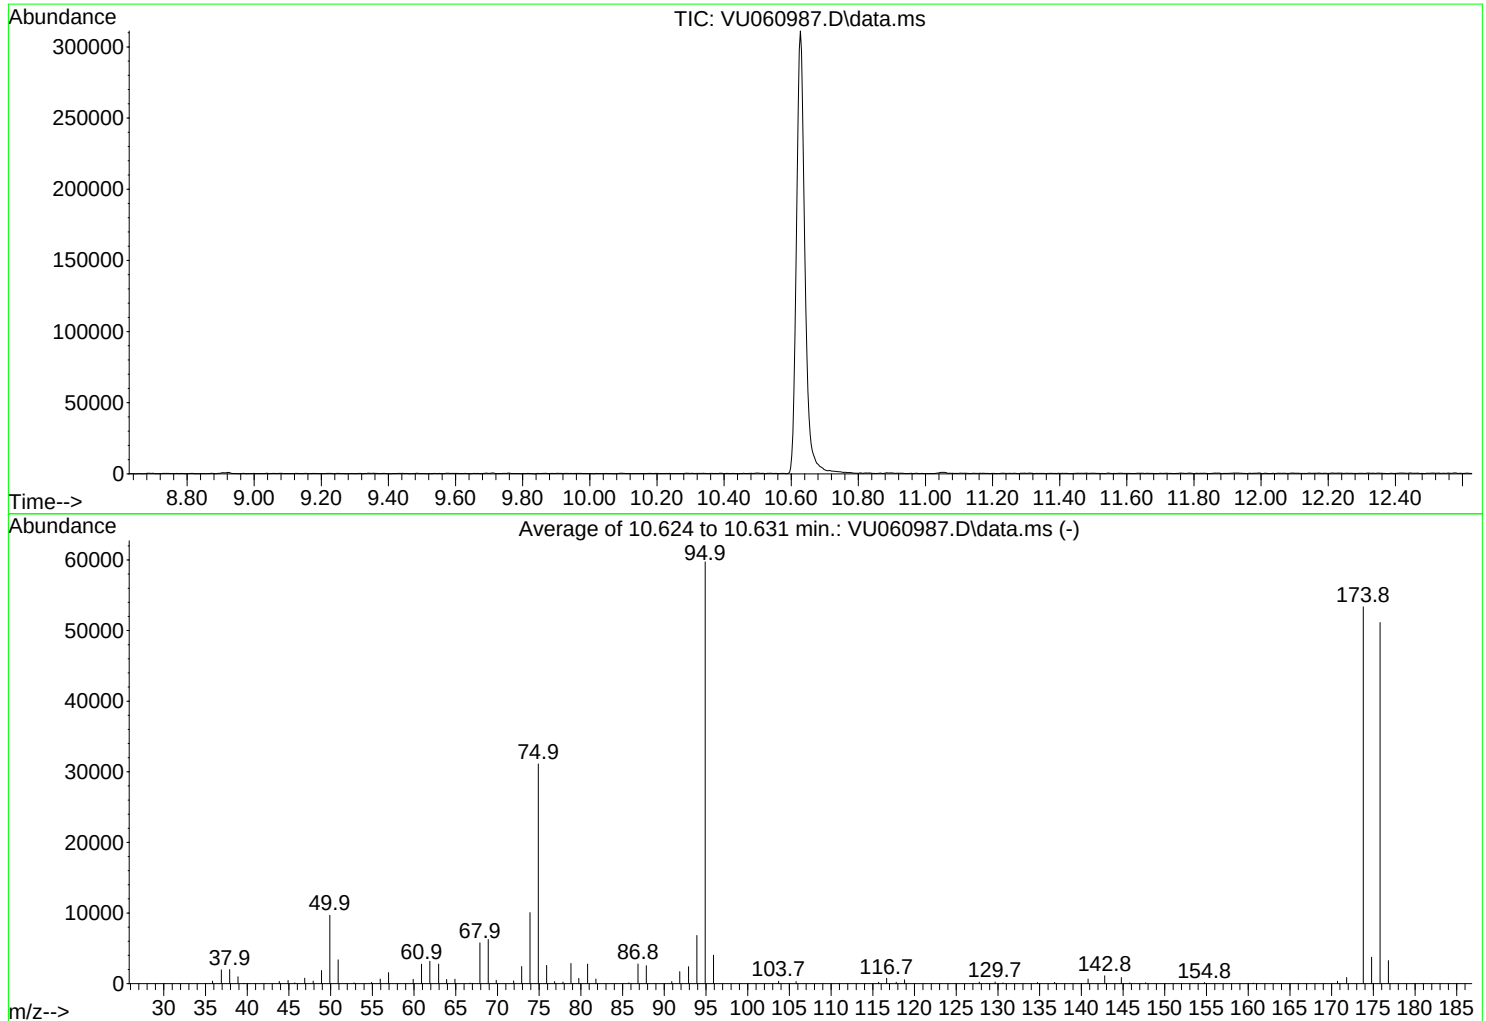

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	9677	PASS
75	95	30	80	52.1	31115	PASS
95	95	100	100	100.0	59731	PASS
96	95	5	9	6.8	4039	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.3	53357	PASS
175	174	5	9	7.0	3750	PASS
176	174	95	101	95.9	51147	PASS
177	176	5	9	6.4	3270	PASS

m/z	Abundance
43.80	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.80	398.0
36.90	2013.0
37.90	2082.0
38.90	965.0
43.90	536.0
44.90	471.0
45.70	209.0
46.90	792.0
47.90	363.0
48.90	1956.0
49.90	9921.0
50.90	3429.0
51.80	103.0
52.80	168.0
54.90	200.0
56.00	713.0
56.90	1619.0
59.90	566.0
60.90	2842.0
61.90	3218.0
63.00	2719.0
63.90	669.0
64.90	577.0
67.00	148.0
67.90	6044.0
68.90	6293.0
69.90	443.0
71.90	368.0
72.90	2468.0
73.90	9994.0
74.90	31296.0
75.90	2484.0
76.90	245.0
77.90	225.0
78.80	2813.0
79.70	780.0
80.80	2576.0
81.80	679.0
85.70	208.0
86.80	2670.0
87.80	2354.0
90.90	307.0
91.90	1806.0
92.90	2199.0
93.90	6340.0
94.90	59200.0
95.90	3990.0
103.70	317.0
105.80	260.0
115.70	187.0
116.70	757.0
117.80	209.0
118.80	580.0
127.80	235.0
129.70	249.0
130.60	130.0
134.70	130.0
136.80	197.0
140.80	652.0
142.80	1098.0
144.80	899.0
147.70	132.0
154.70	149.0
170.70	340.0
171.80	800.0
173.80	52120.0
174.80	3834.0
175.80	49072.0
176.80	3065.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.90	357.0
36.90	1987.0
37.90	2014.0
38.90	1014.0
43.90	577.0
44.90	465.0
45.70	162.0
46.90	805.0
47.90	383.0
48.90	1887.0
49.90	9902.0
50.90	3499.0
52.80	147.0
54.90	193.0
56.00	679.0
56.90	1597.0
59.90	627.0
60.90	2838.0
61.90	3195.0
62.90	2857.0
63.90	594.0
64.90	649.0
66.70	121.0
67.90	5969.0
68.90	6519.0
69.80	456.0
72.00	395.0
72.90	2526.0
73.90	10345.0
74.90	32096.0
75.90	2602.0
76.90	276.0
77.90	234.0
78.80	2984.0
79.80	757.0
80.80	2829.0
81.80	706.0
85.80	140.0
86.90	2894.0
87.80	2642.0
90.90	313.0
91.90	1685.0
92.90	2464.0
93.90	7062.0
94.90	61432.0
95.90	4185.0
103.70	361.0
105.80	303.0
115.70	217.0
116.60	784.0
117.80	209.0
118.80	552.0
127.80	240.0
129.60	263.0
130.60	127.0
134.80	169.0
136.80	188.0
140.80	692.0
142.80	1043.0
144.80	918.0
145.80	130.0
147.70	159.0
154.80	160.0
160.60	118.0
170.70	336.0
171.80	903.0
173.80	55208.0
174.80	3864.0
175.80	52744.0
176.80	3395.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004

m/z	Abundance
35.90	322.0
36.90	1846.0
37.90	1883.0
38.90	935.0
39.60	152.0
43.90	548.0
44.90	406.0
46.90	720.0
47.90	336.0
48.90	1732.0
49.90	9209.0
50.90	3205.0
54.90	142.0
55.90	600.0
57.00	1463.0
59.90	645.0
60.90	2640.0
61.90	3095.0
62.90	2726.0
63.90	524.0
64.90	664.0
66.70	141.0
67.90	5336.0
68.90	5928.0
69.80	499.0
72.00	410.0
72.90	2316.0
73.90	9828.0
74.90	29952.0
75.90	2655.0
76.80	365.0
77.80	198.0
78.80	2745.0
79.80	695.0
80.80	2898.0
81.80	598.0
86.90	2781.0
87.90	2603.0
90.90	301.0
91.80	1594.0
92.90	2564.0
93.90	7086.0
94.90	58560.0
95.90	3943.0
103.70	372.0
105.80	291.0
115.70	206.0
116.60	701.0
117.80	204.0
118.80	497.0
127.70	237.0
128.70	112.0
129.70	231.0
130.60	100.0
134.80	161.0
136.80	174.0
140.80	658.0
142.80	1185.0
144.80	799.0
145.80	189.0
147.70	146.0
154.80	168.0
160.60	102.0
170.70	335.0
171.80	913.0
173.80	52744.0
174.80	3552.0
175.80	51624.0
176.80	3351.0

Instrument :
MSVOA_U
ClientSampleId :
BFB004