




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063631.D
Acq On : 24 Sep 2025 10:03
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:05:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

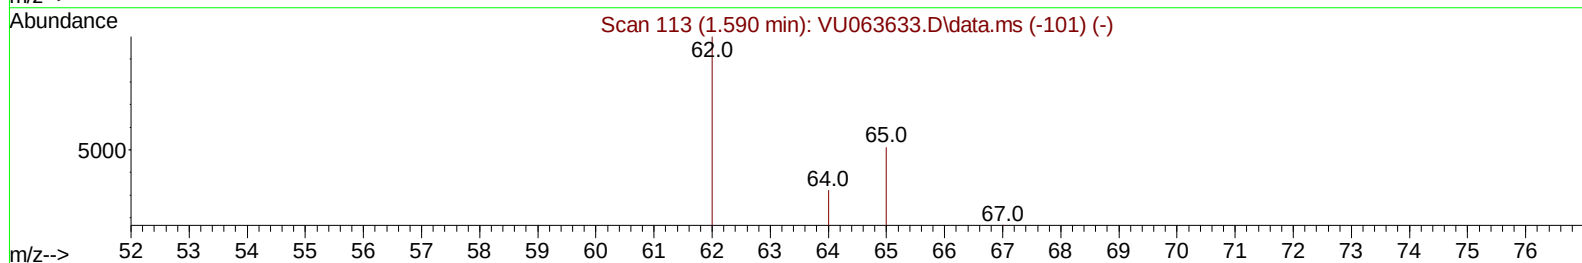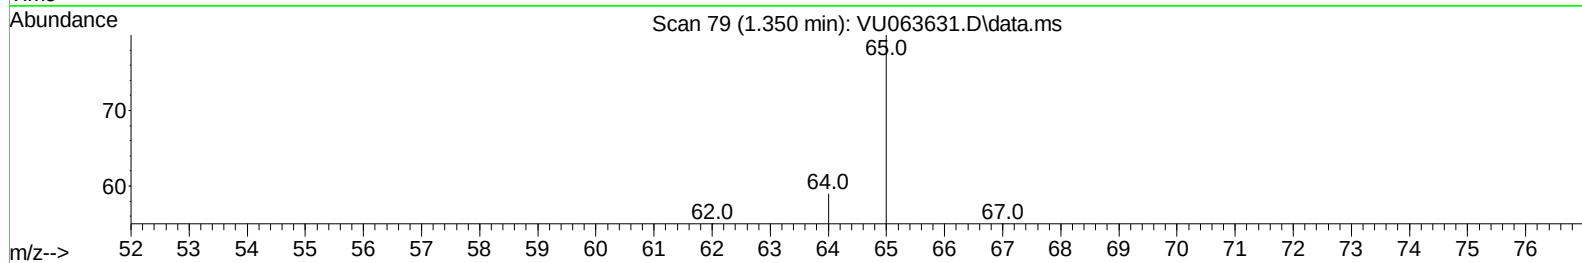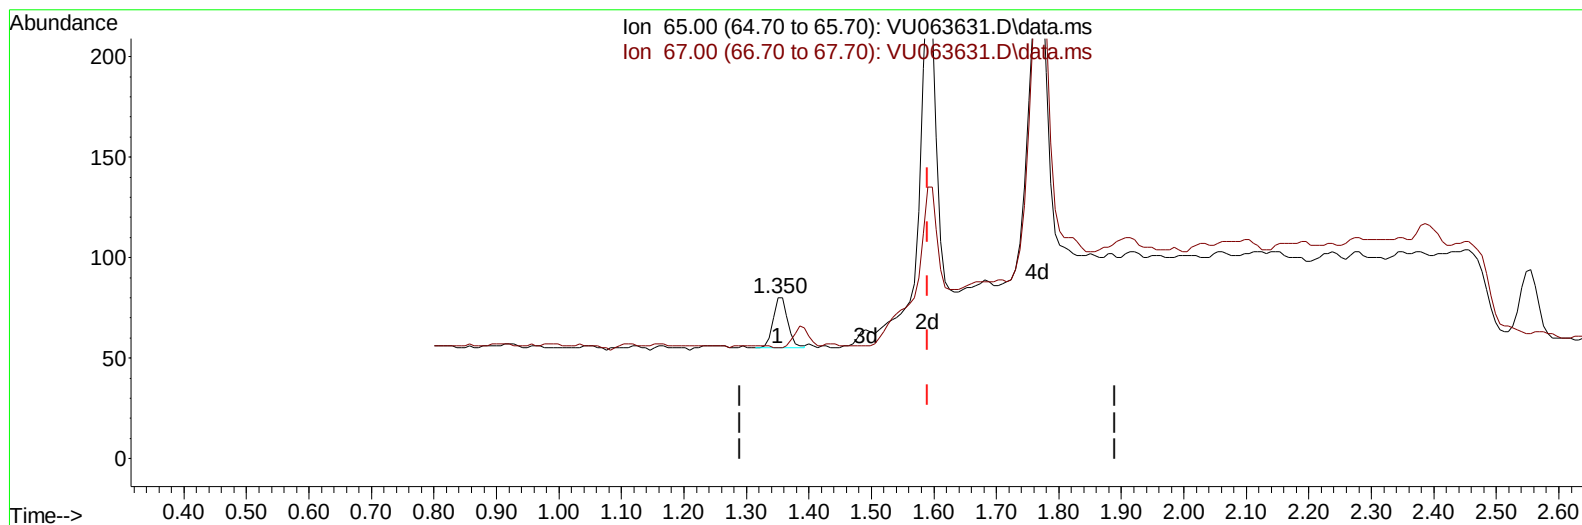

TIC: VU063631.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.350min (-0.240) 0.01 ug/L

response 41

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	37.80	46.34
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063631.D
Acq On : 24 Sep 2025 10:03
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:05:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

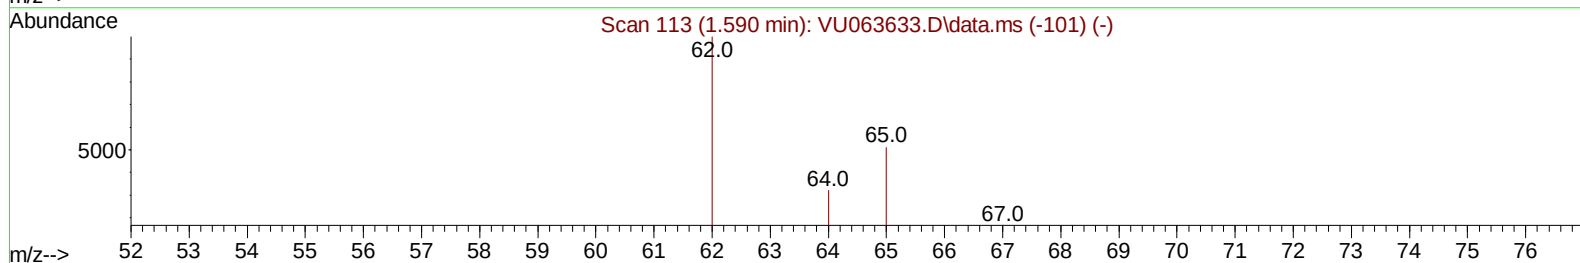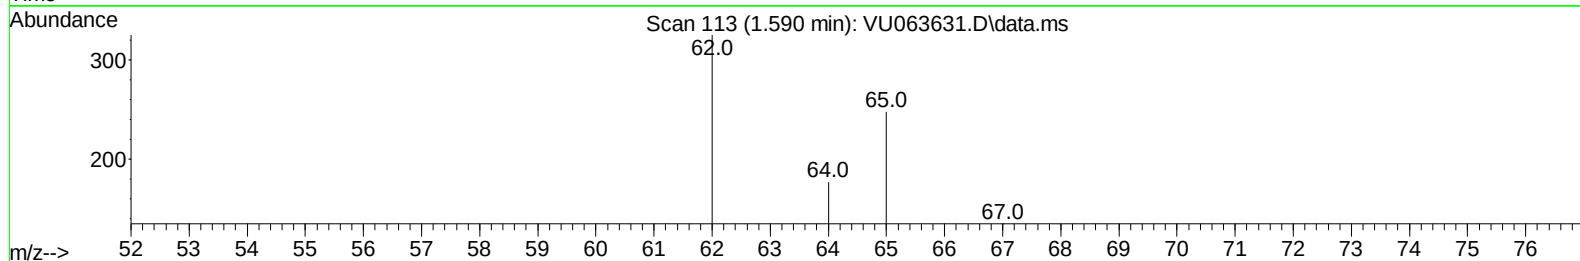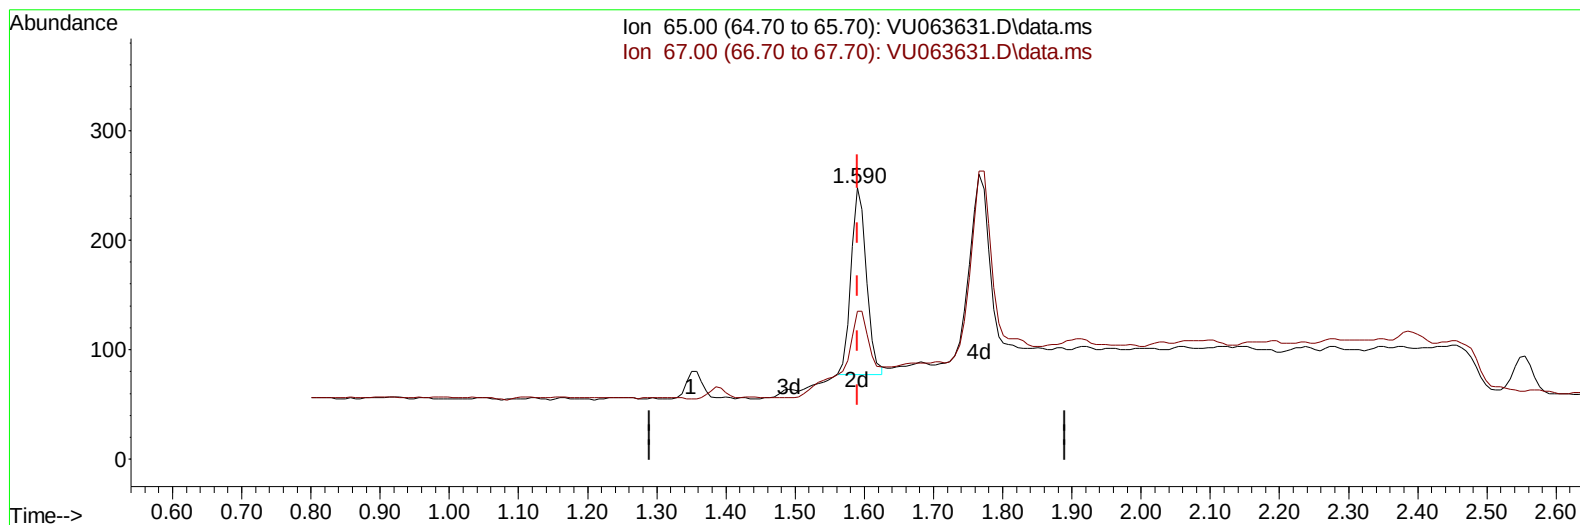

TIC: VU063631.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.590min (-0.000) 0.06 ug/L m

response 265

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	37.80	7.17#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
 Data File : VU063631.D
 Acq On : 24 Sep 2025 10:03
 Operator : MD/SY
 Sample : VSTD0.0562
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.05062

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
 Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:05:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 25 04:05:23 2025
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.258	114		7228	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117		10268	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152		3607	0.500	ug/L	0.02
System Monitoring Compounds							
2) Vinyl Chloride-d3	1.590	65		265m	0.059	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.709	65		179	0.066	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.687	67		125	0.048	ug/L	0.00
8) Toluene-d8	7.903	98		530	0.061	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.745	84		139	0.067	ug/L	0.00
Target Compounds							Qvalue
3) Vinyl chloride	1.590	62		520	0.063	ug/L #	65
6) Trichloroethene	6.544	95		358	0.058	ug/L	94
9) 1,2-Dibromoethane	8.924	107		161	0.047	ug/L #	87
12) 1,2,3-Trichloropropane	10.814	75		158	0.050	ug/L #	88
13) 1,2-Dibromo-3-chloropr...	13.007	75		28	0.052	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063631.D
Acq On : 24 Sep 2025 10:03
Operator : MD/SY
Sample : VSTD0.0562
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.05062

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:05:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

