




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063632.D
Acq On : 24 Sep 2025 10:39
Operator : MD/SY
Sample : VSTD0.163
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.1063

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:06:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

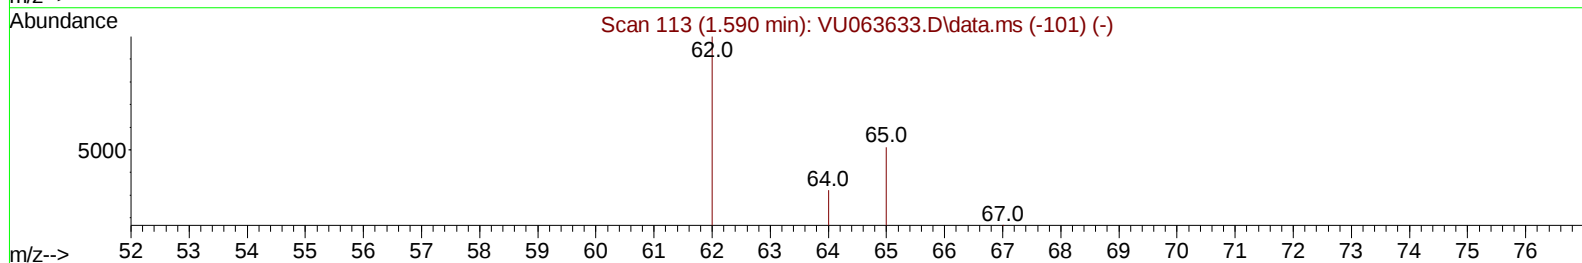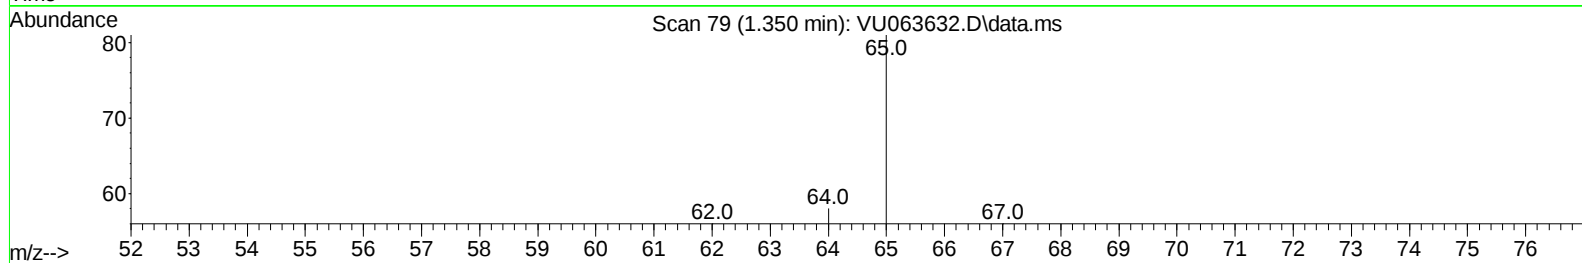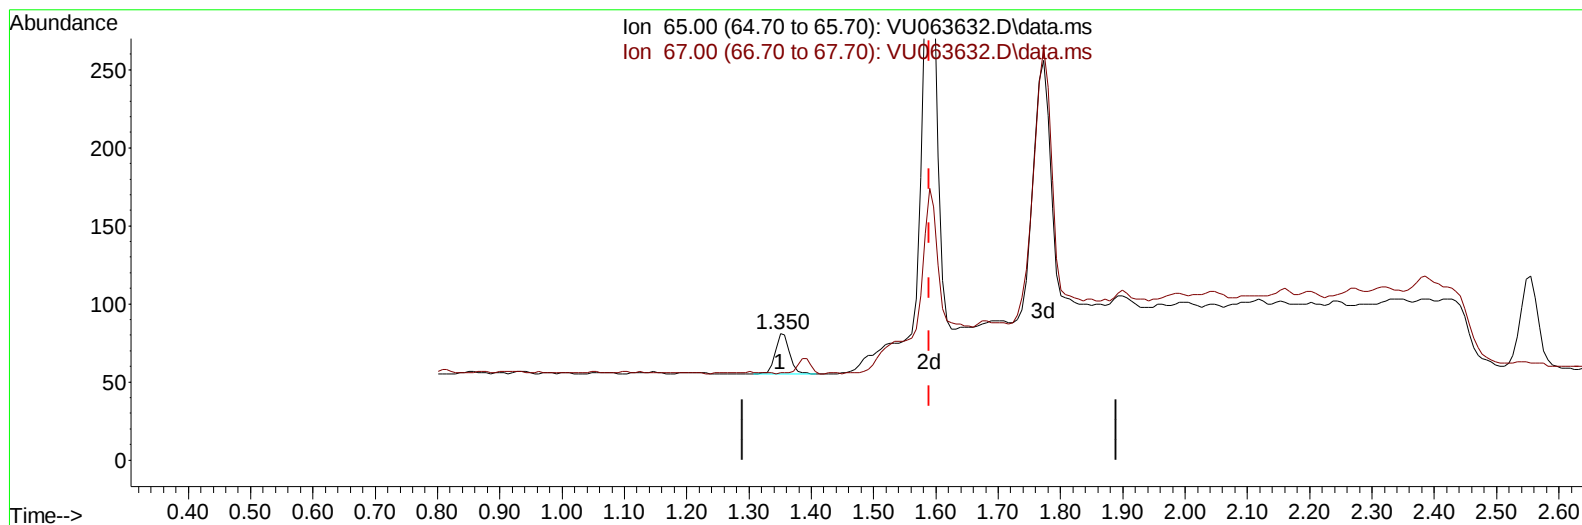

TIC: VU063632.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.350min (-0.240) 0.01 ug/L

response 42

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	37.80	38.10
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063632.D
Acq On : 24 Sep 2025 10:39
Operator : MD/SY
Sample : VSTD0.163
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.1063

Manual IntegrationsAPPROVED

Quant Time: Sep 25 04:06:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

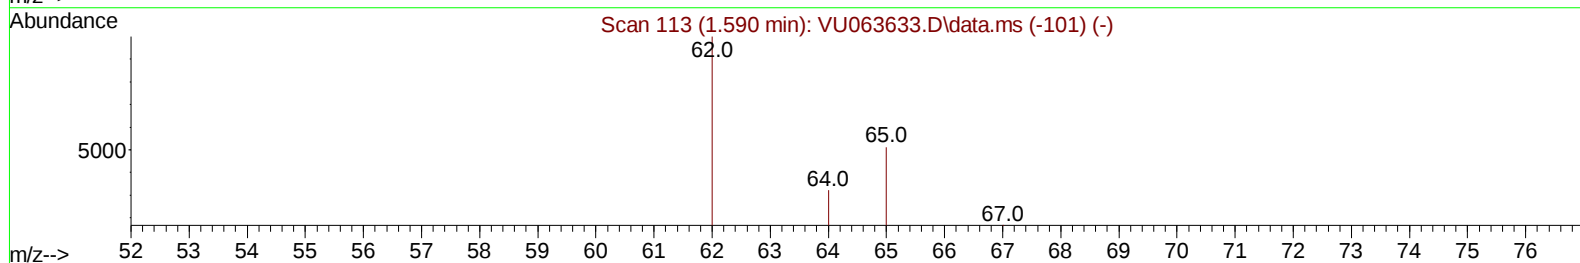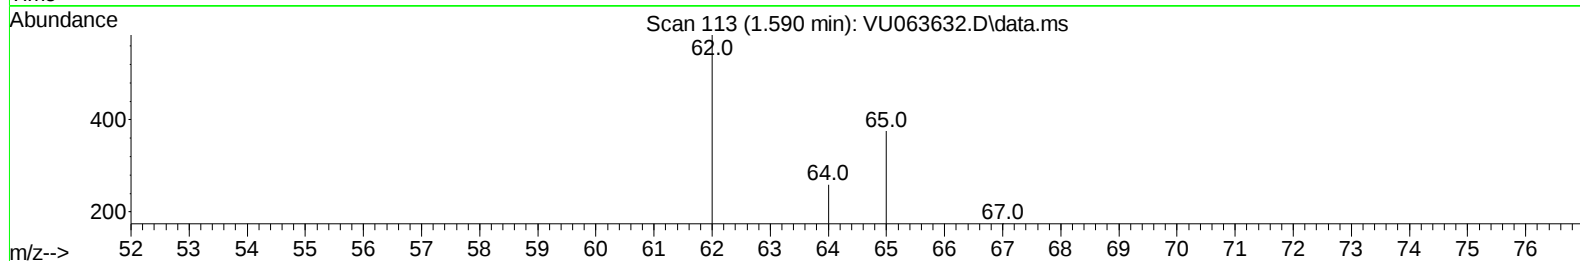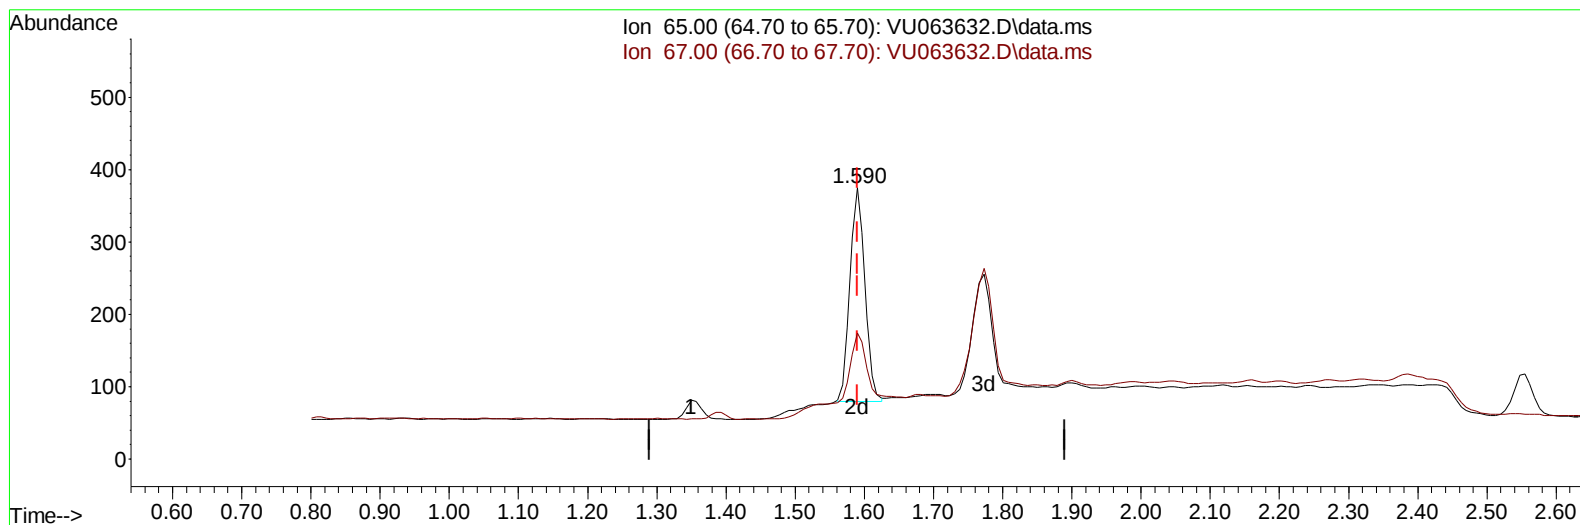

TIC: VU063632.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.590min (-0.000) 0.10 ug/L m

response 440

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	37.80	3.64#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
 Data File : VU063632.D
 Acq On : 24 Sep 2025 10:39
 Operator : MD/SY
 Sample : VSTD0.163
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VSTD0.1063

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/26/2025
 Supervised By :Semsettin Yesilyurt 09/26/2025

Quant Time: Sep 25 04:06:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 25 04:05:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.257	114	6895	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	9741	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.825	152	3445	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	440m	0.104	ug/L	0.00
4) 1,2-Dichloroethane-d4	5.709	65	281	0.109	ug/L	0.00
7) 1,2-Dichloropropane-d6	6.687	67	252	0.102	ug/L	0.00
8) Toluene-d8	7.903	98	818	0.099	ug/L	0.02
10) 1,1,2,2-Tetrachloroeth...	10.745	84	199	0.101	ug/L	0.00
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.590	62	920	0.117	ug/L #	82
6) Trichloroethene	6.544	95	607	0.104	ug/L	94
9) 1,2-Dibromoethane	8.923	107	298	0.092	ug/L #	90
12) 1,2,3-Trichloropropane	10.814	75	267	0.088	ug/L	89
13) 1,2-Dibromo-3-chloropr...	13.007	75	39	0.076	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063632.D
Acq On : 24 Sep 2025 10:39
Operator : MD/SY
Sample : VSTD0.163
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VSTD0.1063

Manual IntegrationsAPPROVED

Quant Time: Sep 25 04:06:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 25 04:05:23 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/26/2025
Supervised By :Semsettin Yesilyurt 09/26/2025

