


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092425\
Data File : VU063630.D
Acq On : 24 Sep 2025 08:52
Operator : MD/SY
Sample : BFB026
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB026

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM092425.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 25 04:13:39 2025

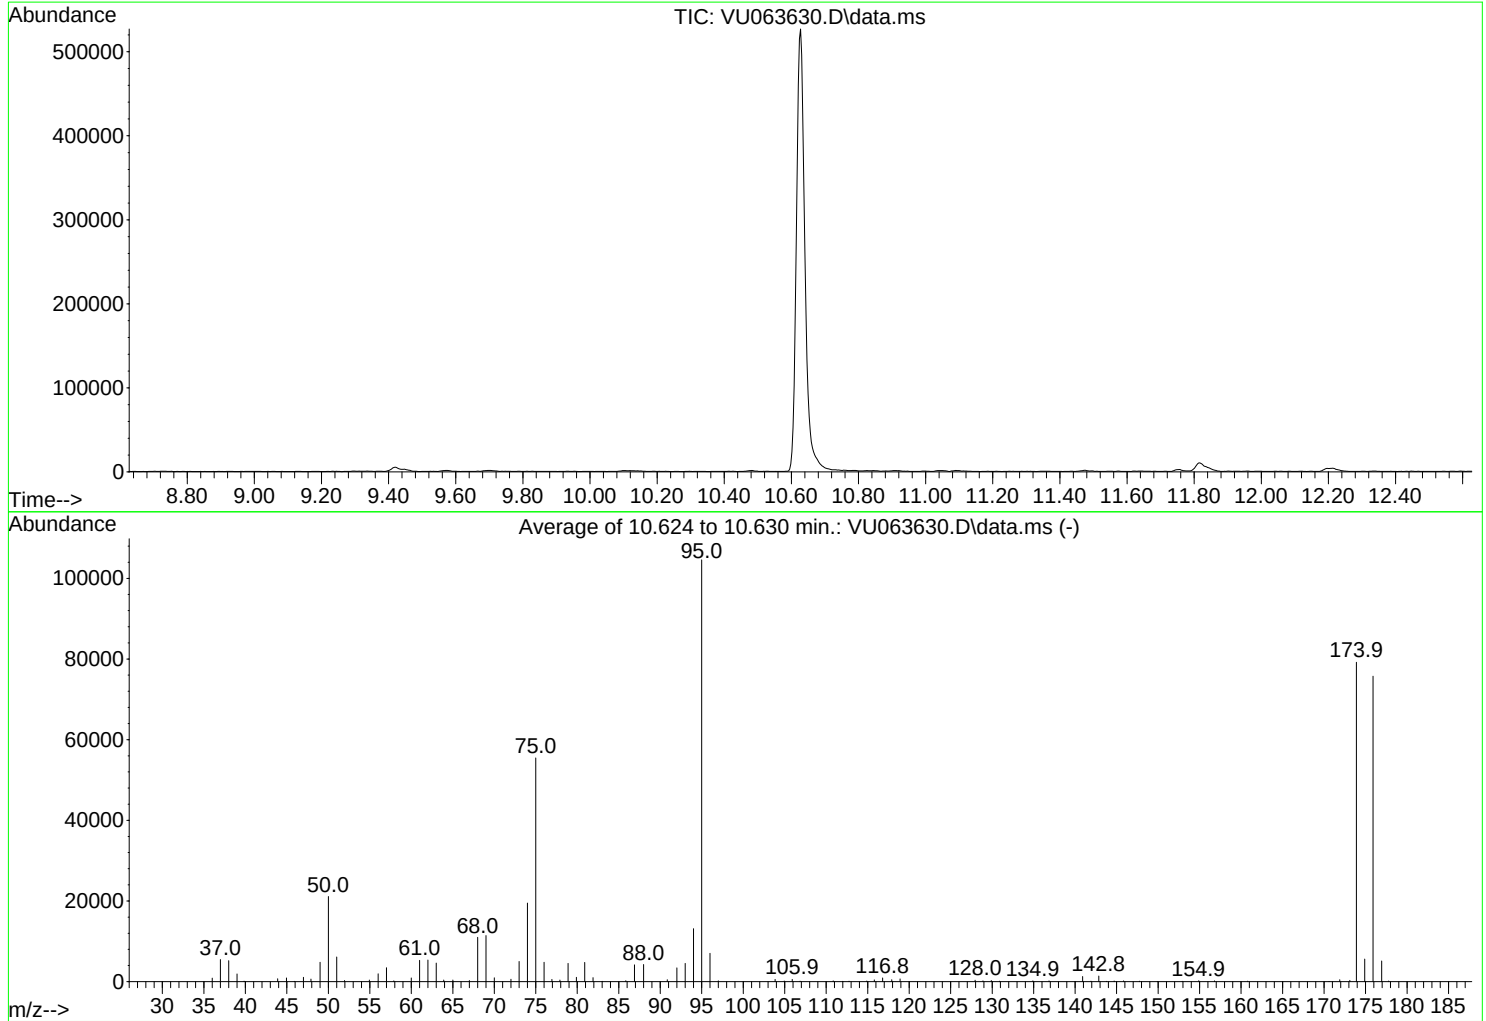

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	21117	PASS
75	95	30	80	53.0	55472	PASS
95	95	100	100	100.0	104592	PASS
96	95	5	9	6.7	7013	PASS
173	174	0.00	2	0.4	306	PASS
174	95	50	120	75.7	79181	PASS
175	174	5	9	7.1	5594	PASS
176	174	95	101	95.6	75725	PASS
177	176	5	9	6.7	5109	PASS

m/z	Abundance
39.80	171.0
44.00	548.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	922.0
37.00	5421.0
38.00	5014.0
39.00	1999.0
39.90	282.0
43.90	1341.0
45.00	1052.0
45.90	139.0
47.10	1211.0
47.90	696.0
49.00	4889.0
50.00	21456.0
51.00	6209.0
51.90	268.0
55.00	451.0
56.00	1964.0
57.00	3462.0
57.90	207.0
60.00	974.0
61.00	5336.0
62.00	5792.0
63.00	4526.0
63.90	406.0
65.00	391.0
67.00	260.0
68.00	11222.0
69.00	11813.0
70.00	925.0
72.00	592.0
73.00	5121.0
74.00	19728.0
75.00	55528.0
76.00	4727.0
77.00	586.0
77.90	388.0
78.90	4670.0
79.90	1150.0
80.90	4803.0
81.90	996.0
85.90	222.0
86.90	4306.0
88.00	4273.0
90.90	539.0
92.00	3571.0
93.00	4495.0
94.00	12936.0
95.00	105608.0
96.00	7431.0
97.00	185.0
103.90	515.0
104.90	157.0
105.90	536.0
106.90	145.0
110.90	175.0
112.80	109.0
114.90	171.0
115.80	455.0
116.80	891.0
117.90	509.0
118.90	620.0
127.90	407.0
128.90	221.0
129.80	269.0
130.90	124.0
134.90	168.0
136.80	221.0
140.90	1289.0
141.90	159.0
142.90	1477.0
144.70	184.0
145.90	192.0
147.70	206.0
149.90	101.0
154.90	276.0
156.80	199.0
160.80	122.0
171.90	426.0
173.10	919.0
173.90	77664.0
174.90	5833.0
175.90	74976.0
176.90	5035.0
177.80	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	908.0
37.00	5713.0
38.00	5362.0
39.00	1905.0
39.90	289.0
43.90	1322.0
45.00	930.0
45.90	138.0
47.00	1087.0
47.90	639.0
49.00	5028.0
50.00	21704.0
51.00	6133.0
52.00	282.0
54.90	400.0
56.00	2025.0
57.00	3566.0
57.90	200.0
60.00	885.0
61.00	5418.0
62.00	5519.0
63.00	4769.0
63.90	390.0
65.00	430.0
67.00	296.0
68.00	11295.0
69.00	11725.0
70.00	986.0
72.00	611.0
73.00	5122.0
74.00	19880.0
75.00	56752.0
76.00	4954.0
77.00	587.0
77.90	418.0
78.90	4629.0
79.90	1090.0
80.90	4910.0
81.90	1009.0
83.00	100.0
85.90	244.0
86.90	4295.0
88.00	4395.0
90.80	498.0
92.00	3539.0
93.00	4690.0
94.00	13438.0
95.00	107664.0
96.00	7137.0
97.00	210.0
103.80	553.0
105.00	161.0
105.90	614.0
106.80	152.0
110.80	211.0
112.00	117.0
112.80	122.0
114.90	155.0
115.80	460.0
116.80	911.0
117.90	473.0
118.90	715.0
128.00	363.0
128.90	235.0
129.90	278.0
130.90	135.0
134.90	222.0
136.90	196.0
140.00	105.0
140.90	1307.0
141.90	147.0
142.80	1419.0
143.80	110.0
144.70	187.0
145.90	181.0
147.80	151.0
152.90	129.0
154.90	230.0
156.80	189.0
160.80	149.0
171.90	455.0
173.90	81568.0
174.90	5663.0
175.90	78048.0
176.90	5289.0
177.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
36.00	846.0
37.00	5332.0
38.00	5181.0
39.00	1762.0
39.90	263.0
43.90	1138.0
44.90	742.0
46.90	970.0
47.90	542.0
49.00	4495.0
50.00	20192.0
51.00	5942.0
52.00	276.0
54.90	316.0
56.00	1883.0
57.00	3319.0
57.90	172.0
60.00	835.0
61.00	5096.0
62.00	4817.0
63.00	4522.0
63.90	392.0
65.00	328.0
67.00	329.0
68.00	10446.0
69.00	10738.0
70.00	918.0
72.00	570.0
73.00	4757.0
74.00	18808.0
75.00	54136.0
76.00	4771.0
76.90	555.0
77.90	450.0
78.90	4289.0
79.90	989.0
80.90	4557.0
81.90	965.0
83.00	155.0
85.80	261.0
86.90	3959.0
88.00	4082.0
90.90	430.0
92.00	3181.0
93.00	4444.0
94.00	13062.0
95.00	100504.0
96.00	6472.0
97.00	205.0
103.90	576.0
105.00	178.0
105.90	587.0
106.80	133.0
110.80	199.0
112.00	116.0
112.70	103.0
114.90	146.0
115.80	430.0
116.80	904.0
117.90	409.0
118.90	658.0
128.00	284.0
128.90	197.0
130.00	303.0
130.90	115.0
134.90	206.0
136.90	171.0
140.90	1164.0
141.90	113.0
142.80	1236.0
143.80	112.0
144.70	139.0
145.80	169.0
148.00	180.0
152.90	127.0
154.90	198.0
156.80	187.0
160.80	143.0
170.60	124.0
171.90	509.0
173.90	78312.0
174.90	5287.0
175.90	74152.0
177.00	5003.0
177.80	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026