


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU092518\
Data File : VU027122.D
Acq On : 25 Sep 2018 10:02
Operator : MD/SY
Sample : BFB45
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM092518WMA.M
Title : VOC Analysis
Last Update : Wed Sep 26 02:22:28 2018

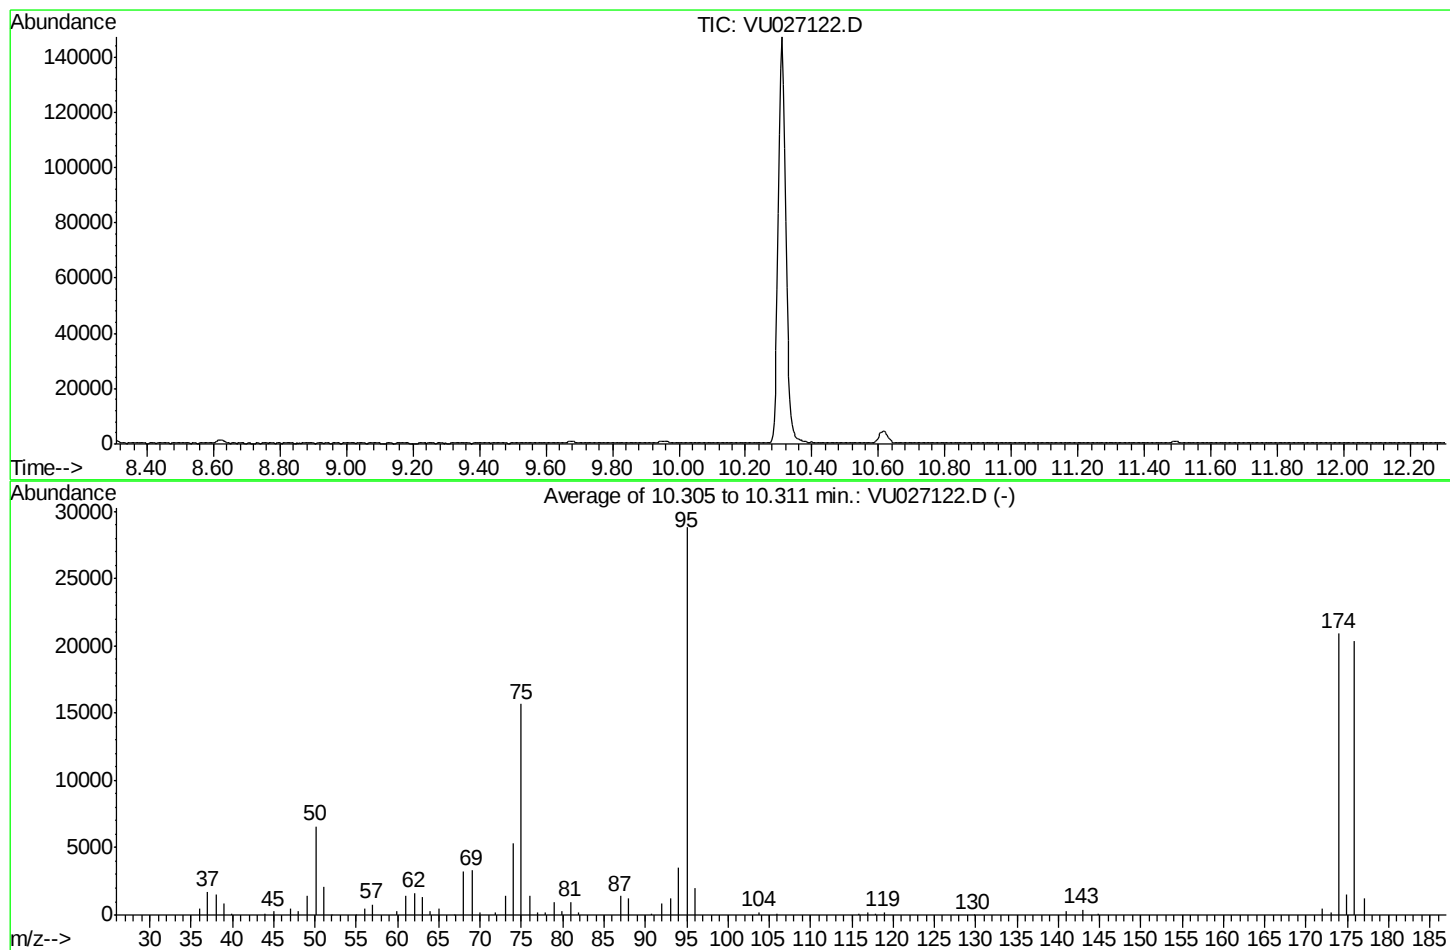

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	6588	PASS
75	95	30	80	54.4	15677	PASS
95	95	100	100	100.0	28802	PASS
96	95	5	9	6.9	1977	PASS
173	174	0.00	2	0.7	155	PASS
174	95	50	120	72.5	20882	PASS
175	174	5	9	7.5	1566	PASS
176	174	95	101	97.5	20352	PASS
177	176	5	9	6.3	1285	PASS

Scan 2829 (10.270 min): VU027122.D
BFB45

m/z	Abundance
39.90	107.0
43.90	407.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.00	447.0
37.00	1768.0
38.00	1511.0
39.00	862.0
39.00	169.0
43.00	528.0
45.00	316.0
47.00	446.0
47.00	243.0
49.00	1398.0
50.00	6423.0
51.00	2023.0
55.00	115.0
56.00	462.0
56.00	751.0
60.00	277.0
61.00	1435.0
62.00	1579.0
63.00	1296.0
63.00	259.0
65.00	437.0
68.00	3065.0
69.00	3129.0
70.00	220.0
71.00	199.0
73.00	1371.0
74.00	5216.0
75.00	15110.0
76.00	1351.0
76.00	194.0
77.00	127.0
78.00	885.0
80.00	237.0
80.00	929.0
81.00	178.0
86.00	1346.0
88.00	1162.0
90.00	127.0
91.00	826.0
93.00	1258.0
94.00	3267.0
95.00	27256.0
96.00	1973.0
103.00	195.0
105.00	110.0
115.00	121.0
116.00	203.0
117.00	117.0
118.00	245.0
140.00	313.0
142.00	393.0
144.00	108.0
171.00	445.0
174.00	19520.0
175.00	1477.0
175.00	18840.0
177.00	1154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	462.0
37.00	1797.0
38.00	1574.0
39.00	886.0
39.90	168.0
43.90	522.0
45.00	273.0
47.00	431.0
48.00	263.0
49.00	1493.0
50.00	6777.0
51.00	2199.0
52.00	104.0
55.90	479.0
57.00	841.0
59.90	320.0
61.00	1469.0
62.00	1708.0
63.00	1397.0
64.00	266.0
65.00	458.0
66.90	100.0
68.00	3383.0
69.00	3413.0
70.00	243.0
71.90	196.0
73.00	1536.0
74.00	5437.0
75.00	16277.0
76.00	1483.0
76.90	211.0
77.90	141.0
78.90	953.0
79.90	245.0
80.90	997.0
81.80	216.0
86.90	1433.0
88.00	1285.0
90.80	152.0
92.00	893.0
93.00	1318.0
94.00	3619.0
95.00	29696.0
96.00	2074.0
103.80	205.0
105.90	132.0
115.80	139.0
116.90	221.0
117.90	146.0
118.90	238.0
140.90	337.0
142.90	422.0
144.90	133.0
171.00	523.0
174.00	21520.0
174.90	1582.0
175.90	21072.0
177.00	1320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	386.0
37.00	1685.0
38.00	1519.0
39.00	800.0
39.90	140.0
43.90	480.0
45.00	221.0
46.90	434.0
48.00	254.0
49.00	1424.0
50.10	6564.0
51.00	2135.0
56.00	463.0
57.00	825.0
59.90	311.0
61.00	1407.0
62.00	1596.0
63.00	1328.0
64.00	251.0
65.00	425.0
68.00	3350.0
69.00	3342.0
69.90	227.0
71.90	158.0
73.00	1517.0
74.00	5321.0
75.00	15646.0
76.00	1484.0
76.90	212.0
77.90	175.0
78.90	1000.0
79.80	242.0
80.90	971.0
81.80	227.0
87.00	1369.0
88.00	1260.0
90.80	143.0
92.00	862.0
93.00	1254.0
94.00	3679.0
95.00	29456.0
96.00	1885.0
103.80	187.0
105.90	143.0
115.80	124.0
116.90	200.0
117.90	140.0
118.90	192.0
129.80	100.0
140.90	330.0
142.90	376.0
144.90	119.0
171.90	551.0
173.00	466.0
174.00	21608.0
175.00	1639.0
175.90	21144.0
177.00	1383.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45