
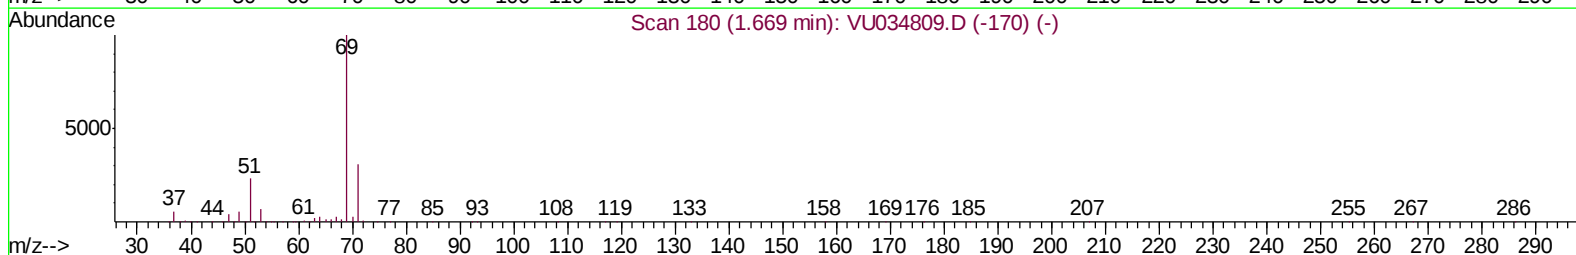
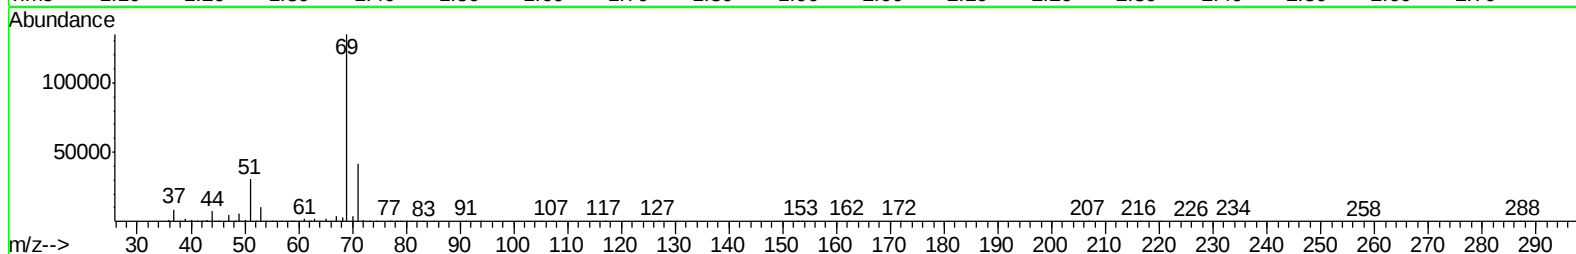


Data File : VU034810.D  
Acq On : 25 Sep 2019 18:23  
Operator : JC/SP  
Sample : VU0925WBL02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Sep 26 06:59:29 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM091919WMA.M  
Quant Title : VOC Analysis  
QLast Update : Thu Sep 26 06:56:48 2019  
Response via : Initial Calibration

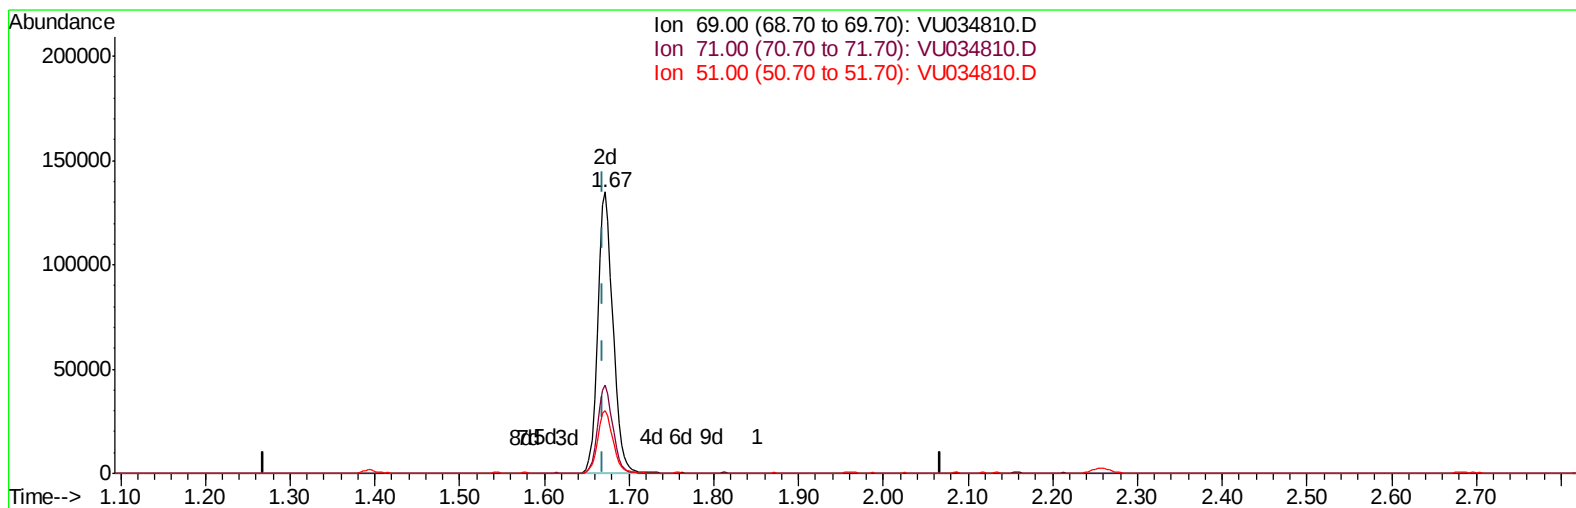

TIC: VU034810.D

(7) Chloroethane-d5 (S)

1.672min (+0.003) 48.41ug/L m

response 168533

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 69.00 | 100   | 100   |
| 71.00 | 31.80 | 0.05# |
| 51.00 | 32.70 | 0.06# |
| 0.00  | 0.00  | 0.00  |