
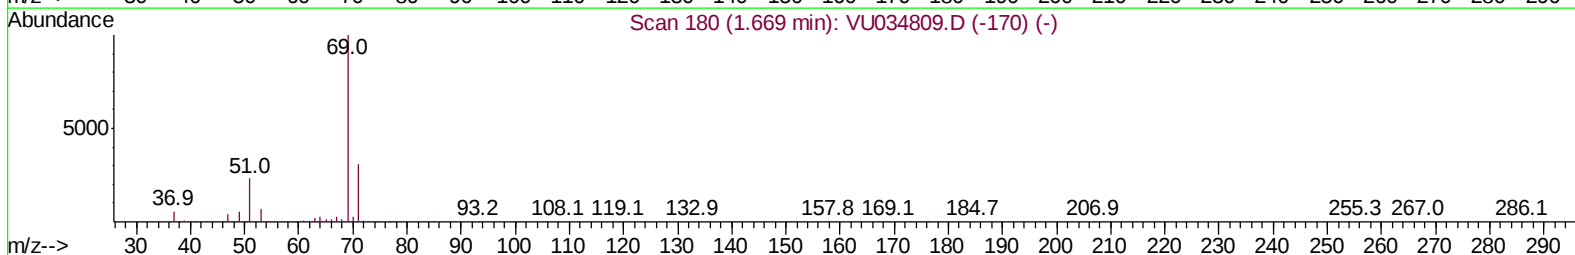
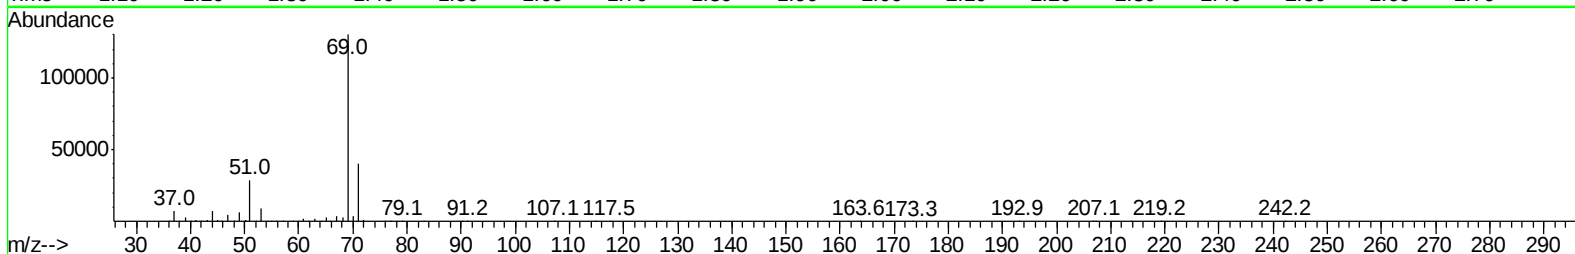


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU092519\
Data File : VU034827.D
Acq On : 26 Sep 2019 01:02
Operator : JC/SP
Sample : K4983-17
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Quant Time: Sep 26 07:03:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM091919WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 06:56:48 2019
Response via : Initial Calibration

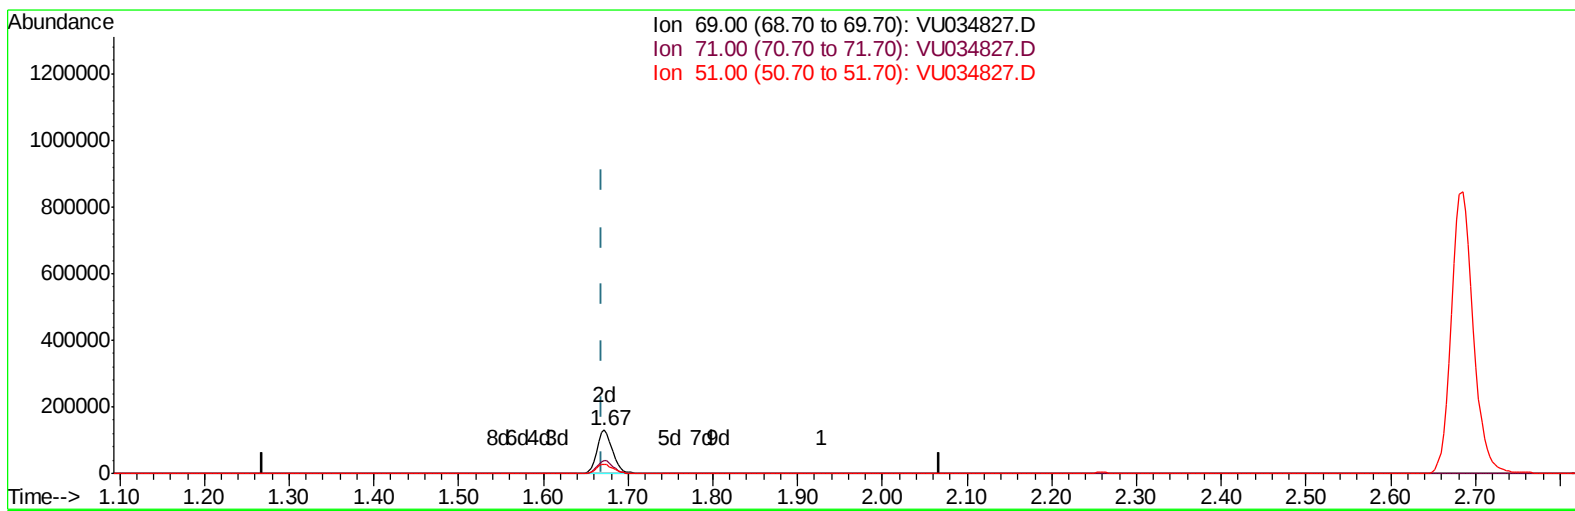

TIC: VU034827.D

(7) Chloroethane-d5 (S)

1.672min (+0.003) 46.38ug/L m

response 164568

Ion	Exp%	Act%
69.00	100	100
71.00	31.80	0.08#
51.00	32.70	0.08#
0.00	0.00	0.00